


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM041520\
 Data File : BM025955.D
 Acq On : 15 Apr 2020 08:04
 Operator : MA/SJ
 Sample : DFTPP98
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP98

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 15 12:24:52 2020

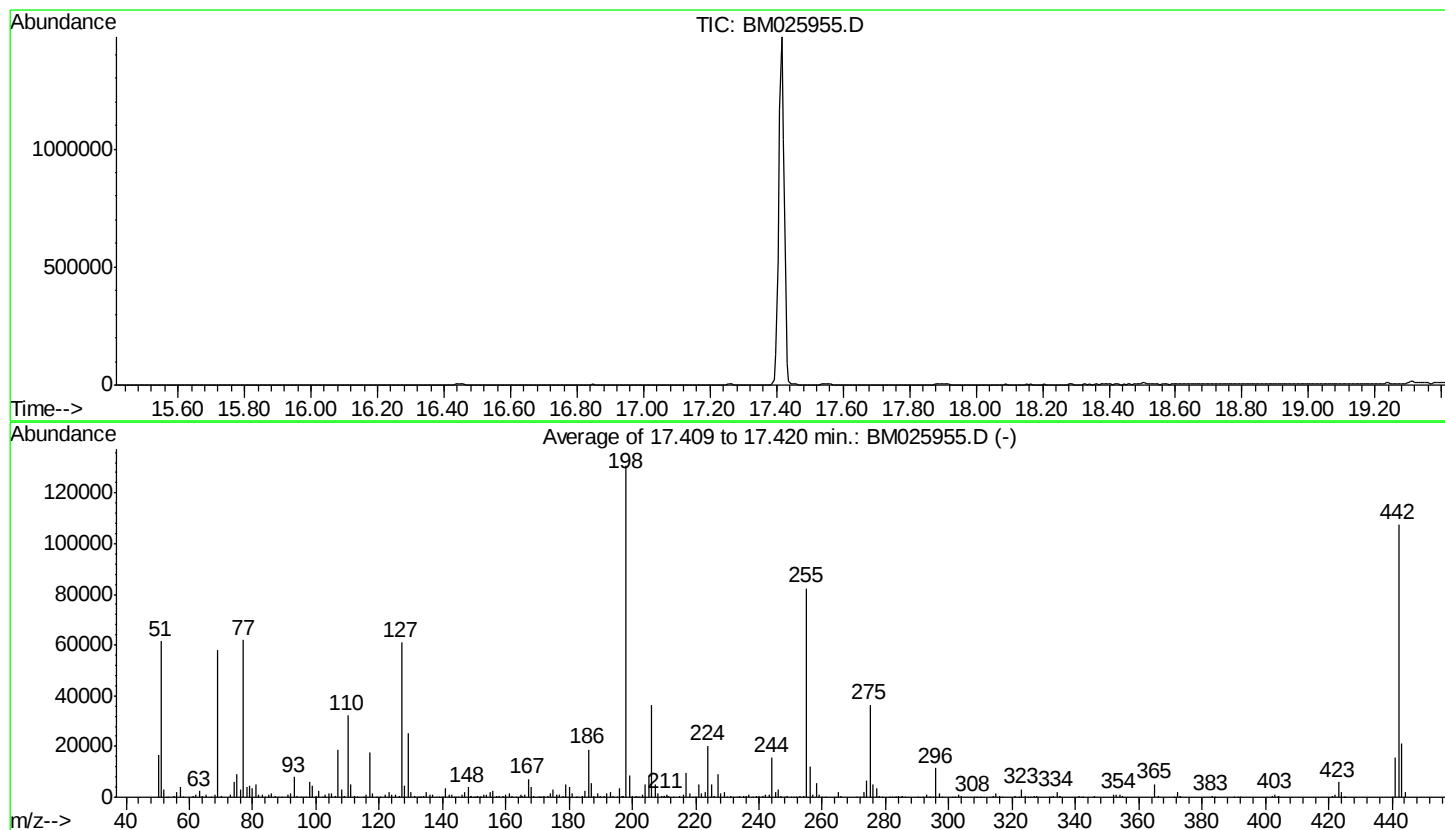

AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.0	61520	PASS
68	69	0.00	2	1.8	1023	PASS
69	198	0.00	100	44.4	58010	PASS
70	69	0.00	2	0.5	316	PASS
127	198	10	80	46.6	60901	PASS
197	198	0.00	2	0.4	537	PASS
198	198	100	100	100.0	130762	PASS
199	198	5	9	6.6	8691	PASS
275	198	10	60	28.0	36589	PASS
365	198	1	100	4.0	5192	PASS
441	198	0.01	100	11.8	15446	PASS
442	198	50	100	82.1	107293	PASS
443	442	15	24	19.7	21185	PASS

Scan 2495 (17.363 min): BM025955.D
DFTPP98

m/z	Abundance
73.00	354.0
84.00	186.0
207.10	430.0
280.90	198.0

Instrument :
BNA_M
ClientSampleId :
DFTPP98

m/z	Abundance
50.10	18960.0
51.10	68352.0
52.10	3393.0
55.00	457.0
56.00	2232.0
57.00	4057.0
58.00	196.0
61.10	933.0
62.10	903.0
63.10	2724.0
64.10	504.0
65.10	1187.0
68.10	1162.0
69.00	63104.0
70.10	392.0
73.10	1410.0
74.10	6093.0
75.10	9902.0
76.10	3338.0
77.10	65720.0
78.10	4591.0
79.00	5006.0
80.00	3493.0
81.00	5364.0
82.00	1545.0
82.90	1078.0
84.00	234.0
85.00	883.0
86.00	1697.0
87.10	736.0
88.10	264.0
91.00	1527.0
92.00	1605.0
93.00	8398.0
94.00	459.0
95.00	183.0
96.10	270.0
98.00	6199.0
99.00	5311.0
100.00	363.0
101.00	2417.0
103.00	998.0
104.00	1691.0
105.00	1709.0
106.00	478.0
107.10	19248.0
108.00	3190.0
108.90	617.0
110.00	32696.0
111.00	5111.0
112.00	902.0
112.90	202.0
116.00	991.0
117.00	18080.0
118.00	1533.0
118.90	280.0
122.00	1046.0
123.10	2035.0
124.10	975.0
125.10	836.0
126.20	284.0
127.00	61320.0
128.10	4334.0
129.00	26112.0
130.00	2032.0
131.00	332.0
132.90	217.0
134.00	591.0
135.00	2170.0
136.10	691.0
137.00	1055.0
138.00	251.0
139.80	258.0
141.00	3375.0
142.10	884.0
142.90	696.0
143.90	286.0
144.90	226.0
146.10	1074.0
147.00	1825.0
148.00	3556.0
148.90	1075.0
149.90	331.0
151.00	443.0
151.80	183.0
153.00	1049.0
153.90	815.0
155.00	1844.0
156.00	2691.0
157.00	478.0
158.00	523.0
159.10	580.0

Instrument :
BNA_M
ClientSampleId :
DFTPP98

160.00	1121.0
161.00	1803.0
162.00	420.0
163.00	177.0
164.10	204.0
164.90	1550.0
166.10	1239.0
167.00	7015.0
168.00	4109.0
168.90	753.0
170.30	303.0
171.10	239.0
172.00	497.0
173.10	689.0
174.10	1337.0
175.00	2984.0
176.10	921.0
177.00	1097.0
177.90	518.0
179.00	5210.0
180.00	3852.0
181.00	1520.0
181.90	291.0
184.00	323.0
185.00	2216.0
186.00	17576.0
187.00	5675.0
188.00	729.0
189.00	1440.0
189.90	243.0
191.00	663.0
192.10	2044.0
192.90	1936.0
193.90	405.0
195.10	164.0
196.00	3146.0
196.80	871.0
198.00	123432.0
199.00	8524.0
199.90	688.0
201.40	660.0
203.10	844.0
204.00	4561.0
205.10	8298.0
206.00	33976.0
207.10	5806.0
208.00	1526.0
209.10	671.0
210.00	609.0
211.00	1227.0
214.90	387.0
216.10	930.0
217.00	8970.0
217.90	1301.0
220.30	234.0
221.10	4433.0
222.00	1388.0
223.00	2186.0
224.00	19992.0
225.00	4509.0
226.00	613.0
227.00	8477.0
228.00	1295.0
229.00	1662.0
230.00	187.0
231.00	593.0
233.90	427.0
235.00	721.0
236.00	499.0
237.00	1123.0
238.90	215.0
239.90	231.0
241.00	564.0
242.00	778.0
243.00	945.0
244.00	14605.0
245.00	1921.0
246.00	3049.0
247.00	628.0
247.90	208.0
249.00	528.0
253.00	353.0
254.20	525.0
255.00	74976.0
256.00	11172.0
257.00	1142.0
258.00	4723.0
259.00	624.0
259.90	227.0
261.10	157.0
265.00	1836.0
265.90	331.0
270.80	161.0
272.00	201.0
273.00	2123.0
274.00	6188.0

Instrument :
BNA_M
ClientSampleId :
DFTPP98

275.00	32512.0
276.00	4812.0
277.00	3227.0
278.00	614.0
279.10	172.0
280.90	346.0
282.90	389.0
284.00	222.0
285.20	571.0
292.00	214.0
293.00	874.0
293.80	208.0
295.00	151.0
296.00	10579.0
296.90	1349.0
303.00	898.0
303.90	163.0
310.10	160.0
314.10	369.0
315.00	1258.0
316.10	656.0
321.00	209.0
323.00	2726.0
324.10	609.0
327.00	536.0
327.90	273.0
331.80	295.0
333.00	509.0
334.10	1818.0
334.90	541.0
340.90	547.0
346.00	544.0
352.00	793.0
353.00	622.0
354.00	1064.0
355.00	405.0
365.00	4114.0
366.10	395.0
371.00	186.0
372.10	1639.0
372.90	384.0
383.00	618.0
390.00	202.0
392.00	172.0
402.10	591.0
403.00	738.0
403.90	322.0
421.00	632.0
422.10	653.0
423.10	4362.0
424.00	1660.0
424.90	374.0
441.10	11818.0
442.10	75552.0
443.10	15197.0
444.10	1542.0

Instrument :
BNA_M
ClientSampleId :
DFTPP98

m/z	Abundance
50.10	19408.0
51.10	71896.0
52.10	3905.0
53.00	243.0
55.10	358.0
56.00	1922.0
57.10	4688.0
58.00	178.0
61.00	893.0
62.10	972.0
63.10	2602.0
64.10	464.0
65.10	1564.0
67.00	158.0
68.10	1132.0
69.00	68904.0
70.00	316.0
73.10	1207.0
74.10	8091.0
75.10	11217.0
76.10	3586.0
77.10	75040.0
78.10	4961.0
79.00	5525.0
80.00	3831.0
81.00	6386.0
82.00	1229.0
83.00	1084.0
84.00	194.0
85.00	959.0
86.10	1854.0
87.10	802.0
87.90	310.0
91.10	1255.0
92.00	1379.0
93.00	9672.0
94.00	696.0
96.00	345.0
96.90	196.0
98.00	7207.0
99.00	5346.0
100.00	655.0
101.00	2931.0
102.00	231.0
103.00	1174.0
104.00	2010.0
105.00	2025.0
106.00	581.0
107.00	22344.0
108.00	3133.0
109.00	654.0
110.00	38992.0
111.00	6493.0
112.00	743.0
112.90	324.0
116.00	1381.0
117.00	21464.0
118.00	1656.0
118.90	203.0
120.10	214.0
122.00	1692.0
123.00	2102.0
124.00	1142.0
125.00	1221.0
126.20	387.0
127.00	73176.0
128.00	6267.0
129.00	30768.0
130.00	2666.0
131.10	604.0
131.90	201.0
132.20	198.0
133.10	185.0
134.00	819.0
135.00	2583.0
136.00	1023.0
137.00	1303.0
137.90	192.0
140.00	315.0
141.00	3771.0
142.00	1540.0
143.00	1117.0
143.90	249.0
145.00	220.0
146.10	875.0
147.00	2363.0
148.00	4941.0
149.10	1064.0
150.10	288.0
151.20	624.0
152.00	396.0
152.90	1290.0

Instrument :
BNA_M
ClientSampleId :
DFTPP98

154.00	1037.0
155.00	2032.0
156.00	3363.0
157.10	467.0
158.00	893.0
159.00	533.0
160.00	1207.0
161.10	1673.0
162.00	560.0
164.10	209.0
165.10	1793.0
165.90	1222.0
167.00	8545.0
168.00	4651.0
169.00	566.0
170.00	407.0
170.80	455.0
172.00	960.0
173.00	818.0
174.00	1673.0
175.00	3348.0
176.00	1042.0
177.00	1571.0
178.00	606.0
179.00	6243.0
180.00	4791.0
181.00	2195.0
181.90	175.0
182.80	210.0
184.10	485.0
184.90	3011.0
186.00	23048.0
187.00	6547.0
188.00	906.0
189.10	1743.0
190.00	329.0
190.90	636.0
192.00	1899.0
193.00	2513.0
194.00	369.0
194.90	330.0
196.00	4865.0
197.10	1134.0
198.00	156224.0
199.00	10852.0
200.00	869.0
201.30	591.0
202.00	213.0
203.10	1230.0
204.00	6437.0
205.00	10097.0
206.10	43568.0
207.10	5969.0
208.00	1685.0
209.10	441.0
209.90	618.0
210.20	526.0
210.80	1475.0
211.80	416.0
214.90	523.0
216.00	973.0
217.00	11599.0
218.00	1748.0
218.80	171.0
220.10	296.0
221.00	6997.0
221.90	1944.0
222.90	2156.0
224.00	23848.0
225.00	6356.0
226.00	848.0
227.00	11327.0
228.00	1564.0
229.00	2489.0
229.80	243.0
231.00	891.0
231.80	202.0
233.00	192.0
234.00	805.0
235.00	820.0
236.00	536.0
237.00	1084.0
237.90	214.0
239.00	804.0
240.00	486.0
241.00	680.0
242.00	1373.0
243.10	1400.0
244.10	18824.0
245.10	2145.0
245.90	4013.0
246.90	885.0
248.00	222.0
249.00	602.0
250.00	163.0
250.80	167.0

Instrument :
BNA_M
ClientSampleId :
DFTPP98

251.80	162.0
252.90	367.0
254.00	746.0
255.00	98384.0
256.10	14411.0
257.10	1378.0
258.00	6797.0
259.00	1068.0
260.00	201.0
261.00	173.0
264.00	155.0
265.10	2565.0
266.00	563.0
270.90	368.0
272.00	215.0
273.00	2481.0
274.00	7338.0
275.00	43440.0
276.00	6094.0
277.00	4463.0
278.00	751.0
278.90	227.0
281.10	386.0
282.00	270.0
282.90	396.0
284.00	471.0
284.90	787.0
286.00	239.0
290.20	155.0
291.90	227.0
293.00	1240.0
293.80	208.0
295.00	235.0
296.00	13992.0
297.00	1751.0
297.90	219.0
301.00	189.0
301.90	320.0
303.00	1553.0
304.00	385.0
307.90	205.0
308.90	150.0
313.90	531.0
315.00	1514.0
316.00	621.0
316.90	267.0
321.00	620.0
322.00	282.0
323.10	3814.0
324.10	739.0
325.90	167.0
327.00	761.0
327.90	374.0
332.00	338.0
332.90	539.0
334.00	2542.0
335.10	594.0
341.00	478.0
341.90	157.0
342.20	239.0
346.00	898.0
352.10	1202.0
353.00	1179.0
354.10	1376.0
355.10	527.0
365.00	6274.0
366.00	1032.0
371.00	401.0
372.00	2252.0
373.00	652.0
383.10	588.0
384.00	188.0
390.00	183.0
391.10	222.0
392.10	173.0
402.00	869.0
403.10	1330.0
404.10	539.0
421.00	975.0
422.10	957.0
423.00	7201.0
424.10	2161.0
424.90	382.0
440.00	231.0
441.00	18280.0
442.10	129752.0
443.10	25488.0
444.10	2337.0

Instrument :
BNA_M
ClientSampleId :
DFTPP98

m/z	Abundance
50.10	11381.0
51.10	44312.0
52.10	2059.0
55.10	287.0
56.00	1330.0
57.00	3274.0
61.10	429.0
62.00	645.0
63.10	1600.0
64.10	322.0
65.10	761.0
68.00	775.0
69.00	42024.0
70.00	240.0
73.10	796.0
74.00	4347.0
75.10	6726.0
76.10	2128.0
77.10	45152.0
78.10	2965.0
79.00	3440.0
80.00	2596.0
81.00	3333.0
82.00	803.0
83.00	741.0
83.90	220.0
85.10	774.0
86.00	945.0
86.90	458.0
87.90	158.0
89.00	172.0
91.00	822.0
92.00	943.0
93.00	5652.0
93.90	590.0
97.00	177.0
98.00	4364.0
99.00	3328.0
100.00	263.0
101.00	1554.0
103.00	580.0
104.00	1351.0
105.00	1312.0
106.10	578.0
107.00	14389.0
108.10	2108.0
109.10	417.0
110.00	24768.0
111.00	3652.0
112.00	547.0
113.10	152.0
115.20	192.0
116.10	710.0
117.00	13776.0
118.00	1094.0
120.10	209.0
122.10	1096.0
123.00	1679.0
124.00	664.0
124.90	457.0
126.20	453.0
127.00	48208.0
128.10	3489.0
129.00	19600.0
130.00	1715.0
131.00	371.0
131.80	155.0
134.00	535.0
135.00	1676.0
136.00	628.0
137.00	855.0
137.90	250.0
139.00	186.0
140.10	303.0
141.00	3005.0
142.00	1147.0
142.90	747.0
144.10	165.0
146.00	597.0
147.00	2142.0
148.00	3248.0
149.00	717.0
150.10	155.0
150.90	435.0
152.20	277.0
152.90	901.0
154.00	994.0
155.00	1721.0
156.00	1909.0
156.90	431.0
157.90	587.0
158.90	358.0

Instrument :
BNA_M
ClientSampleId :
DFTPP98

160.10	861.0
161.00	1529.0
162.10	248.0
163.10	202.0
164.20	290.0
164.90	1104.0
166.00	921.0
167.00	5808.0
168.00	2919.0
168.90	503.0
170.20	239.0
171.10	301.0
172.00	384.0
173.00	740.0
174.00	1293.0
175.00	2300.0
176.00	551.0
177.00	1142.0
178.10	539.0
179.00	4494.0
180.00	3215.0
181.00	1355.0
182.00	343.0
182.70	153.0
183.90	526.0
185.00	2185.0
186.00	16181.0
187.00	4462.0
188.00	491.0
189.10	1074.0
189.90	317.0
190.90	555.0
192.00	1272.0
193.00	1629.0
194.10	370.0
196.00	3384.0
196.80	491.0
197.10	477.0
198.00	112632.0
199.00	6698.0
200.00	615.0
201.30	345.0
201.60	385.0
202.90	809.0
204.00	4641.0
205.10	7464.0
206.00	32096.0
207.10	4857.0
208.00	1183.0
208.90	444.0
210.20	491.0
210.80	980.0
211.20	921.0
213.00	207.0
215.00	342.0
215.90	621.0
217.00	8828.0
218.00	939.0
219.90	208.0
221.00	4501.0
221.80	964.0
222.10	981.0
223.00	1947.0
224.00	17112.0
225.00	4791.0
225.90	406.0
227.00	8156.0
228.00	1209.0
228.90	1846.0
229.90	231.0
231.10	551.0
233.90	462.0
234.90	496.0
235.90	433.0
236.90	801.0
239.00	428.0
239.90	193.0
241.00	490.0
242.00	1041.0
243.10	1032.0
244.00	13176.0
245.00	1850.0
246.00	2642.0
247.10	588.0
248.00	292.0
248.90	414.0
250.10	176.0
250.90	181.0
253.00	451.0
254.20	659.0
255.00	73760.0
256.00	10796.0
257.00	1060.0
258.00	4622.0
259.10	637.0
265.00	1707.0

Instrument :
BNA_M
ClientSampleId :
DFTPP98

266.10	271.0
272.10	226.0
273.00	2092.0
274.00	5692.0
275.00	33816.0
276.10	4531.0
277.00	3105.0
278.00	476.0
279.00	178.0
282.00	350.0
283.10	408.0
284.10	267.0
285.10	617.0
293.00	864.0
294.00	233.0
294.90	190.0
296.00	10276.0
297.00	1392.0
297.90	154.0
302.00	209.0
303.00	1080.0
304.00	361.0
314.00	519.0
315.00	1250.0
316.00	525.0
321.00	434.0
322.00	229.0
323.00	3195.0
324.00	834.0
325.00	166.0
326.90	730.0
328.00	312.0
332.10	197.0
332.90	329.0
334.10	1745.0
335.00	364.0
341.00	335.0
345.90	731.0
352.00	1091.0
353.00	603.0
354.10	1044.0
355.10	386.0
365.00	5190.0
366.00	871.0
372.10	1681.0
373.20	454.0
382.90	482.0
390.00	217.0
401.90	757.0
403.00	1036.0
404.10	331.0
421.00	694.0
422.10	781.0
423.00	6176.0
424.10	1818.0
425.10	258.0
441.10	16242.0
442.10	116576.0
443.00	22872.0
444.10	2170.0

Instrument :
BNA_M
ClientSampleId :
DFTPP98