

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM041521\
 Data File : BM029508.D
 Acq On : 15 Apr 2021 18:04
 Operator : CG/JU
 Sample : M1959-03
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B43

Quant Time: Apr 16 04:39:45 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM040721MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 14 17:30:14 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	115813	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	477057	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.32	164	287893	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.06	188	561967	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	465362	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	411483	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL
5) Phenol-d5	0.00	99	0	0.00	ng/ul
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0d	0.00	ng/ul
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul
44) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul
47) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul
58) Fluorene-d10	0.00	176	0	0.00	ng/ul
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul
71) Anthracene-d10	0.00	188	0d	0.00	ng/ul
79) Pyrene-d10	0.00	212	0	0.00	ng/ul
90) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul


Target Compounds				Ovalue
77) Fluoranthene	19.11	202	42875	1.171 ng/ul# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM041521\
Data File : BM029508.D
Acq On : 15 Apr 2021 18:04
Operator : CG/JU
Sample : M1959-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B43

Quant Time: Apr 16 04:39:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM040721MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 14 17:30:14 2021
Response via : Initial Calibration

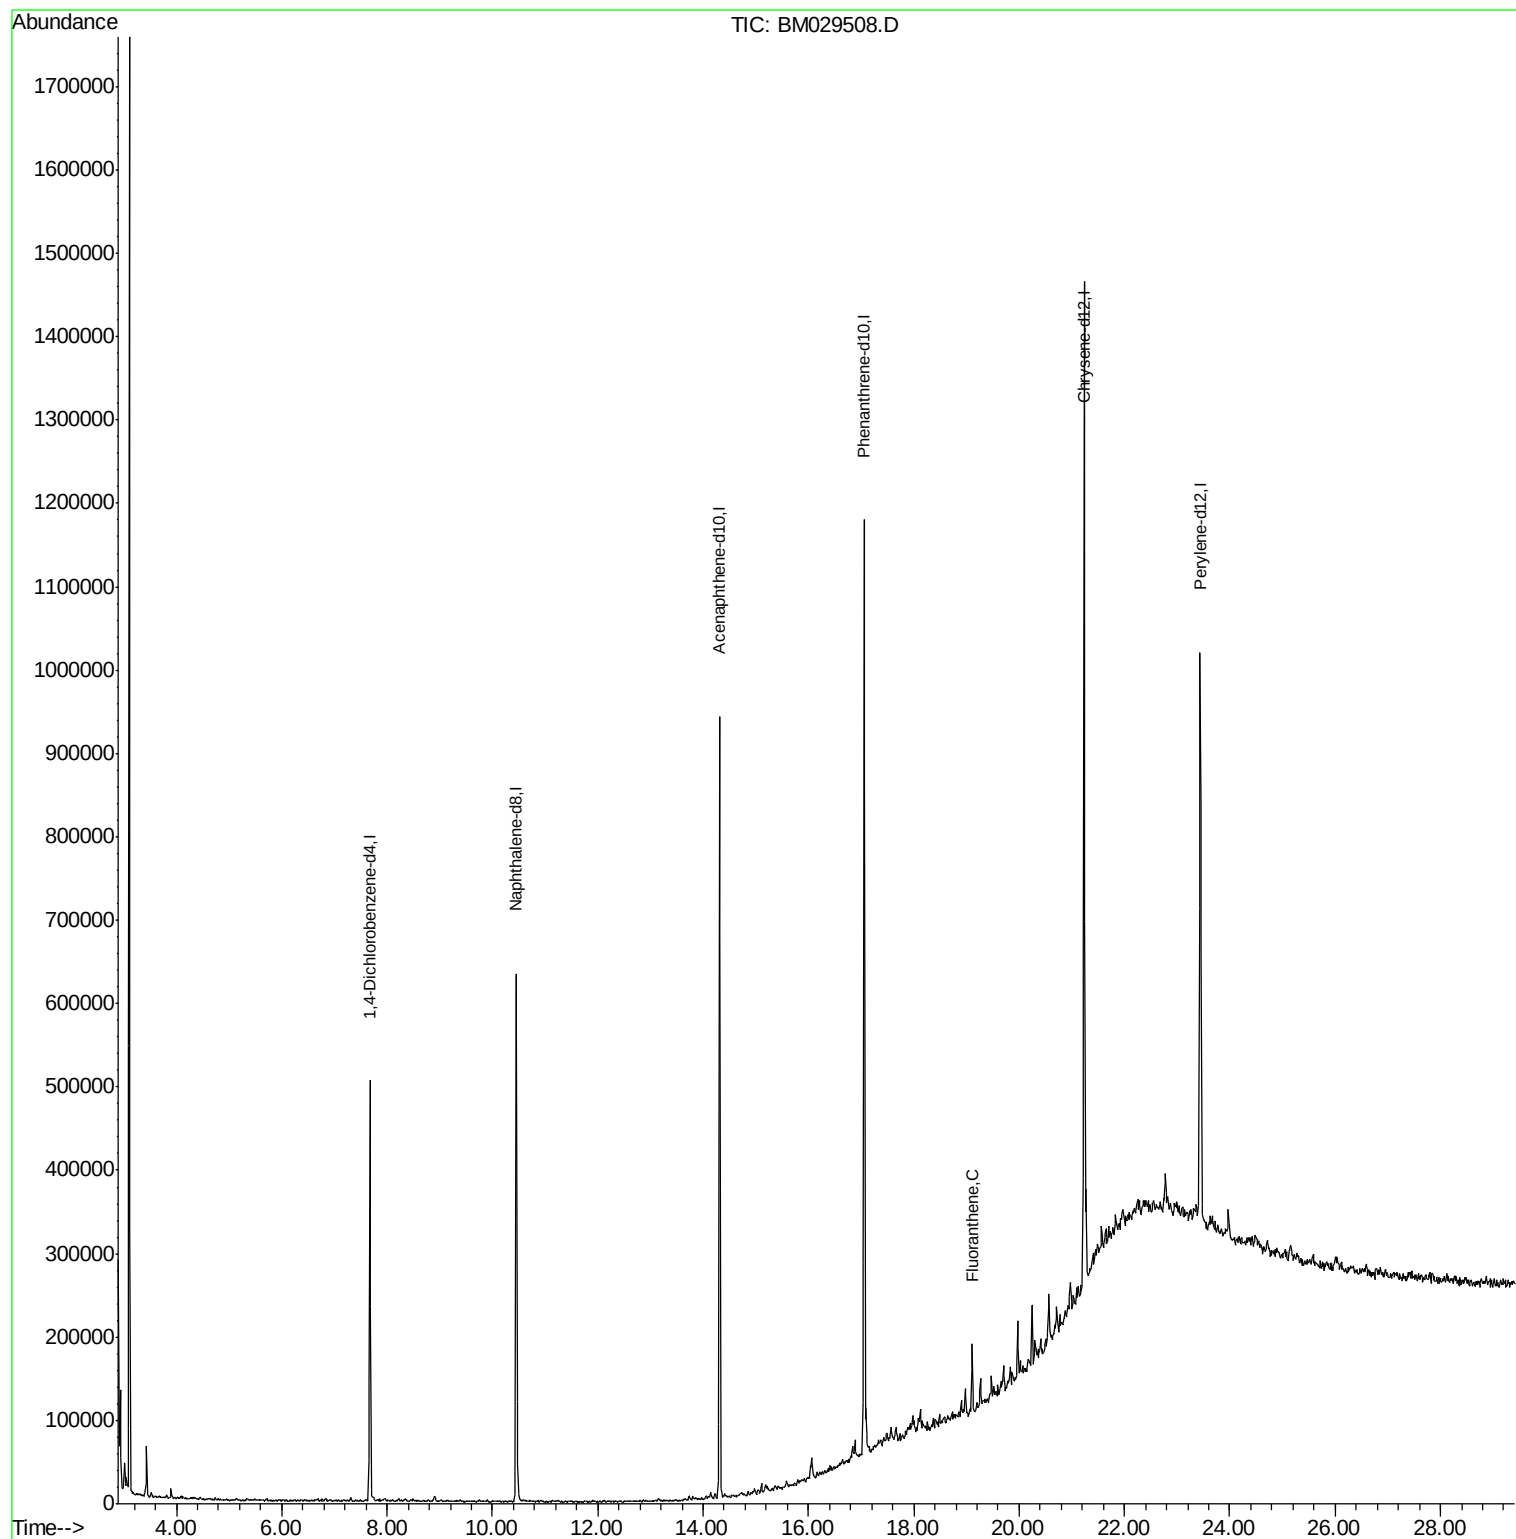

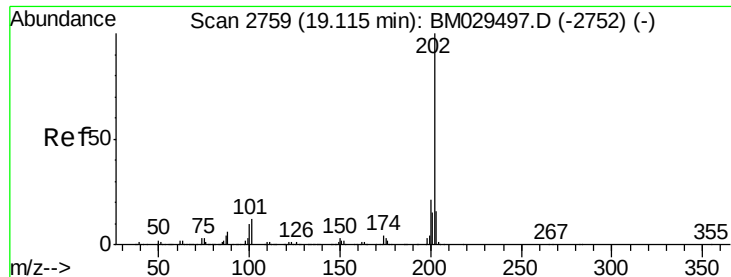

#77
 Fluoranthene
 Concen: 1.171 ng/ul
 RT: 19.11 min Scan# 2758
 Delta R.T. -0.01 min
 Lab File: BM029508.D
 Acq: 15 Apr 2021 18:04

Instrument :
 BNA_M
 ClientSampleId :
 C0B43

Tot Ion	Ratio	Lower	Upper
202	100		
101	14.8	9.8	14.6
100	10.5	7.4	11.0

