

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM041521\
 Data File : BM029468.D
 Acq On : 14 Apr 2021 17:00
 Operator : CG/JU
 Sample : M2002-05
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM040721MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.922	3	6	13	rVB	33852	47552	4.79%	0.911%
2	3.905	170	173	178	rVB4	6055	8833	0.89%	0.169%
3	4.446	263	265	266	rVB2	2333	1175	0.12%	0.023%
4	4.516	275	277	279	rBV4	1742	1421	0.14%	0.027%
5	4.852	332	334	336	rBV3	1652	1047	0.11%	0.020%
6	5.663	469	472	473	rVB3	1330	1269	0.13%	0.024%
7	5.681	473	475	476	rBV2	1548	1290	0.13%	0.025%
8	6.146	551	554	555	rBV3	1091	1128	0.11%	0.022%
9	6.246	569	571	574	rBV3	1045	1013	0.10%	0.019%
10	7.057	706	709	710	rVB3	1740	1156	0.12%	0.022%
11	7.140	722	723	727	rBV4	1135	1022	0.10%	0.020%
12	7.681	808	815	827	rBV	315896	528479	53.20%	10.130%
13	8.422	937	941	944	rBV4	1446	1803	0.18%	0.035%
14	8.740	992	995	1000	rVB6	968	1676	0.17%	0.032%
15	9.028	1041	1044	1049	rVB5	600	1040	0.10%	0.020%
16	9.540	1128	1131	1136	rBV5	767	1510	0.15%	0.029%
17	9.734	1162	1164	1169	rVB4	740	1259	0.13%	0.024%
18	10.104	1225	1227	1231	rVB5	1420	1994	0.20%	0.038%
19	10.457	1280	1287	1298	rBV	401765	702546	70.73%	13.466%
20	10.528	1298	1299	1305	rVV3	2504	3494	0.35%	0.067%
21	10.593	1307	1310	1316	rVB5	982	1731	0.17%	0.033%
22	10.728	1331	1333	1338	rVB4	1057	1480	0.15%	0.028%
23	11.575	1474	1477	1480	rBV4	756	1069	0.11%	0.020%
24	11.975	1541	1545	1546	rBV2	731	1051	0.11%	0.020%
25	12.387	1613	1615	1618	rBV3	812	1065	0.11%	0.020%
26	12.563	1642	1645	1647	rBV3	1001	1167	0.12%	0.022%
27	13.228	1755	1758	1763	rBV3	1291	2617	0.26%	0.050%
28	13.851	1860	1864	1868	rVB4	1092	1262	0.13%	0.024%
29	14.316	1936	1943	1952	rBV	627009	906371	91.25%	17.373%
30	14.510	1974	1976	1978	rBV2	897	1011	0.10%	0.019%
31	14.704	2007	2009	2015	rVB4	573	1047	0.11%	0.020%
32	15.128	2079	2081	2084	rBV2	1130	1285	0.13%	0.025%
33	15.322	2110	2114	2117	rBV3	856	1163	0.12%	0.022%
34	16.486	2307	2312	2315	rVV4	773	1297	0.13%	0.025%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM041521\
 Data File : BM029468.D
 Acq On : 14 Apr 2021 17:00
 Operator : CG/JU
 Sample : M2002-05
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM040721MA.M
 Title : SVOA CALIBRATION

35	16.569	2324	2326	2329	rVB3	1393	1342	0.14%	0.026%
36	16.763	2355	2359	2362	rBV3	847	1094	0.11%	0.021%
37	16.851	2370	2374	2376	rVB4	2102	2734	0.28%	0.052%
38	17.057	2403	2409	2420	rBV	708786	993323	100.00%	19.040%
39	17.463	2473	2478	2481	rBV4	863	1673	0.17%	0.032%
40	17.610	2500	2503	2505	rBV4	1402	1106	0.11%	0.021%
41	17.745	2523	2526	2528	rBV3	1181	1239	0.12%	0.024%
42	17.774	2528	2531	2533	rVV3	1004	1283	0.13%	0.025%
43	17.886	2547	2550	2551	rBV3	1074	994	0.10%	0.019%
44	18.198	2601	2603	2605	rBV2	1054	1223	0.12%	0.023%
45	18.269	2611	2615	2617	rBV5	1342	1699	0.17%	0.033%
46	18.351	2626	2629	2630	rBV2	1268	1132	0.11%	0.022%
47	18.468	2645	2649	2650	rBV4	879	1382	0.14%	0.026%
48	18.574	2665	2667	2672	rBV5	2206	2553	0.26%	0.049%
49	18.727	2692	2693	2694	rBV	2424	1262	0.13%	0.024%
50	18.845	2709	2713	2714	rBV3	2259	2783	0.28%	0.053%
51	18.880	2717	2719	2721	rBV3	1746	2099	0.21%	0.040%
52	18.945	2728	2730	2733	rBV4	1353	1567	0.16%	0.030%
53	18.974	2733	2735	2736	rBV2	1341	1021	0.10%	0.020%
54	19.504	2823	2825	2827	rBV3	2252	2319	0.23%	0.044%
55	19.845	2881	2883	2885	rBV3	2793	2769	0.28%	0.053%
56	21.233	3114	3119	3126	rBV	780668	982838	98.94%	18.839%
57	23.445	3489	3495	3503	rVB	533133	973341	97.99%	18.657%


Sum of corrected areas: 5217099

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM041521\
Data File : BM029468.D
Acq On : 14 Apr 2021 17:00
Operator : CG/JU
Sample : M2002-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM040721MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

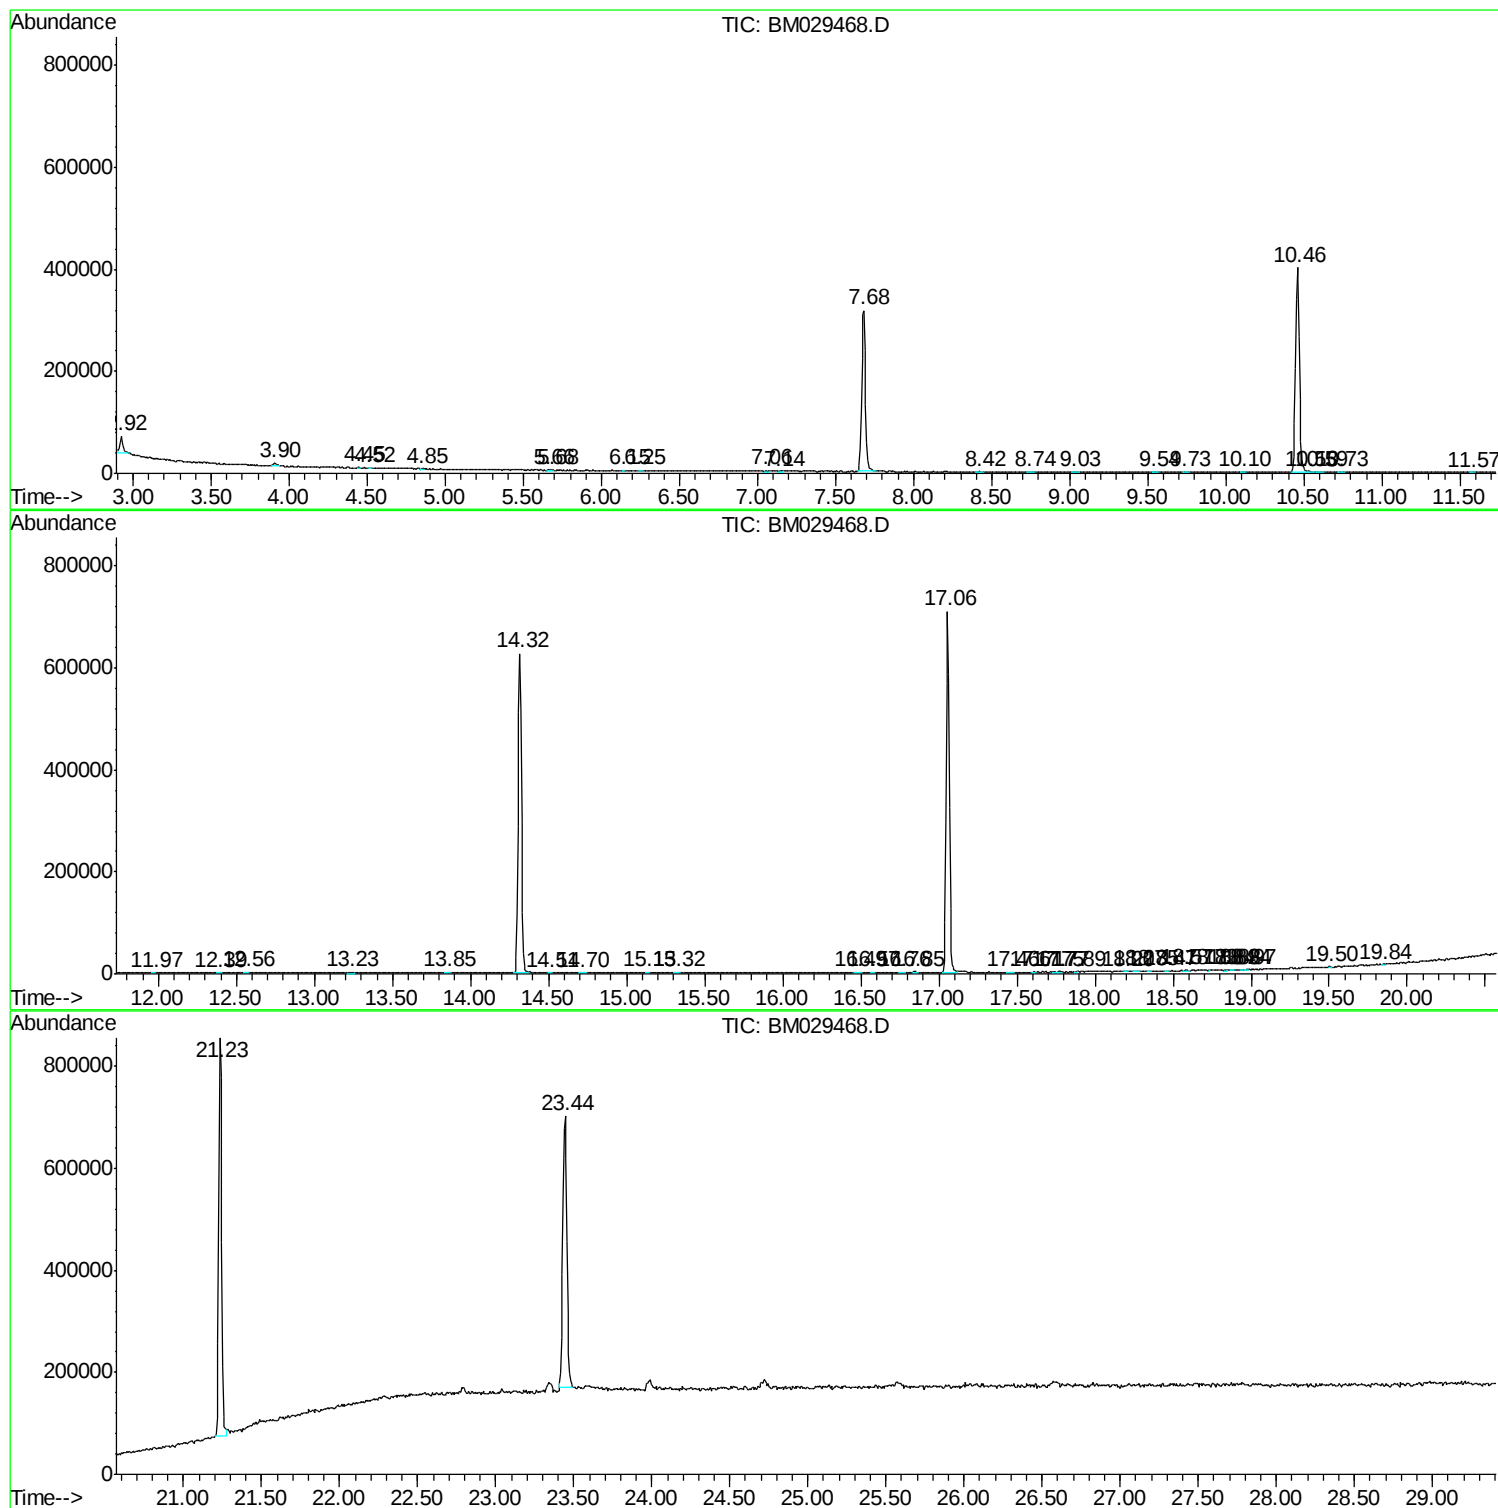

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041521\
Data File : BM029468.D
Acq On : 14 Apr 2021 17:00
Operator : CG/JU
Sample : M2002-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM040721MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041521\
Data File : BM029468.D
Acq On : 14 Apr 2021 17:00
Operator : CG/JU
Sample : M2002-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM040721MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc