
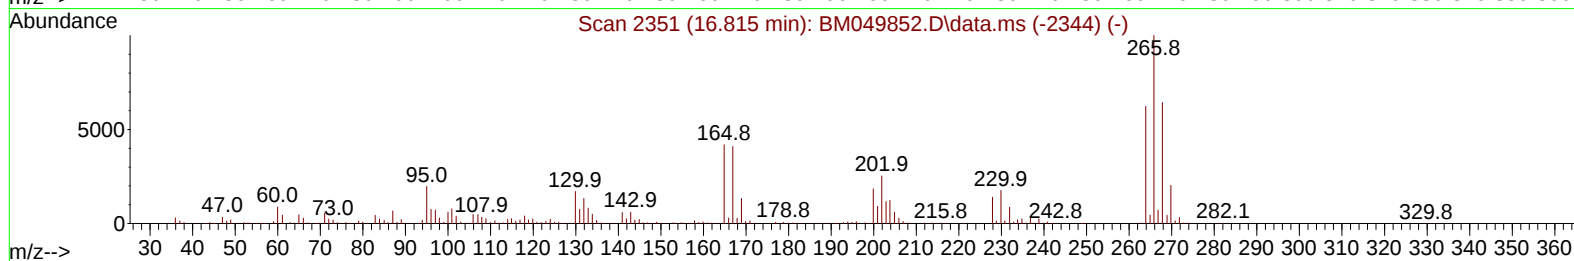
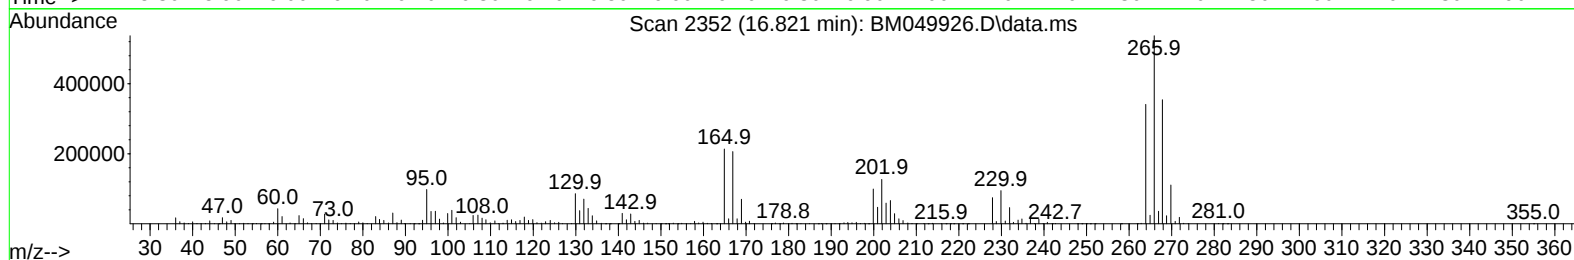


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041525\
Data File : BM049926.D
Acq On : 15 Apr 2025 08:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 11:51:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

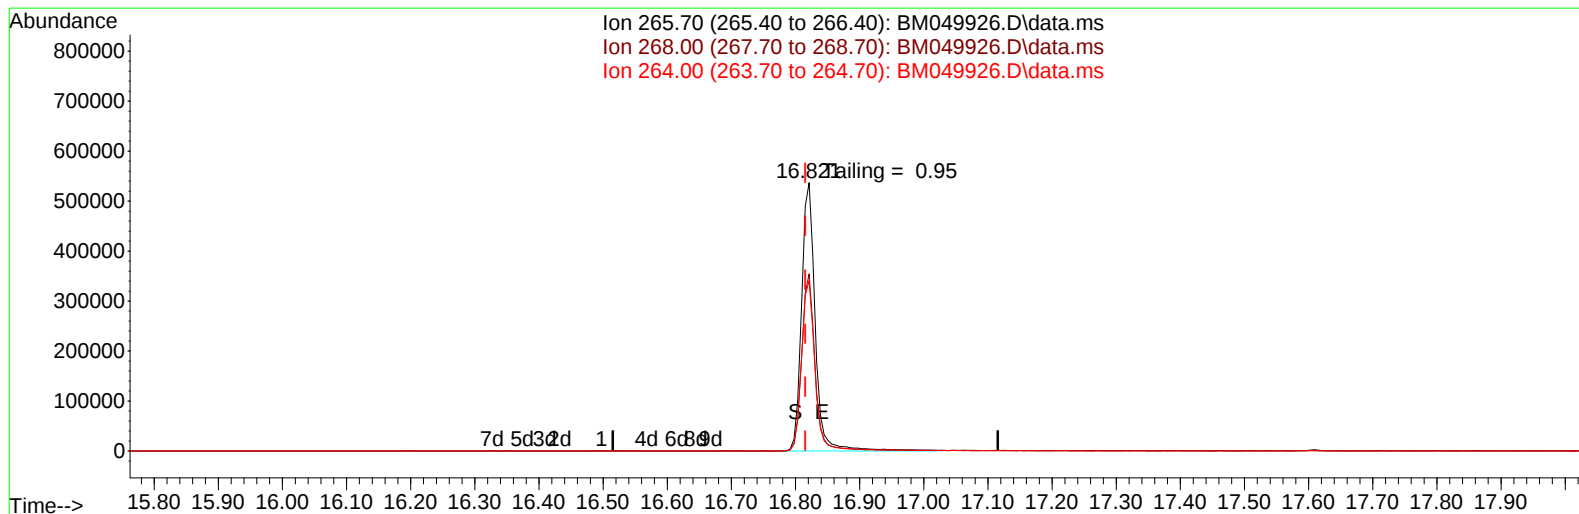

TIC: BM049926.D\data.ms

(70) Pentachlorophenol (C)




16.821min (+ 0.006) 186978.24 ng m

response 802848

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	65.98
264.00	62.30	63.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041525\
Data File : BM049926.D
Acq On : 15 Apr 2025 08:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 11:51:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

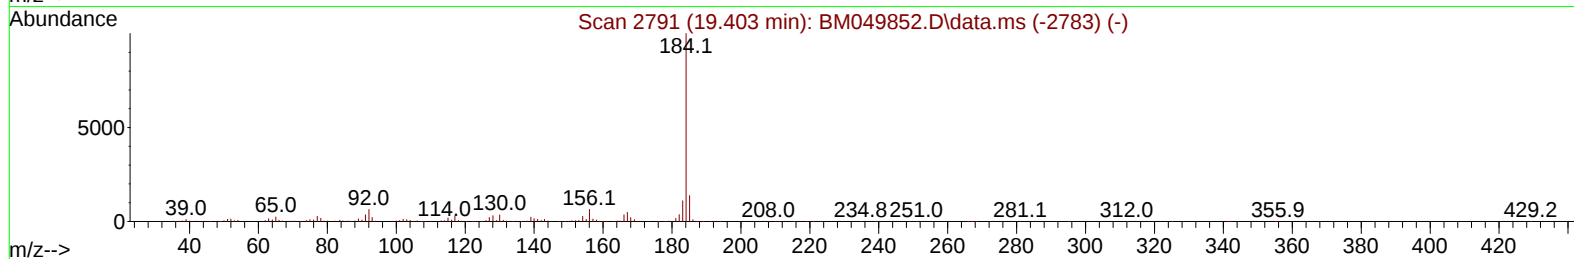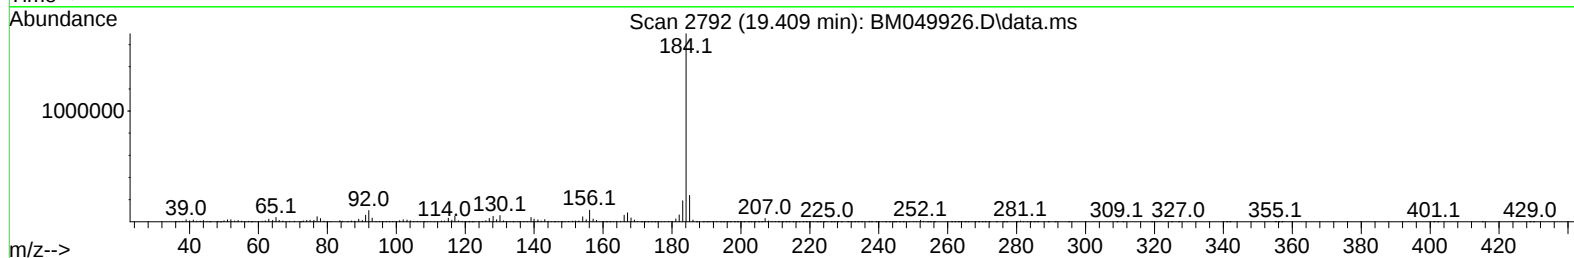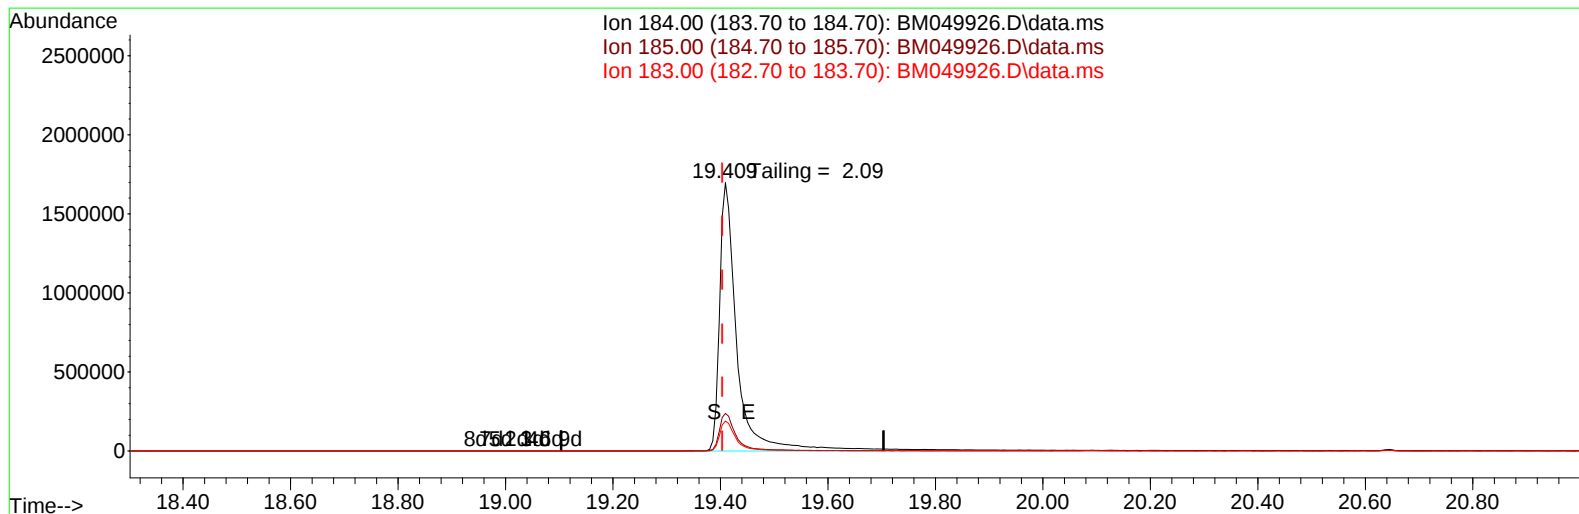

TIC: BM049926.D\data.ms

(77) Benzidine

19.409min (+ 0.006) 889867.19 ng m

response 3942987

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.05
183.00	11.00	11.16
0.00	0.00	0.00