


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041525\
Data File : BM049926.D
Acq On : 15 Apr 2025 08:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 09 04:00:55 2025

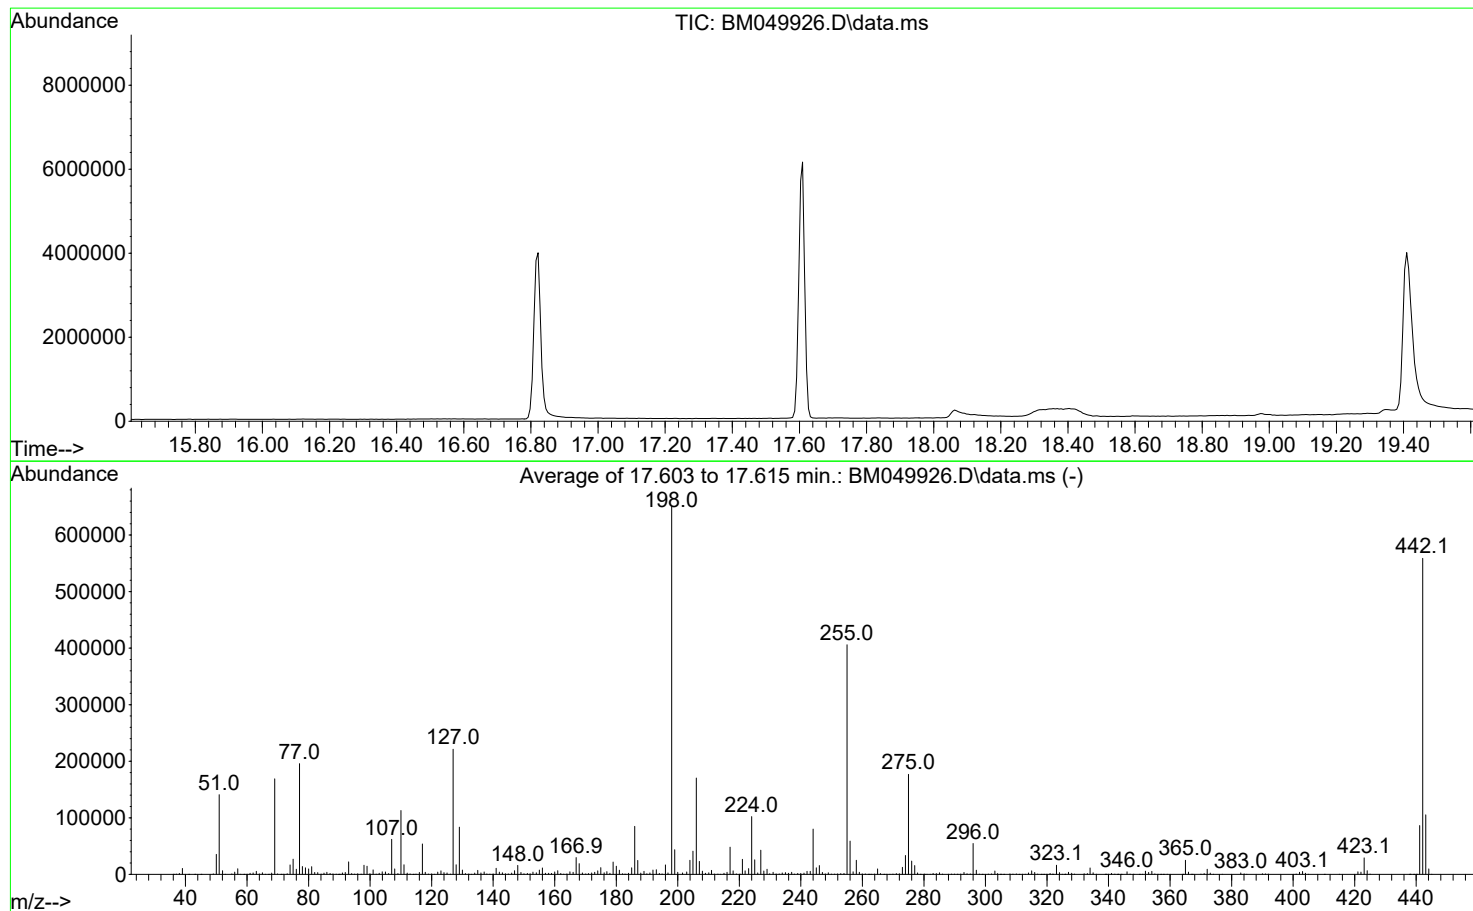

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.7	140879	PASS
68	69	0.00	2	1.3	2252	PASS
69	198	0.00	100	26.0	168883	PASS
70	69	0.00	2	0.6	1014	PASS
127	198	10	80	34.0	221256	PASS
197	198	0.00	2	0.4	2677	PASS
198	198	100	100	100.0	650475	PASS
199	198	5	9	6.7	43643	PASS
275	198	10	60	27.2	176928	PASS
365	198	1	100	3.8	24971	PASS
441	198	0.01	100	13.3	86293	PASS
442	442	50	100	100.0	558869	PASS
443	442	15	24	18.8	105269	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/15/2025	BNA_M	<u>BM049926.D</u>
Compound Name	Response	Retention Time
DDT	2057250	20.644
DDD	47033	20.203
DDE	2263	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
49296	2106546	2.34

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041525\
Data File : BM049926.D
Acq On : 15 Apr 2025 08:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 15 11:51:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

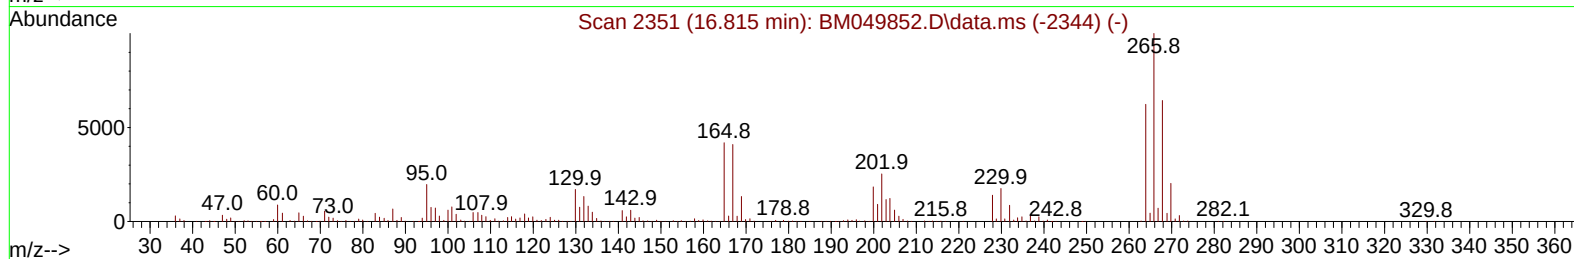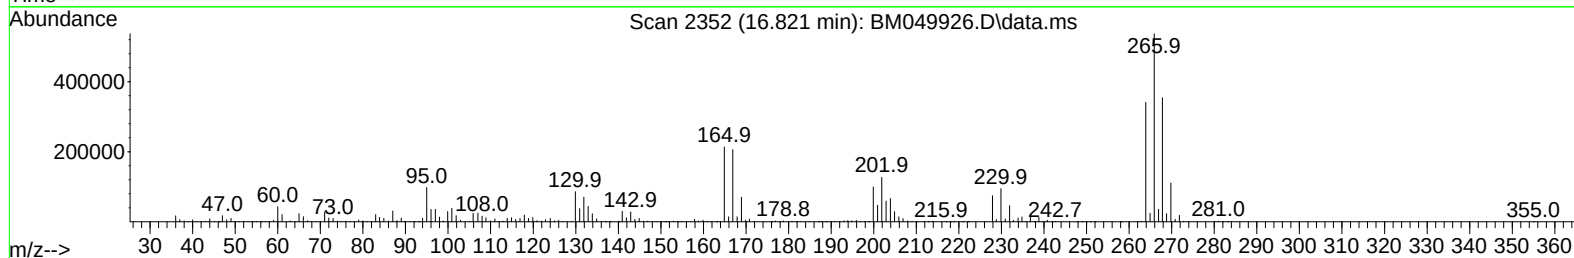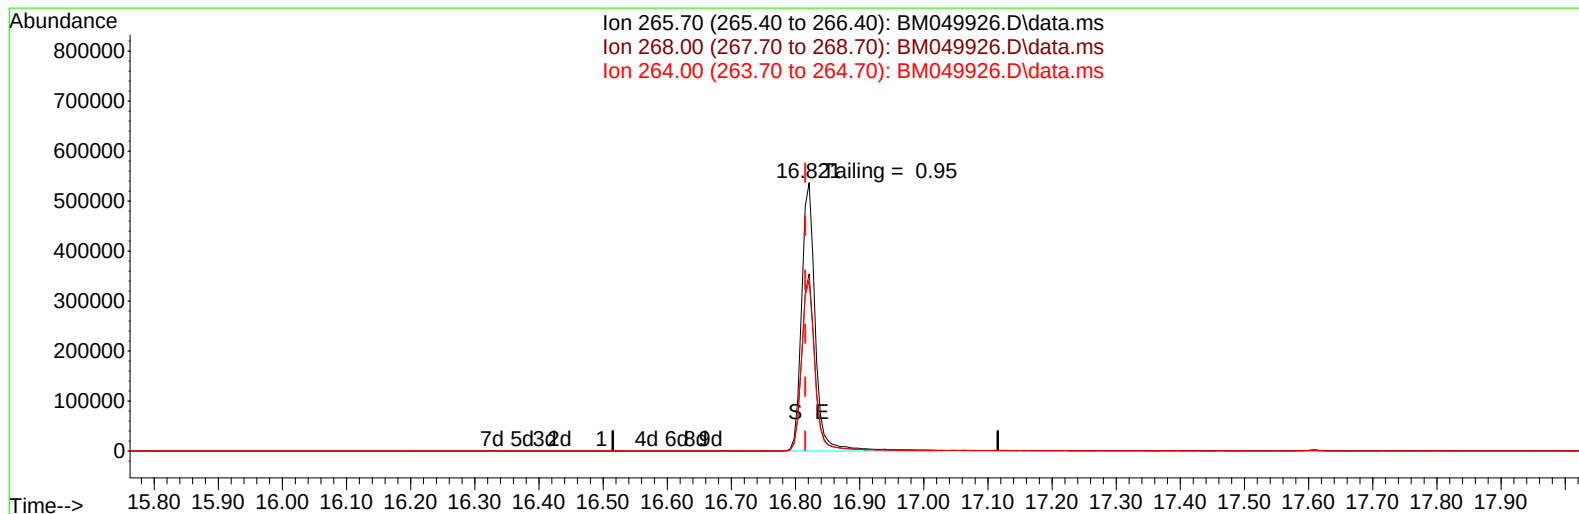

TIC: BM049926.D\data.ms

(70) Pentachlorophenol (C)

16.821min (+ 0.006) 186978.24 ng m




response 802848

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	65.98
264.00	62.30	63.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041525\
Data File : BM049926.D
Acq On : 15 Apr 2025 08:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 15 11:51:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

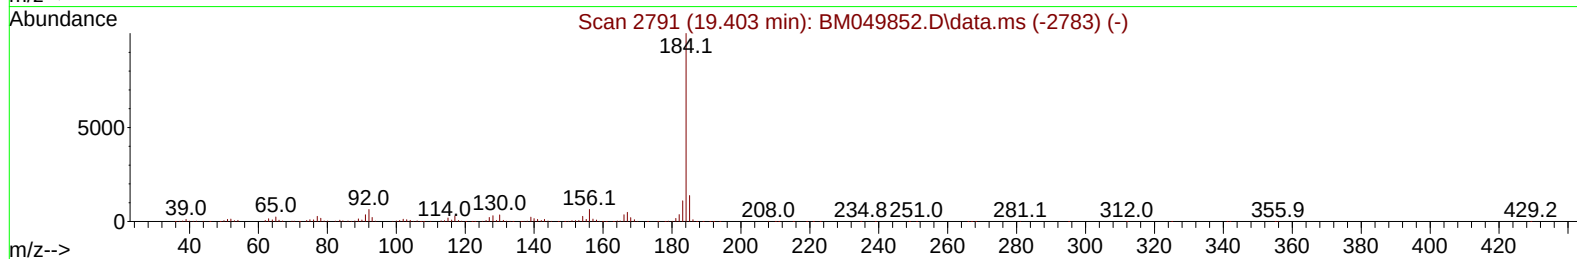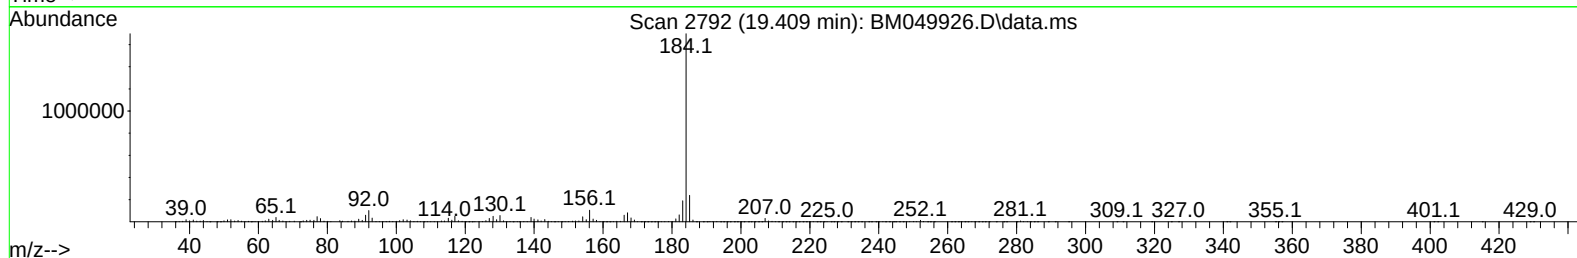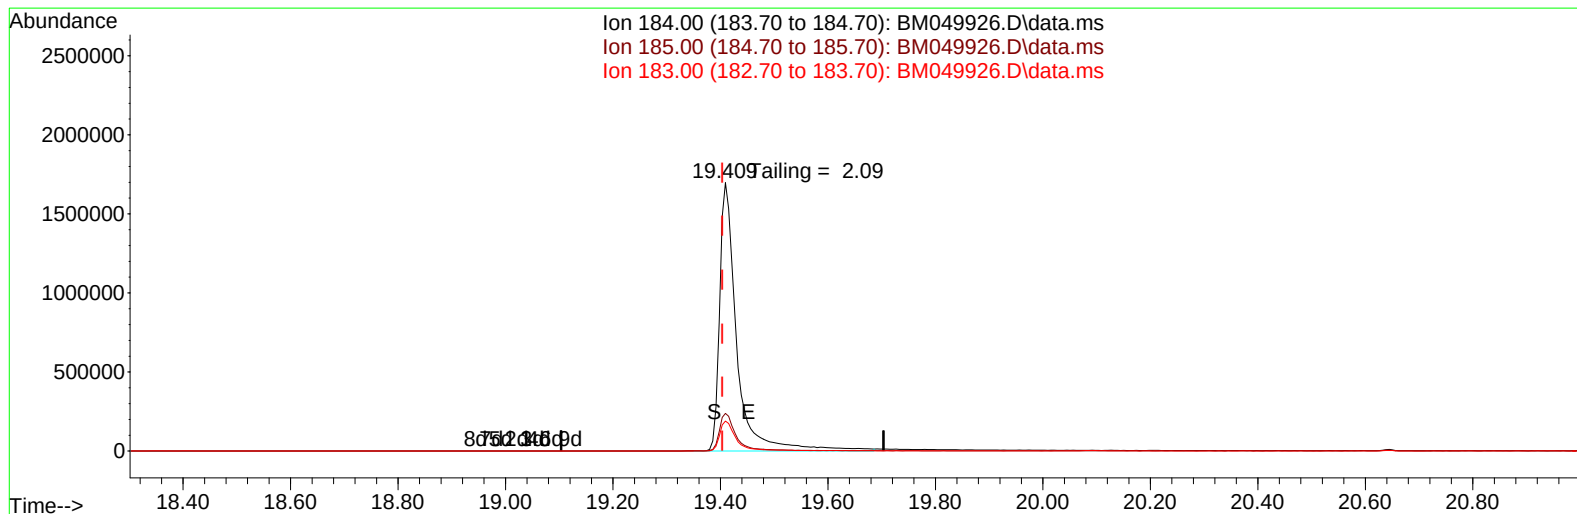

TIC: BM049926.D\data.ms

(77) Benzidine

19.409min (+ 0.006) 889867.19 ng m

response 3942987

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.05
183.00	11.00	11.16
0.00	0.00	0.00