

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041619\
 Data File : BM019928.D
 Acq On : 16 Apr 2019 11:45
 Operator : JU/SJ
 Sample : PB118322BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB118322BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.140	360	366	388	rBV	2598556	3950677	45.84%	8.738%
2	6.722	629	635	657	rBV	2484411	4230449	49.09%	9.357%
3	7.063	687	693	715	rBV	2754397	4427820	51.38%	9.793%
4	7.528	766	772	783	rBV	507576	792722	9.20%	1.753%
5	7.840	818	825	843	rBV	1960736	3097591	35.94%	6.851%
6	8.704	965	972	988	rBV	1207460	2341864	27.17%	5.180%
7	10.310	1238	1245	1269	rBV	456314	1022223	11.86%	2.261%
8	12.804	1662	1669	1684	rBV	3650302	5757219	66.80%	12.733%
9	14.198	1900	1906	1922	rBV2	745725	1380420	16.02%	3.053%
10	15.704	2156	2162	2183	rBV	2879930	4643445	53.88%	10.270%
11	16.962	2370	2376	2397	rBV	876919	1592594	18.48%	3.522%
12	19.609	2820	2826	2840	rBV	6810180	8618057	100.00%	19.061%
13	21.180	3088	3093	3109	rBV	1153445	1792480	20.80%	3.964%
14	23.374	3460	3466	3478	rBV2	721393	1566320	18.17%	3.464%


Sum of corrected areas: 45213881

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041619\
Data File : BM019928.D
Acq On : 16 Apr 2019 11:45
Operator : JU/SJ
Sample : PB118322BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB118322BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

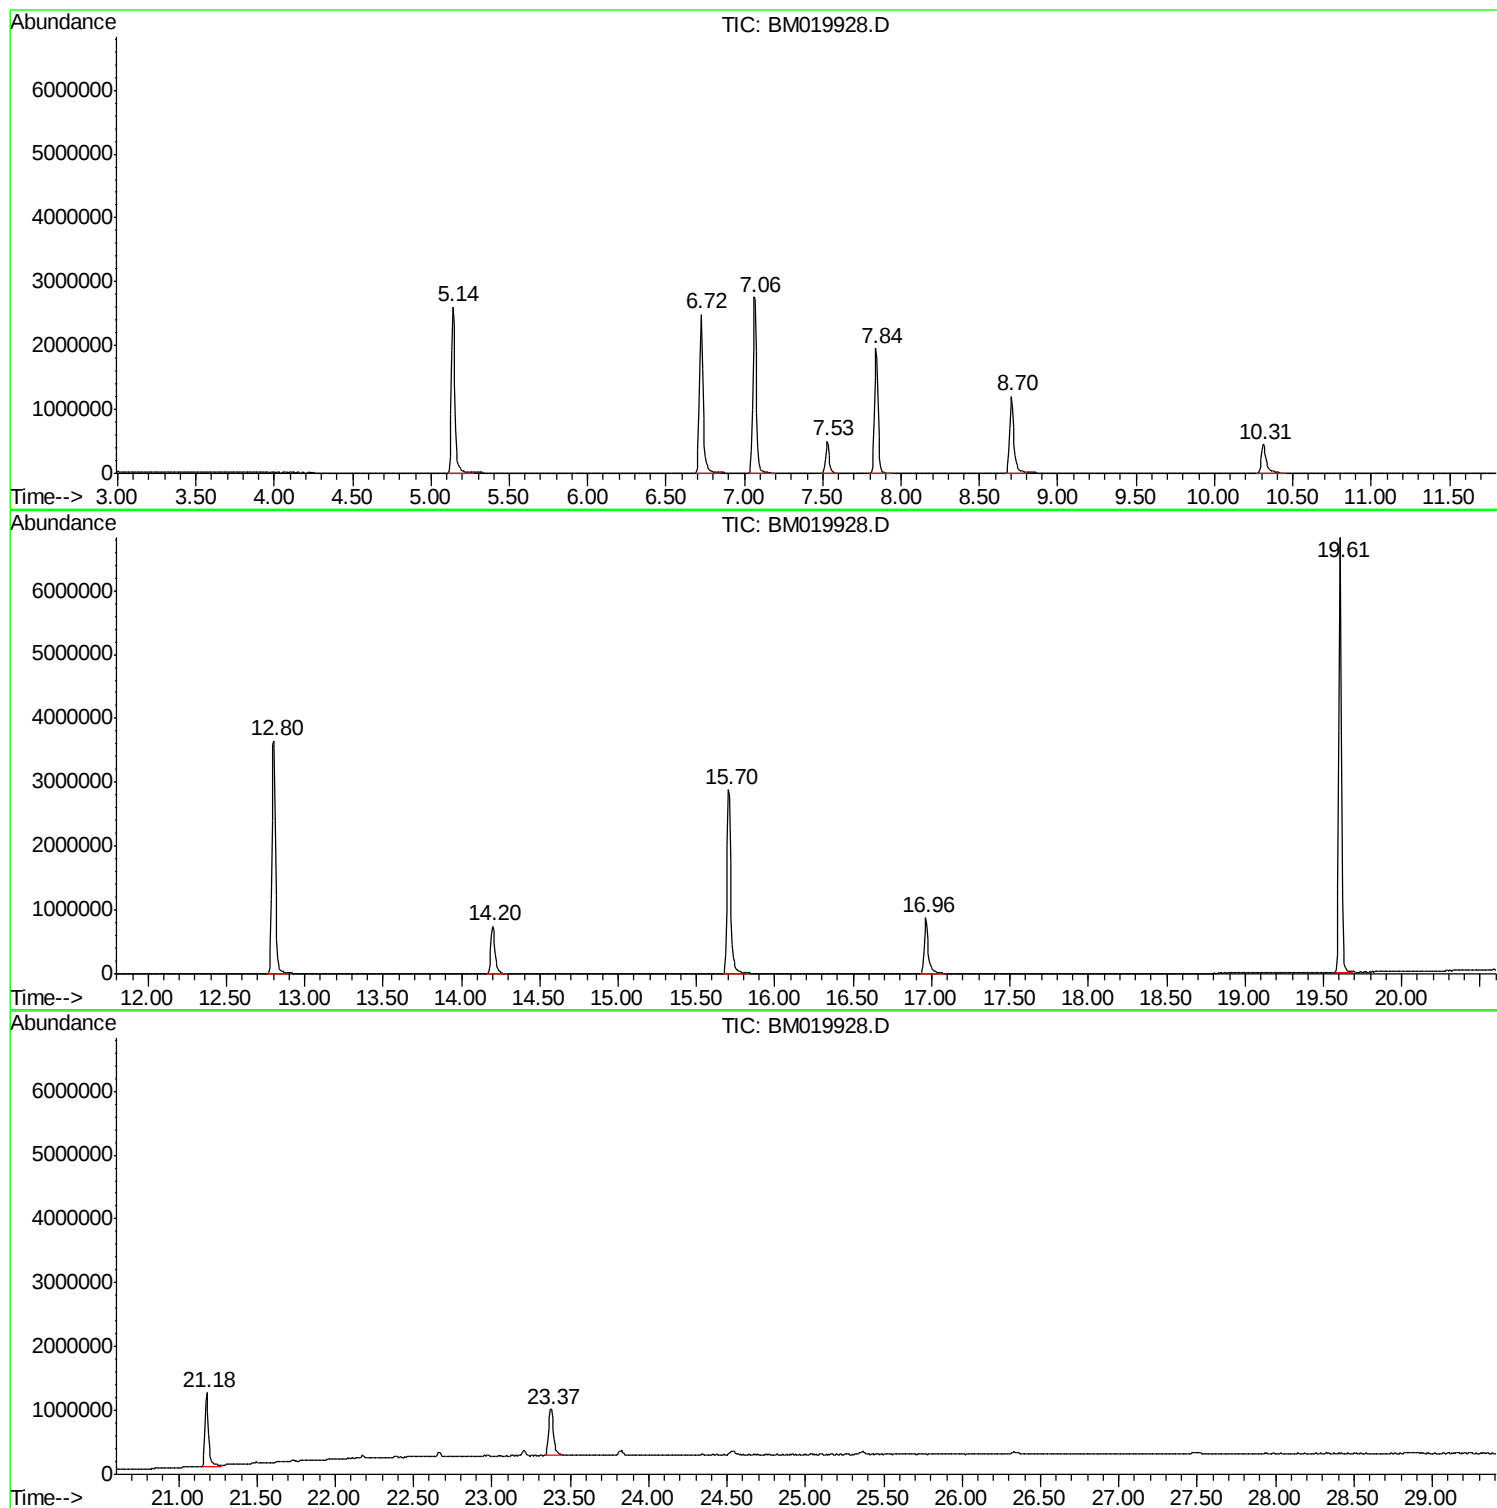

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041619\
Data File : BM019928.D
Acq On : 16 Apr 2019 11:45
Operator : JU/SJ
Sample : PB118322BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB118322BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.06 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.06	111.71 ng	4427820	1,4-Dichlorobenzene-d4	7.53

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
3		Imidazole, 4,5-dicyano-1-methyl-	132	C6H4N4	019485-35-9	22
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
5		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	13

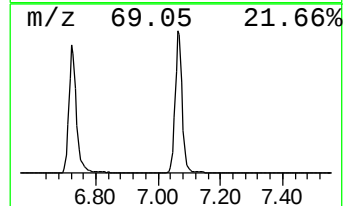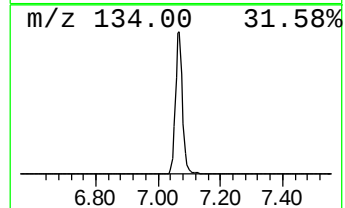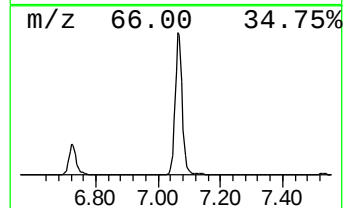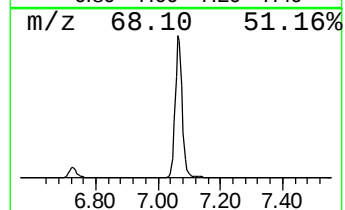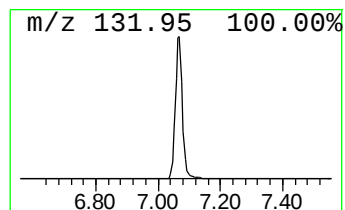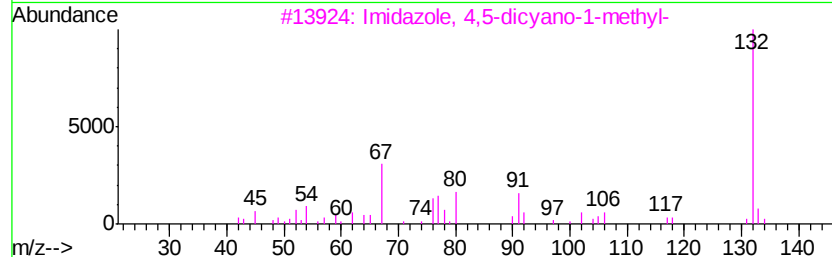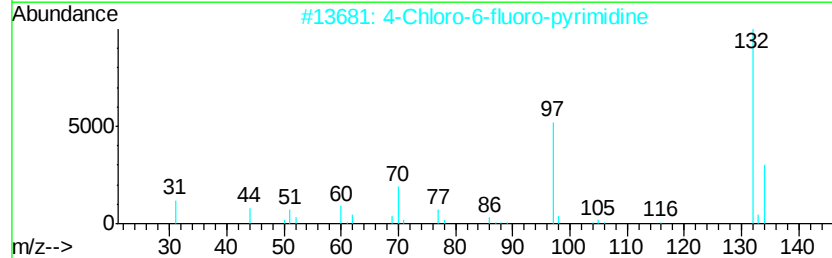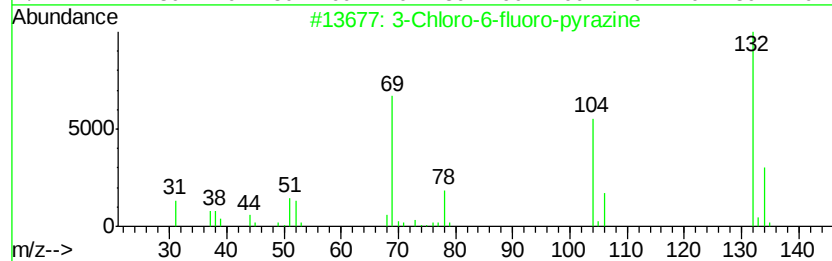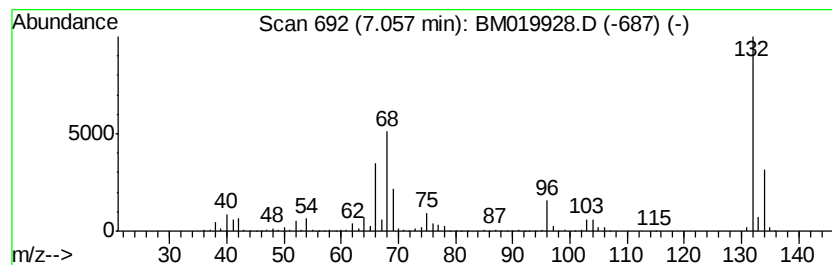

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041619\
Data File : BM019928.D
Acq On : 16 Apr 2019 11:45
Operator : JU/SJ
Sample : PB118322BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB118322BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.06	7.06	111.7	ng	4427820	1	7.53	792722	20.0