


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041619\
 Data File : BM019924.D
 Acq On : 16 Apr 2019 09:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 15 16:16:29 2019

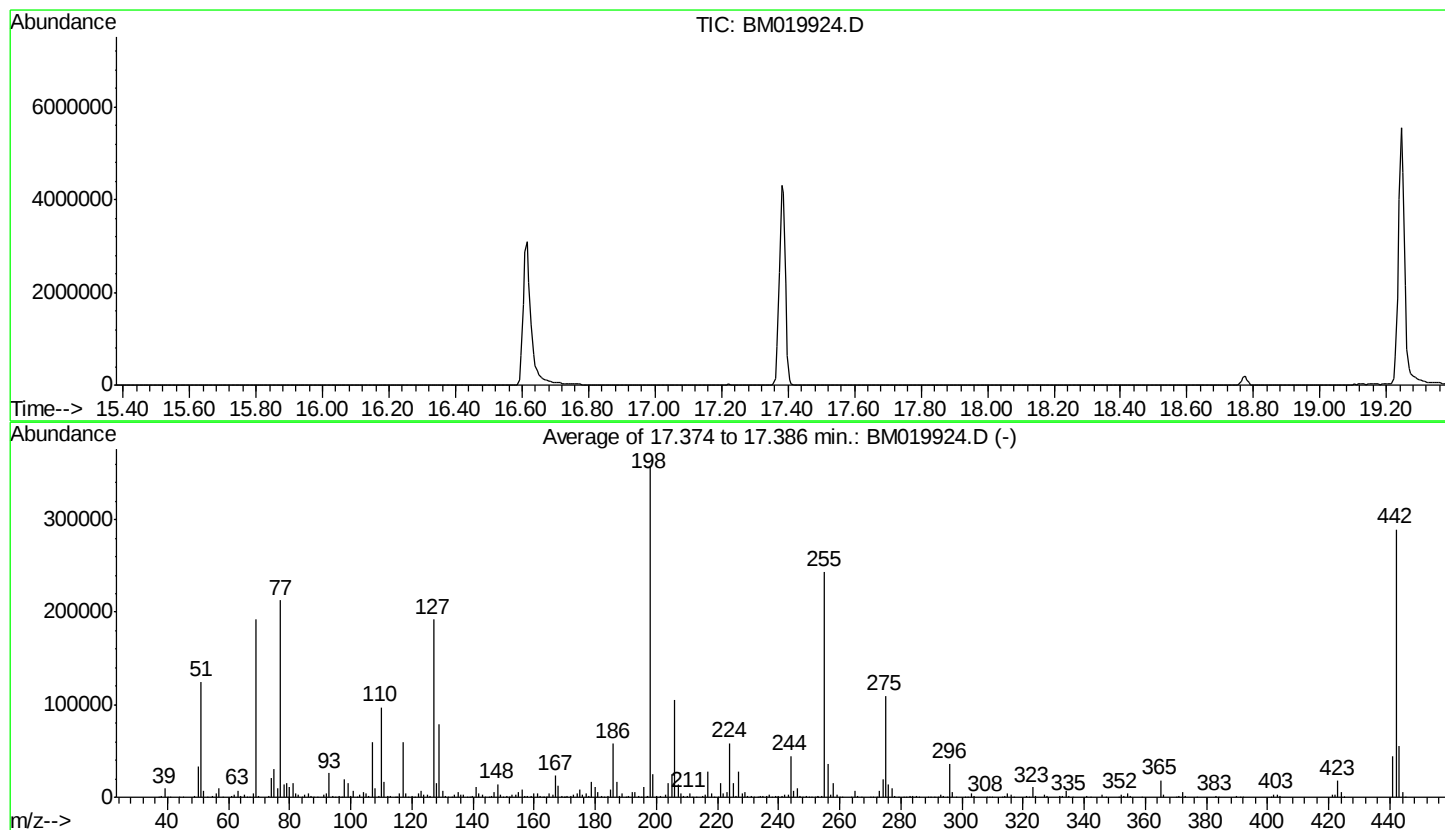

AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	124501	PASS
68	69	0.00	2	1.9	3664	PASS
69	198	0.00	100	53.6	192213	PASS
70	69	0.00	2	0.5	971	PASS
127	198	10	80	53.6	191978	PASS
197	198	0.00	2	0.6	2064	PASS
198	198	100	100	100.0	358336	PASS
199	198	5	9	6.9	24650	PASS
275	198	10	60	30.5	109432	PASS
365	198	1	100	5.0	17994	PASS
441	198	0.01	100	12.5	44821	PASS
442	198	50	100	80.8	289664	PASS
443	442	15	24	19.1	55264	PASS