

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041719\
 Data File : BM019951.D
 Acq On : 17 Apr 2019 22:55
 Operator : JU/SJ
 Sample : K2417-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 FK-PS-01-045

Quant Time: Apr 18 02:01:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 15 16:16:29 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	157148	20.00	ng	0.00
21) Naphthalene-d8	10.30	136	557604	20.00	ng	0.00
39) Acenaphthene-d10	14.19	164	263404	20.00	ng	0.00
64) Phenanthrene-d10	16.96	188	494296	20.00	ng	0.00
76) Chrysene-d12	21.17	240	534243	20.00	ng	0.00
87) Perylene-d12	23.36	264	704177	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.14	112	1398237	144.20	ng	0.00
7) Phenol-d6	6.72	99	1817533	124.55	ng	0.00
23) Nitrobenzene-d5	8.70	82	1121191	89.92	ng	0.00
42) 2,4,6-Tribromophenol	15.70	330	455152	107.35	ng	0.00
45) 2-Fluorobiphenyl	12.80	172	1628700	77.06	ng	0.00
79) Terphenyl-d14	19.60	244	1774069	58.57	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.67	163	244884	10.540	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041719\
Data File : BM019951.D
Acq On : 17 Apr 2019 22:55
Operator : JU/SJ
Sample : K2417-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FK-PS-01-045

Quant Time: Apr 18 02:01:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 16:16:29 2019
Response via : Initial Calibration

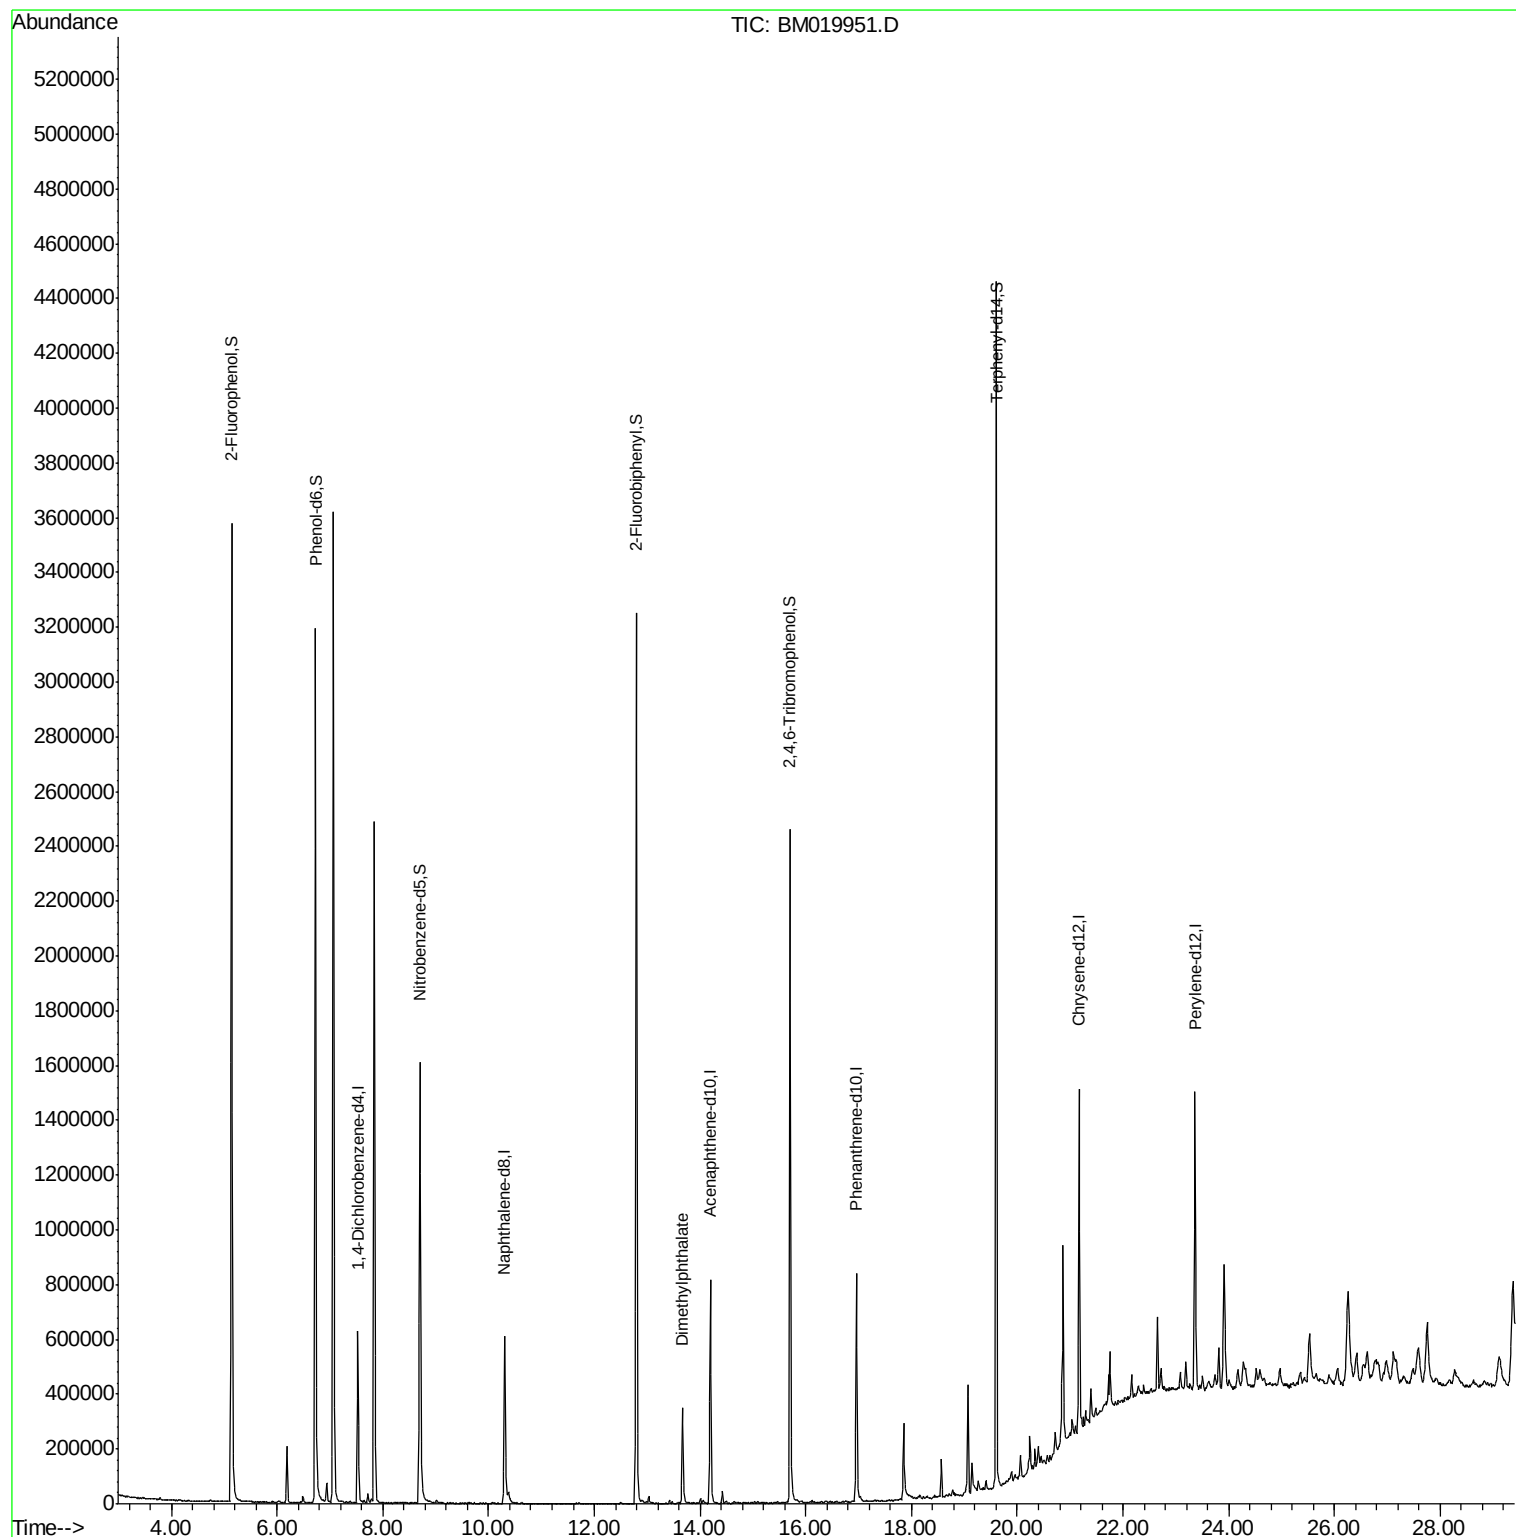

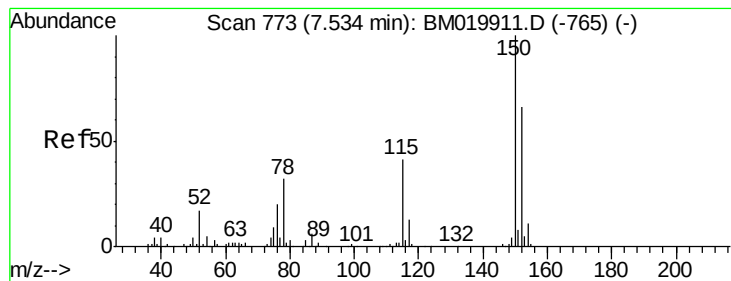


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.53 min Scan# 772
Delta R.T. -0.01 min
Lab File: BM019951.D
Acq: 17 Apr 2019 22:55

Instrument :
BNA_M
ClientSampleId :
FK-PS-01-045

Tgt Ion:152 Resp: 157148
Ion Ratio Lower Upper
152 100
150 157.0 122.1 183.1
115 62.0 50.0 75.0




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

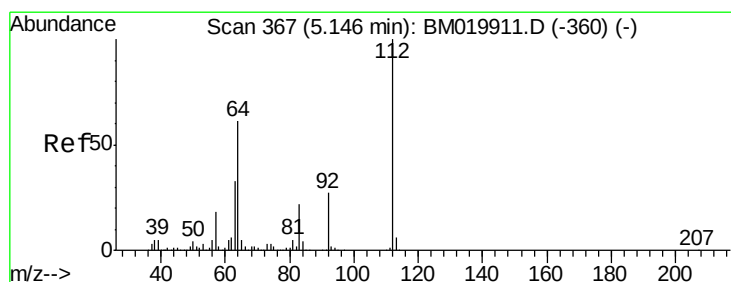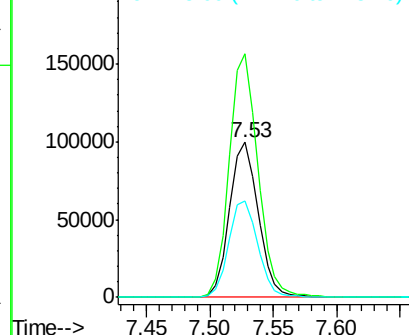



#5


2-Fluorophenol
Concen: 144.199 ng
RT: 5.14 min Scan# 366
Delta R.T. -0.01 min
Lab File: BM019951.D
Acq: 17 Apr 2019 22:55

Tgt Ion:112 Resp: 1398237
Ion Ratio Lower Upper
112 100
64 63.0 49.1 73.7
63 33.2 26.5 39.7

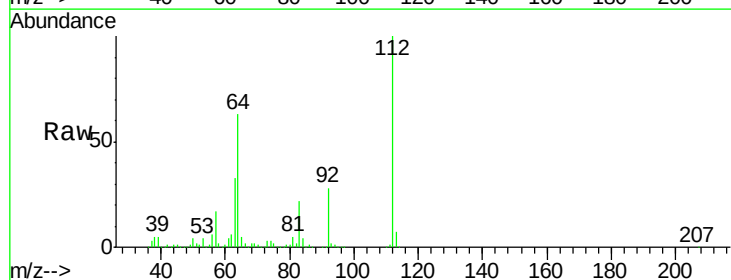

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

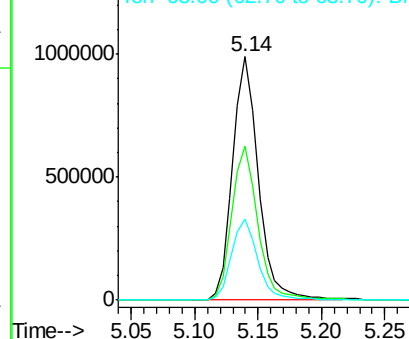

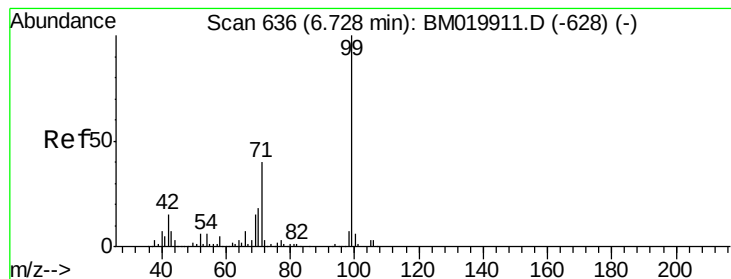

#7

Phenol-d6

Concen: 124.546 ng

RT: 6.72 min Scan# 635

Delta R.T. -0.01 min

Lab File: BM019951.D

Acq: 17 Apr 2019 22:55

Instrument :

BNA_M

ClientSampleId :

FK-PS-01-045


Tgt Ion: 99 Resp: 1817533

Ion Ratio Lower Upper




99 100

42 14.8 11.8 17.8

71 40.5 32.0 48.0



Abundance Ion 99.00 (98.70 to 99.70): BM019951.D (-619) (-)

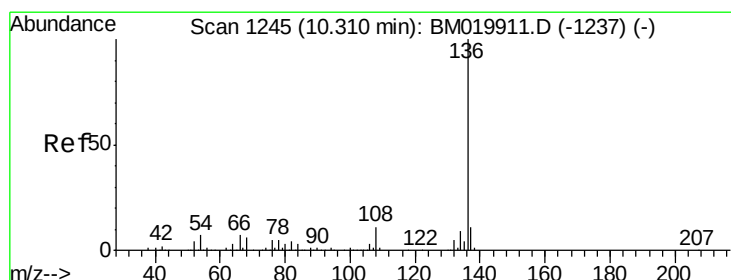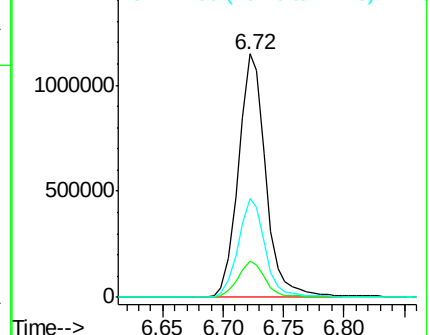

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.30 min Scan# 1244

Delta R.T. -0.01 min

Lab File: BM019951.D

Acq: 17 Apr 2019 22:55

Tgt Ion: 136 Resp: 557604


Ion Ratio Lower Upper

136 100



137 11.0 9.0 13.6


54 6.4 5.3 7.9

68 7.2 5.2 7.8



Abundance Ion 136.00 (135.70 to 136.70): BM019951.D (-1228) (-)



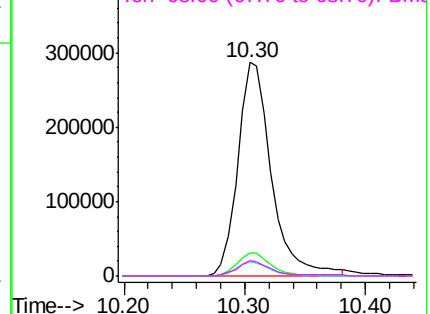





#23
 Nitrobenzene-d5
 Concen: 89.922 ng
 RT: 8.70 min Scan# 971
 Delta R.T. -0.01 min
 Lab File: BM019951.D
 Acq: 17 Apr 2019 22:55




Instrument :
 BNA_M
 ClientSampleId :
 FK-PS-01-045


Tgt Ion: 82 Resp: 1121191
 Ion Ratio Lower Upper
 82 100
 128 37.1 29.0 43.4
 54 38.5 30.2 45.4

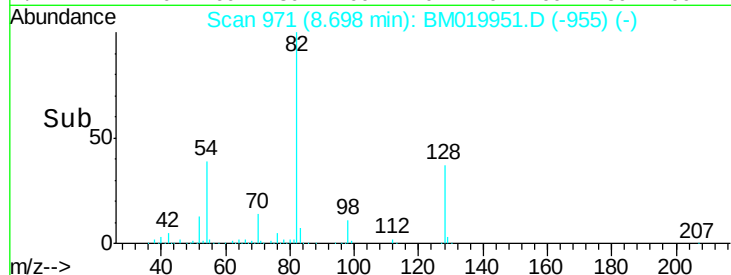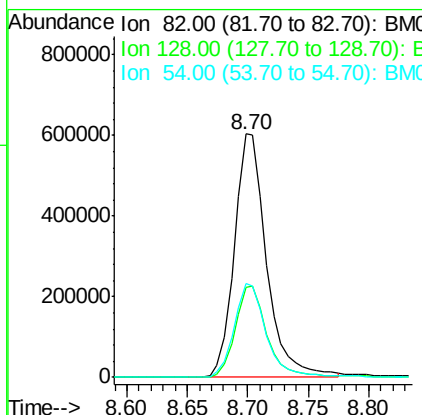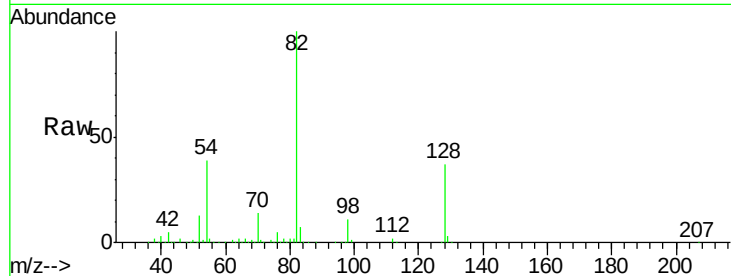

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.19 min Scan# 1905
 Delta R.T. -0.01 min
 Lab File: BM019951.D
 Acq: 17 Apr 2019 22:55

Tgt Ion: 164 Resp: 263404
 Ion Ratio Lower Upper
 164 100
 162 102.6 83.0 124.4
 160 47.4 36.6 55.0

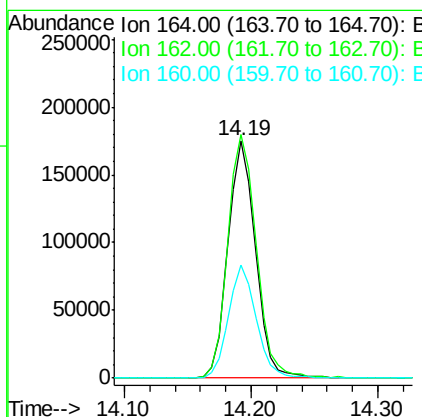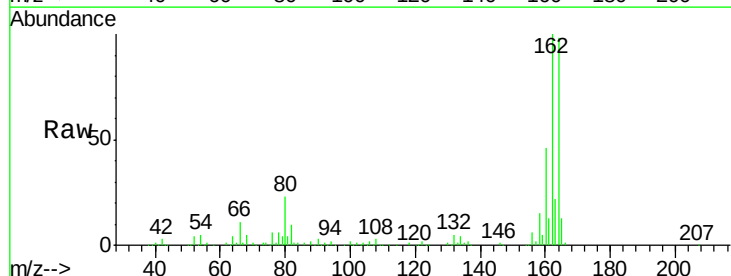


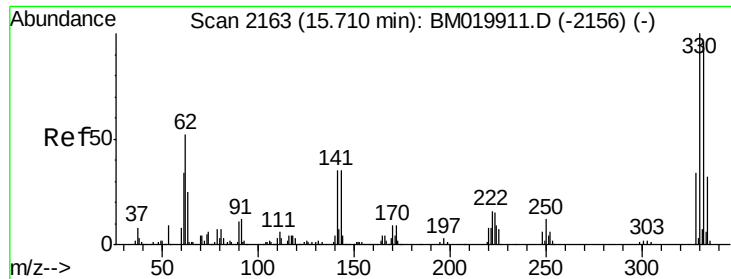




#42
 2,4,6-Tribromophenol
 Concen: 107.345 ng
 RT: 15.70 min Scan# 2162
 Delta R.T. -0.01 min
 Lab File: BM019951.D
 Acq: 17 Apr 2019 22:55

Instrument :
 BNA_M
 ClientSampleId :
 FK-PS-01-045

Tgt Ion:330 Resp: 455152
 Ion Ratio Lower Upper
 330 100
 332 95.9 77.4 116.2
 141 36.8 29.0 43.4




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

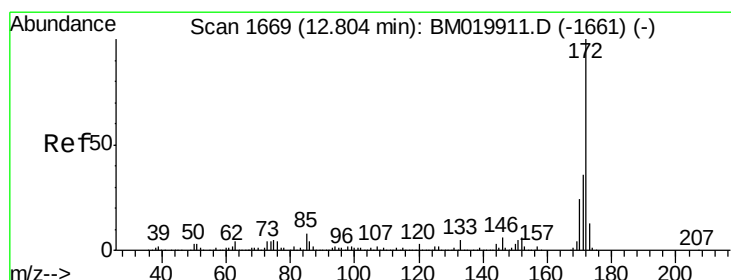
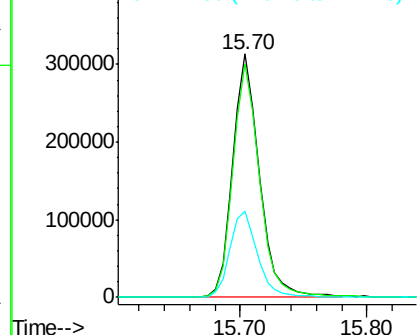



#45
 2-Fluorobiphenyl
 Concen: 77.058 ng
 RT: 12.80 min Scan# 1668
 Delta R.T. -0.01 min
 Lab File: BM019951.D
 Acq: 17 Apr 2019 22:55

Tgt Ion:172 Resp: 1628700
 Ion Ratio Lower Upper
 172 100
 171 36.3 28.9 43.3
 170 23.4 19.0 28.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

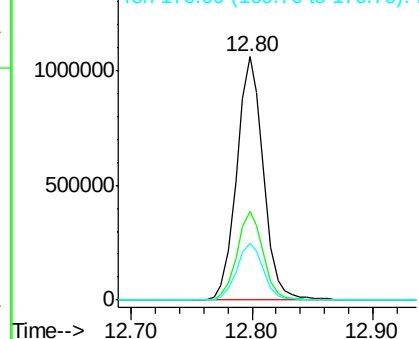

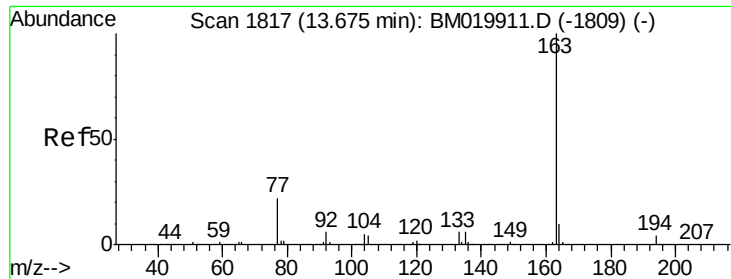

#50

Dimethylphthalate

Concen: 10.540 ng

RT: 13.67 min Scan# 1816

Delta R.T. -0.01 min

Lab File: BM019951.D

Acq: 17 Apr 2019 22:55

Instrument :

BNA_M

ClientSampleId :

FK-PS-01-045


Tgt Ion:163 Resp: 244884

Ion Ratio Lower Upper

163 100

194 3.8 3.1 4.7




164 10.6 7.9 11.9

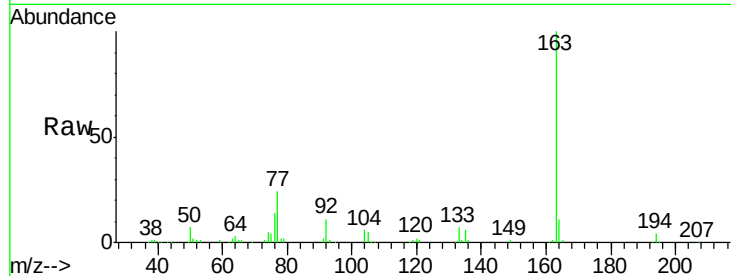

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

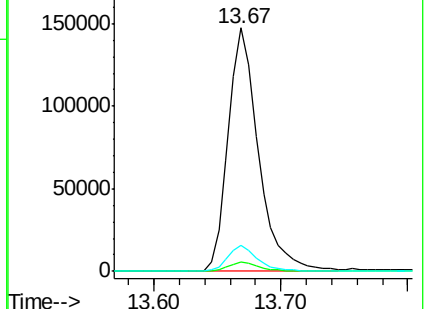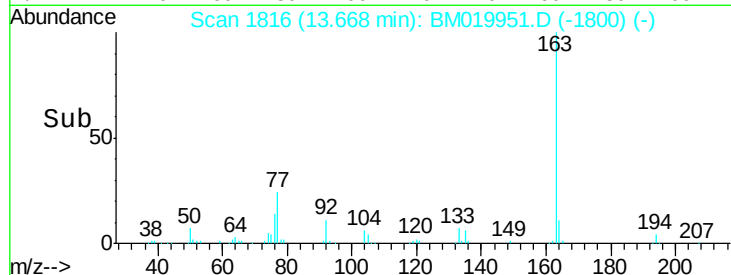

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 16.96 min Scan# 2375

Delta R.T. -0.01 min

Lab File: BM019951.D

Acq: 17 Apr 2019 22:55


Tgt Ion:188 Resp: 494296

Ion Ratio Lower Upper

188 100

94 9.7 7.6 11.4



80 12.1 9.4 14.0




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

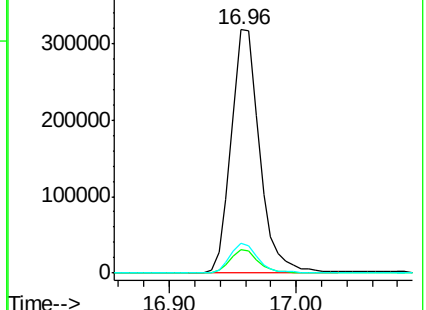







#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.17 min Scan# 3092
Delta R.T. -0.01 min
Lab File: BM019951.D
Acq: 17 Apr 2019 22:55

Instrument :
BNA_M
ClientSampleId :
FK-PS-01-045

Tgt Ion:240 Resp: 534243
Ion Ratio Lower Upper
240 100
120 10.0 8.6 13.0
236 26.5 21.4 32.2

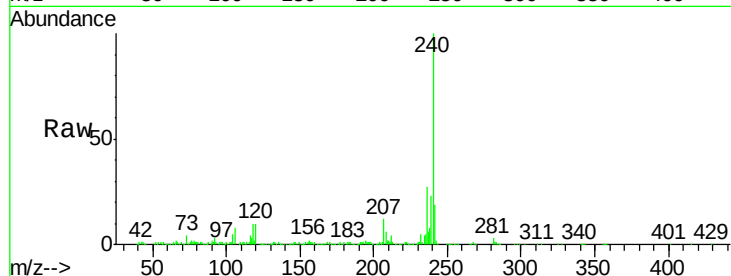


Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E


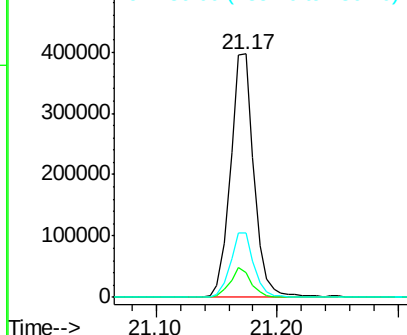



#79
Terphenyl-d14
Concen: 58.572 ng
RT: 19.60 min Scan# 2825
Delta R.T. -0.01 min
Lab File: BM019951.D
Acq: 17 Apr 2019 22:55

Tgt Ion:244 Resp: 1774069
Ion Ratio Lower Upper
244 100
212 7.1 5.7 8.5
122 10.5 9.1 13.7



Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

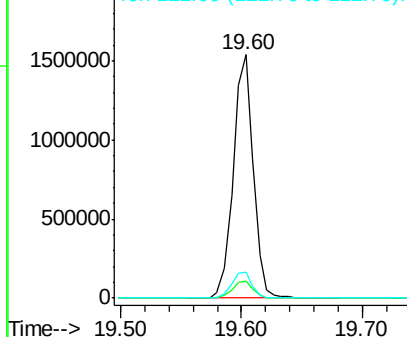




#87
Perylene-d12
Concen: 20.000 ng
RT: 23.36 min Scan# 3464
Delta R.T. -0.02 min
Lab File: BM019951.D
Acq: 17 Apr 2019 22:55

Instrument :
BNA_M
ClientSampleId :
FK-PS-01-045

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.6	19.2	28.8
265	21.6	17.2	25.8

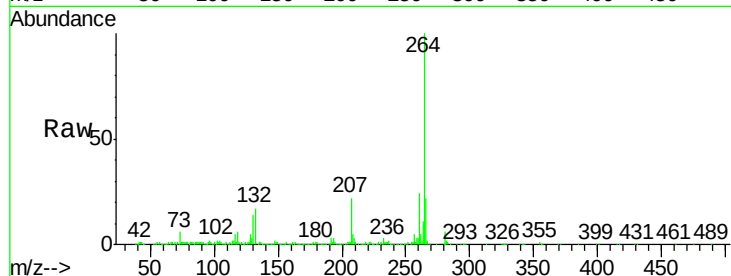

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

