

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041719\
 Data File : BM019952.D
 Acq On : 17 Apr 2019 23:32
 Operator : JU/SJ
 Sample : K2422-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP1-S

Quant Time: Apr 18 02:04:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 15 16:16:29 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	152903	20.00	ng	0.00
21) Naphthalene-d8	10.30	136	557001	20.00	ng	0.00
39) Acenaphthene-d10	14.19	164	274620	20.00	ng	0.00
64) Phenanthrene-d10	16.96	188	505810	20.00	ng	0.00
76) Chrysene-d12	21.17	240	497317	20.00	ng	-0.01
87) Perylene-d12	23.37	264	642990	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.14	112	1049998	111.29	ng	0.00
7) Phenol-d6	6.72	99	1398119	98.47	ng	0.00
23) Nitrobenzene-d5	8.70	82	861800	69.19	ng	0.00
42) 2,4,6-Tribromophenol	15.70	330	381772	86.36	ng	0.00
45) 2-Fluorobiphenyl	12.80	172	1569704	71.23	ng	0.00
79) Terphenyl-d14	19.60	244	1764644	62.59	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.67	163	295491	12.199	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041719\
Data File : BM019952.D
Acq On : 17 Apr 2019 23:32
Operator : JU/SJ
Sample : K2422-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP1-S

Quant Time: Apr 18 02:04:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 16:16:29 2019
Response via : Initial Calibration

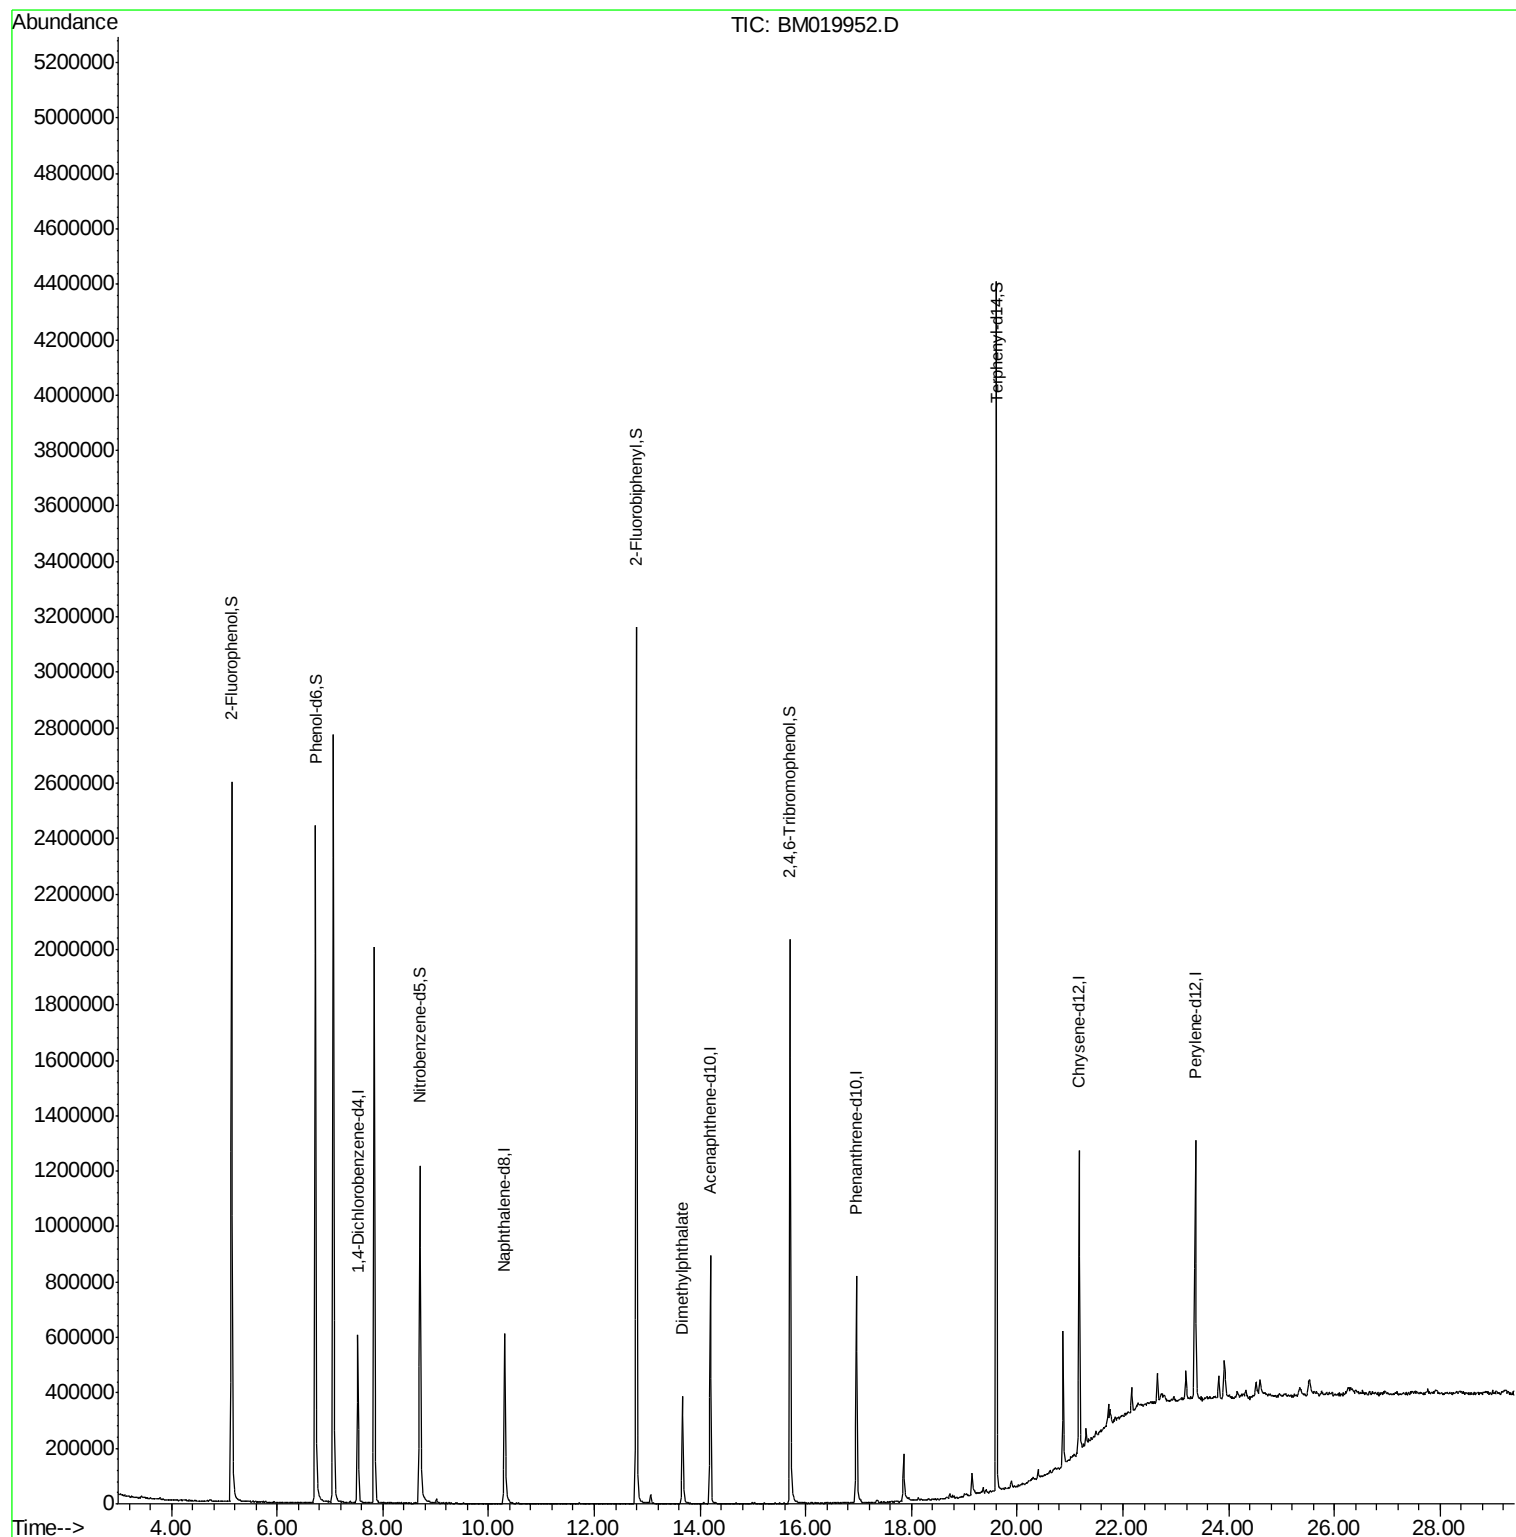

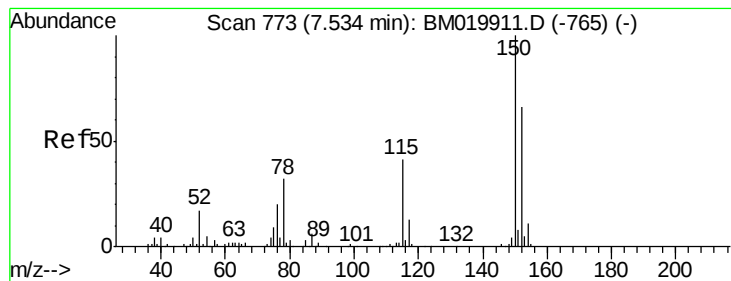


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.53 min Scan# 772
Delta R.T. -0.01 min
Lab File: BM019952.D
Acq: 17 Apr 2019 23:32

Instrument :
BNA_M
ClientSampleId :
TP1-S

Tgt Ion	Ratio	Lower	Upper
152	100		
150	152.3	122.1	183.1
115	63.1	50.0	75.0




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

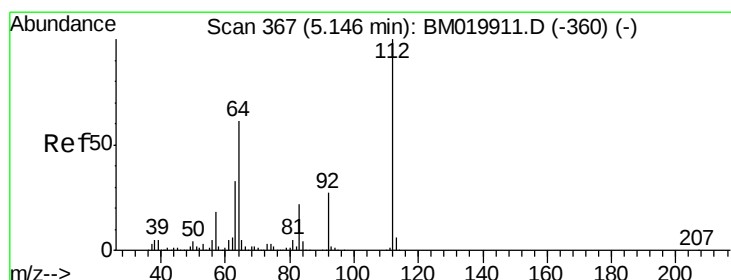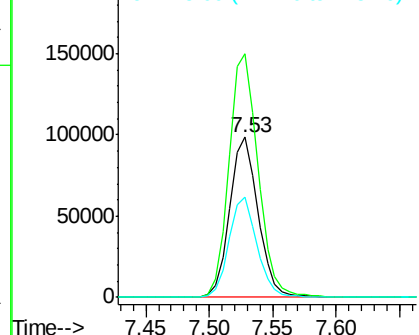



#5


2-Fluorophenol
Concen: 111.291 ng
RT: 5.14 min Scan# 366
Delta R.T. -0.00 min
Lab File: BM019952.D
Acq: 17 Apr 2019 23:32

Tgt Ion	Ratio	Lower	Upper
112	100		
64	62.0	49.1	73.7
63	32.9	26.5	39.7



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

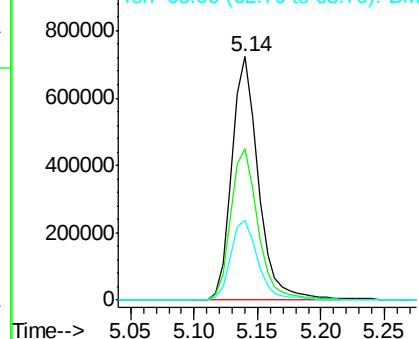

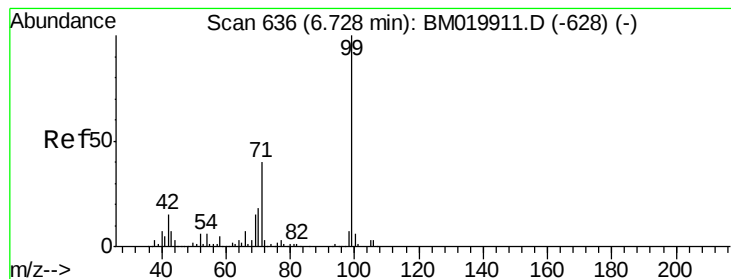

#7

Phenol-d6

Concen: 98.466 ng

RT: 6.72 min Scan# 635

Delta R.T. -0.01 min

Lab File: BM019952.D

Acq: 17 Apr 2019 23:32

Instrument :

BNA_M

ClientSampleId :

TP1-S


Tgt Ion: 99 Resp: 1398119

Ion Ratio Lower Upper

99 100

42 14.5 11.8 17.8

71 40.0 32.0 48.0






Abundance

Ion 99.00 (98.70 to 99.70): BM019952.D (-619) (-)

Ion 42.00 (41.70 to 42.70): BM019952.D (-619) (-)

Ion 71.00 (70.70 to 71.70): BM019952.D (-619) (-)

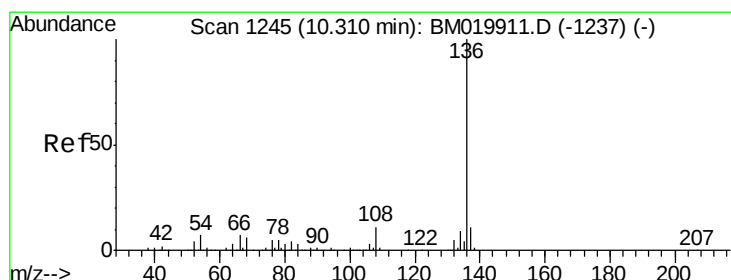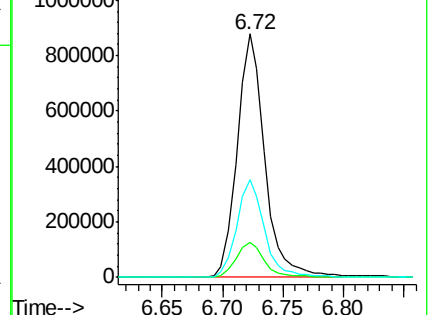

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.30 min Scan# 1244

Delta R.T. -0.01 min

Lab File: BM019952.D

Acq: 17 Apr 2019 23:32

Tgt Ion: 136 Resp: 557001


Ion Ratio Lower Upper

136 100

137 10.7 9.0 13.6

54 6.8 5.3 7.9

68 7.1 5.2 7.8





Abundance


Ion 136.00 (135.70 to 136.70): BM019952.D (-1228) (-)

Ion 137.00 (136.70 to 137.70): BM019952.D (-1228) (-)

Ion 54.00 (53.70 to 54.70): BM019952.D (-1228) (-)

Ion 68.00 (67.70 to 68.70): BM019952.D (-1228) (-)



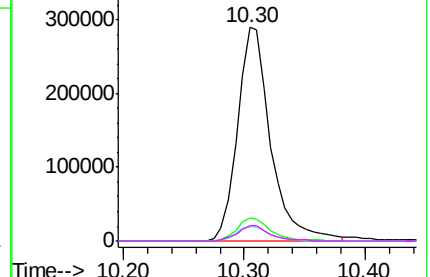





#23
 Nitrobenzene-d5
 Concen: 69.193 ng
 RT: 8.70 min Scan# 972
 Delta R.T. 0.00 min
 Lab File: BM019952.D
 Acq: 17 Apr 2019 23:32




Instrument :
 BNA_M
 ClientSampleId :
 TP1-S


Tgt Ion	Ratio	Lower	Upper
82	100		
128	37.8	29.0	43.4
54	37.5	30.2	45.4

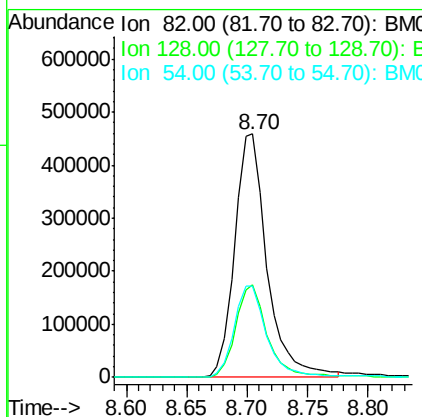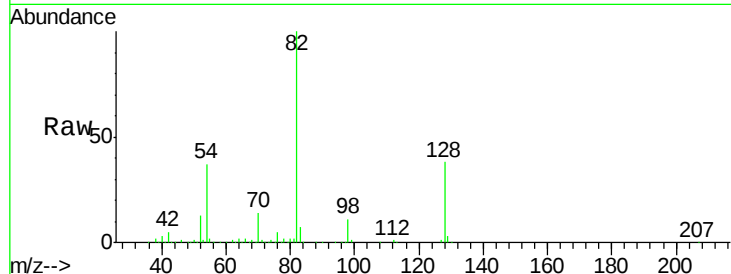

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.19 min Scan# 1905
 Delta R.T. -0.01 min
 Lab File: BM019952.D
 Acq: 17 Apr 2019 23:32

Tgt Ion	Ratio	Lower	Upper
164	100		
162	103.9	83.0	124.4
160	45.3	36.6	55.0



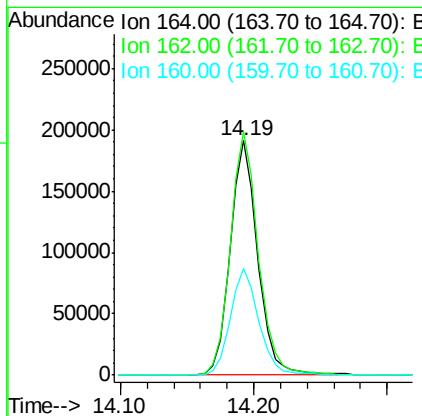



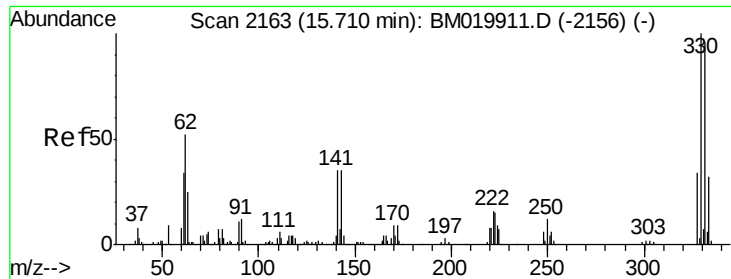

#42
 2,4,6-Tribromophenol
 Concen: 86.362 ng
 RT: 15.70 min Scan# 2162
 Delta R.T. -0.01 min
 Lab File: BM019952.D
 Acq: 17 Apr 2019 23:32




Instrument :
 BNA_M
 ClientSampleId :
 TP1-S


Tgt Ion:330 Resp: 381772
 Ion Ratio Lower Upper
 330 100
 332 97.0 77.4 116.2
 141 37.7 29.0 43.4

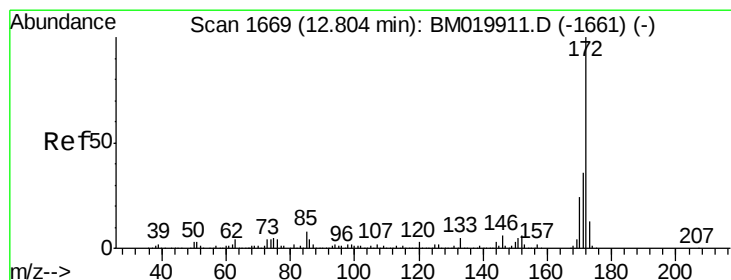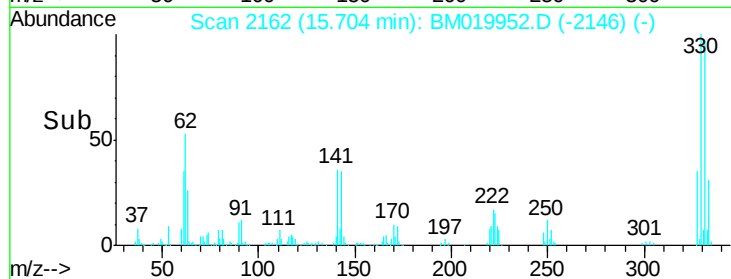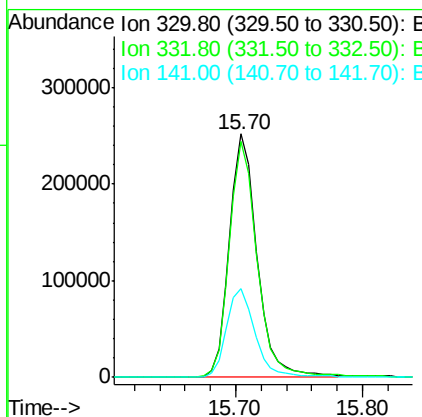

#45
 2-Fluorobiphenyl
 Concen: 71.234 ng
 RT: 12.80 min Scan# 1668
 Delta R.T. -0.01 min
 Lab File: BM019952.D
 Acq: 17 Apr 2019 23:32

Tgt Ion:172 Resp: 1569704
 Ion Ratio Lower Upper
 172 100
 171 36.3 28.9 43.3
 170 23.8 19.0 28.4

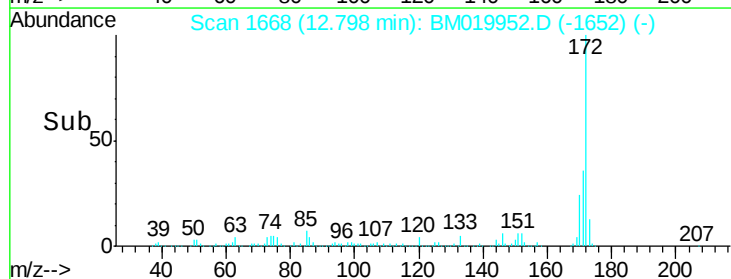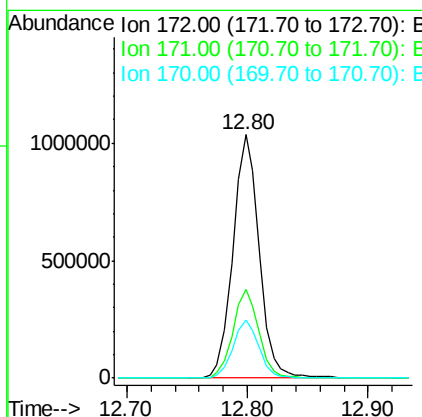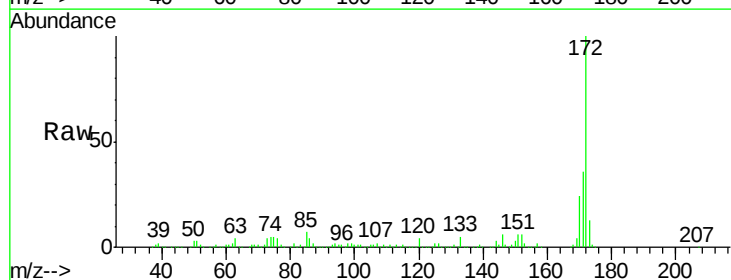



#50

Dimethylphthalate

Concen: 12.199 ng

RT: 13.67 min Scan# 1816

Delta R.T. -0.01 min

Lab File: BM019952.D

Acq: 17 Apr 2019 23:32

Instrument :

BNA_M

ClientSampleId :

TP1-S


Tgt Ion:163 Resp: 295491

Ion Ratio Lower Upper

163 100

194 3.7 3.1 4.7




164 10.0 7.9 11.9

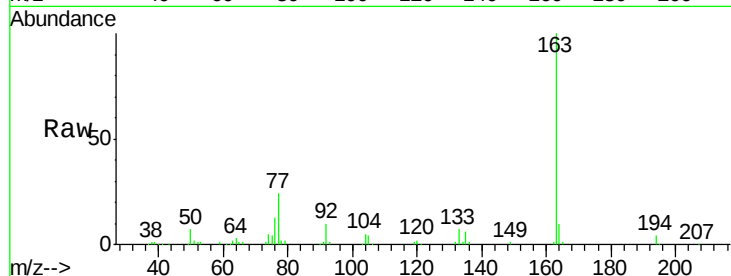

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

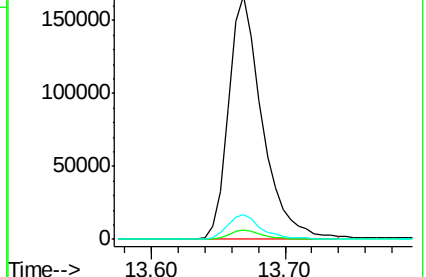

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 16.96 min Scan# 2375

Delta R.T. -0.01 min

Lab File: BM019952.D

Acq: 17 Apr 2019 23:32


Tgt Ion:188 Resp: 505810

Ion Ratio Lower Upper

188 100

94 9.9 7.6 11.4



80 12.2 9.4 14.0




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0



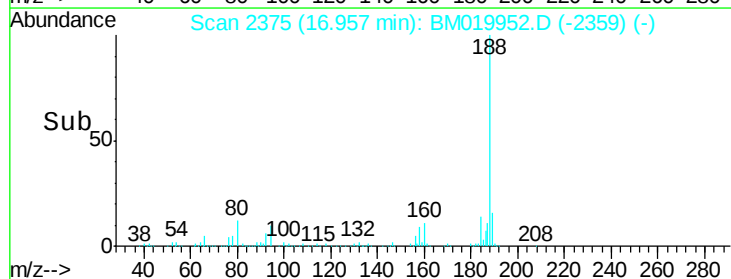
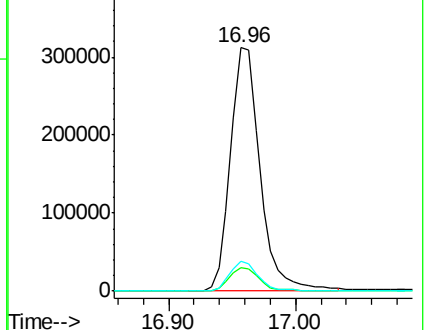


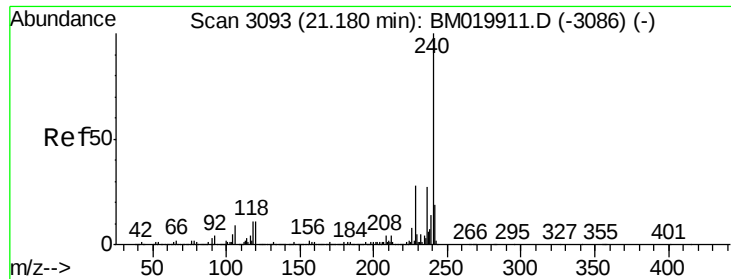

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.17 min Scan# 3091
Delta R.T. -0.01 min
Lab File: BM019952.D
Acq: 17 Apr 2019 23:32




Instrument :
BNA_M
ClientSampleId :
TP1-S


Tgt Ion:240 Resp: 497317
Ion Ratio Lower Upper
240 100
120 11.5 8.6 13.0
236 26.6 21.4 32.2

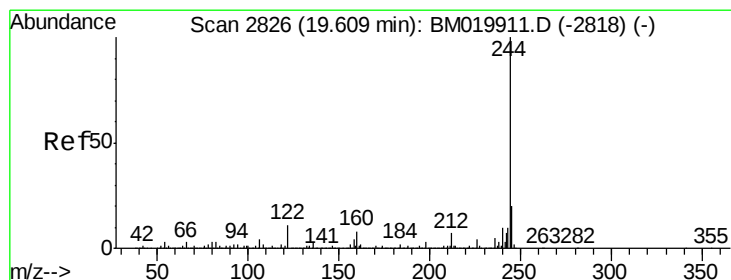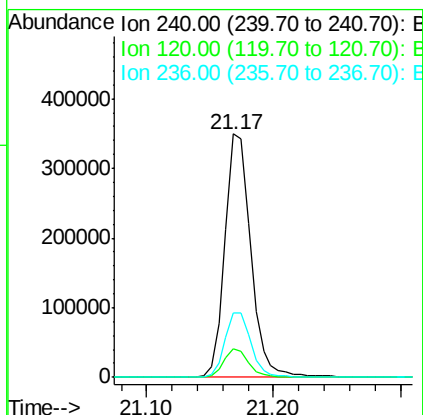

#79
Terphenyl-d14
Concen: 62.586 ng
RT: 19.60 min Scan# 2825
Delta R.T. -0.01 min
Lab File: BM019952.D
Acq: 17 Apr 2019 23:32

Tgt Ion:244 Resp: 1764644
Ion Ratio Lower Upper
244 100
212 7.0 5.7 8.5
122 10.7 9.1 13.7

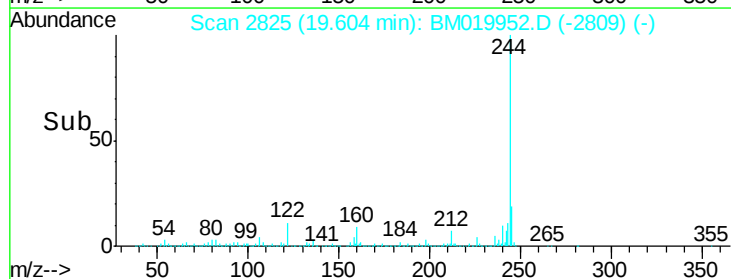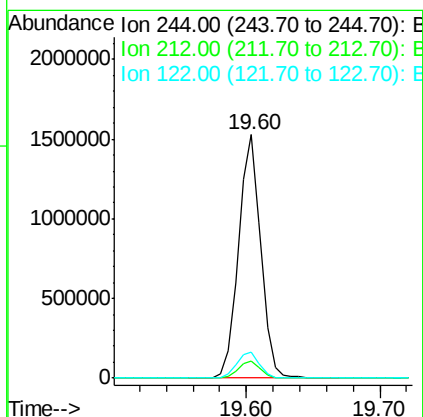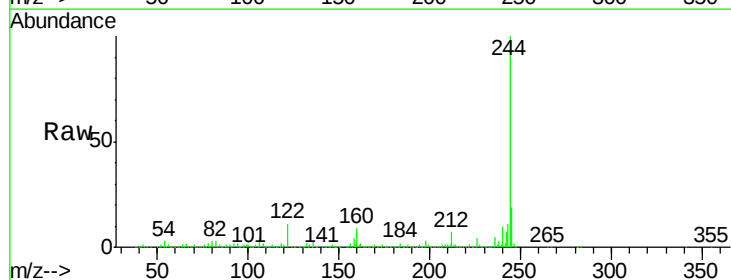


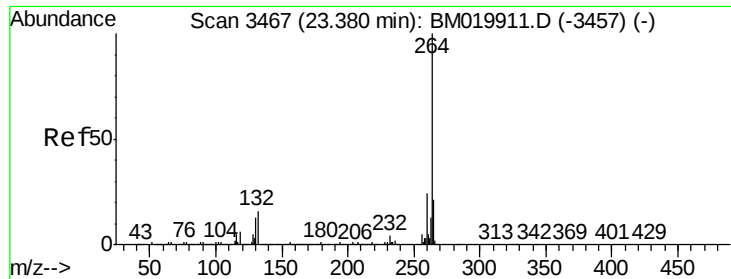

#87
Perylene-d12
Concen: 20.000 ng
RT: 23.37 min Scan# 3465
Delta R.T. -0.01 min
Lab File: BM019952.D
Acq: 17 Apr 2019 23:32

Instrument :
BNA_M
ClientSampleId :
TP1-S

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.3	19.2	28.8
265	22.2	17.2	25.8



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

