


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041719\
 Data File : BM019933.D
 Acq On : 17 Apr 2019 11:20
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 15 16:16:29 2019

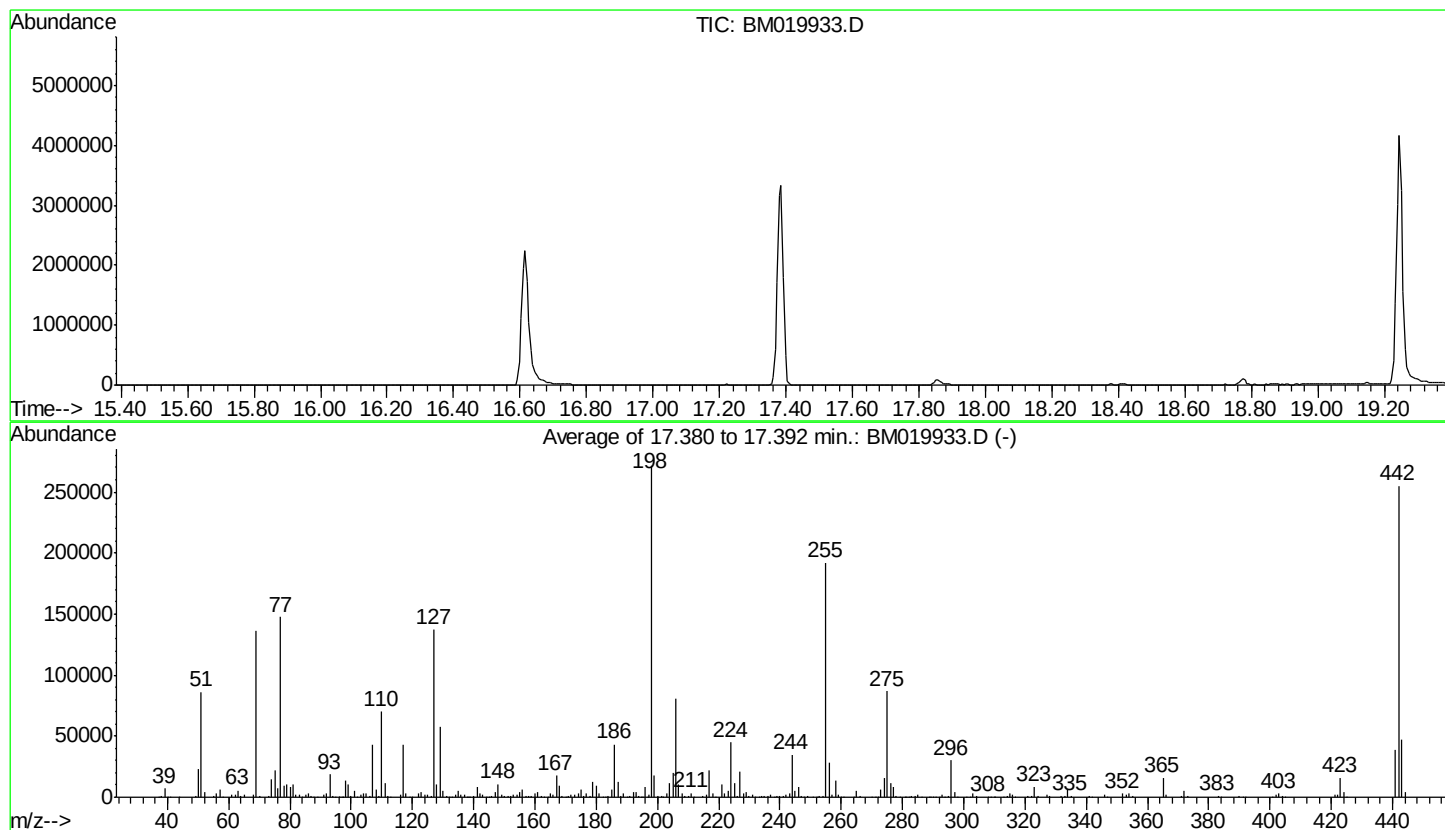

AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	86461	PASS
68	69	0.00	2	1.7	2313	PASS
69	198	0.00	100	50.3	136456	PASS
70	69	0.00	2	0.5	747	PASS
127	198	10	80	50.5	137237	PASS
197	198	0.00	2	0.6	1676	PASS
198	198	100	100	100.0	271552	PASS
199	198	5	9	6.7	18109	PASS
275	198	10	60	32.0	87002	PASS
365	198	1	100	5.9	15985	PASS
441	198	0.01	100	14.4	39200	PASS
442	198	50	100	93.9	255018	PASS
443	442	15	24	18.6	47437	PASS