


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM041819\
 Data File : BM019953.D
 Acq On : 18 Apr 2019 14:13
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 19 00:56:08 2019

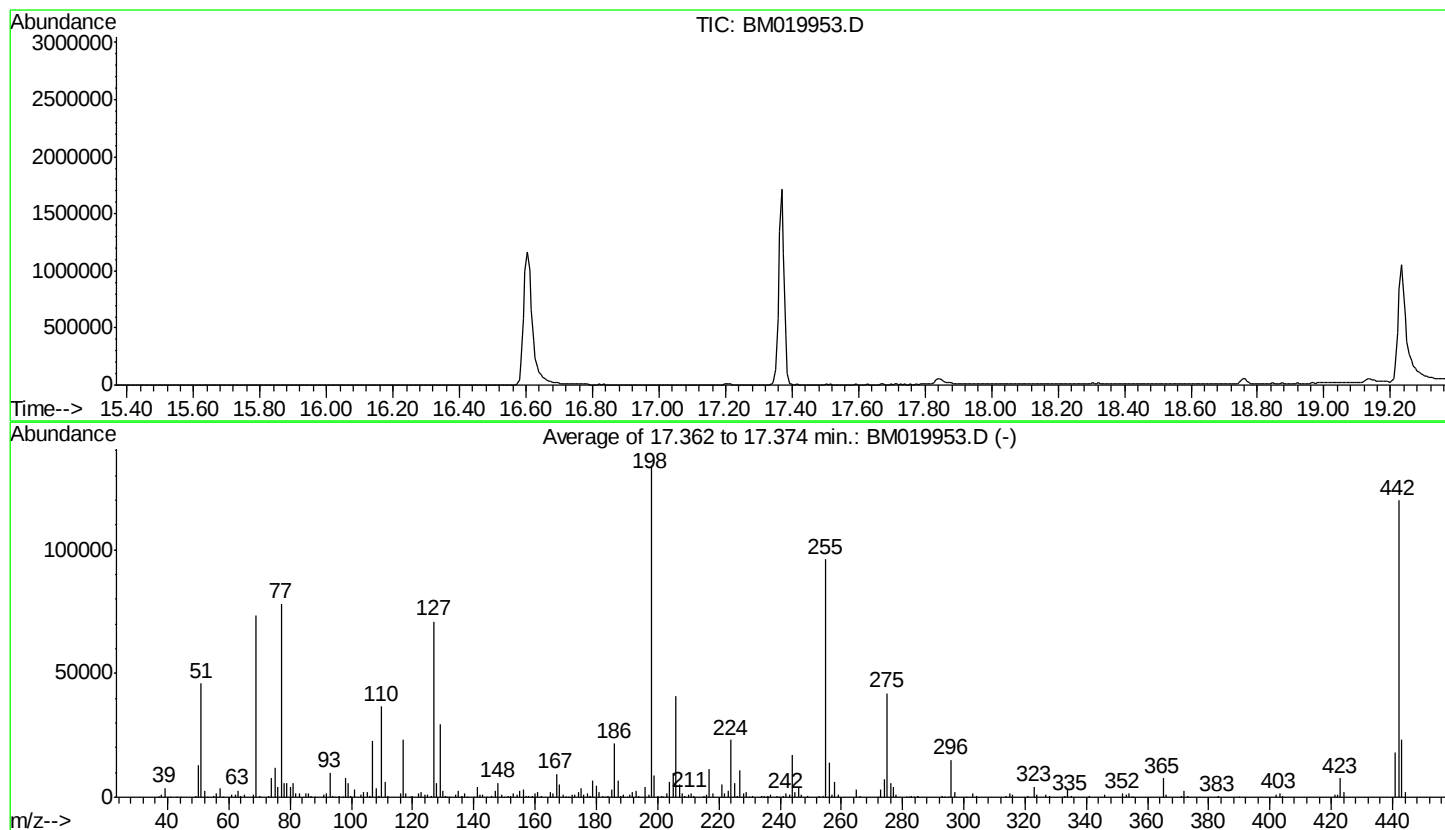

AutoFind: Scans 2444, 2445, 2446; Background Corrected with Scan 2438

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	45957	PASS
68	69	0.00	2	1.6	1185	PASS
69	198	0.00	100	54.8	73400	PASS
70	69	0.00	2	0.7	539	PASS
127	198	10	80	53.0	70973	PASS
197	198	0.00	2	0.6	848	PASS
198	198	100	100	100.0	134026	PASS
199	198	5	9	6.7	8955	PASS
275	198	10	60	31.4	42141	PASS
365	198	1	100	5.6	7522	PASS
441	198	0.01	100	13.5	18127	PASS
442	198	50	100	89.5	120005	PASS
443	442	15	24	19.6	23461	PASS