

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
 Data File : BM045362.D
 Acq On : 18 Apr 2024 19:44
 Operator : MA/JU
 Sample : PB160255BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK255

Quant Time: Apr 18 22:21:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 18 22:19:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.576	152	1407	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.342	136	4013	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.224	164	1905	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.082	188	281247	0.400	ng/ul	# 0.06
17) Chrysene-d12	21.227	240	3235	0.400	ng/ul	0.00
23) Perylene-d12	23.410	264	6122	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	7633	4.130	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.975	152	1346	0.247	ng/ul	-0.02
18) Fluoranthene-d10	19.030	212	2558	0.313	ng/ul	-0.02
Target Compounds						Qvalue
20) Pyrene	19.392	202	588	0.048	ng/ul#	1
26) Benzo(a)pyrene	23.253	252	1428	0.068	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045362.D
Acq On : 18 Apr 2024 19:44
Operator : MA/JU
Sample : PB160255BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK255

Quant Time: Apr 18 22:21:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

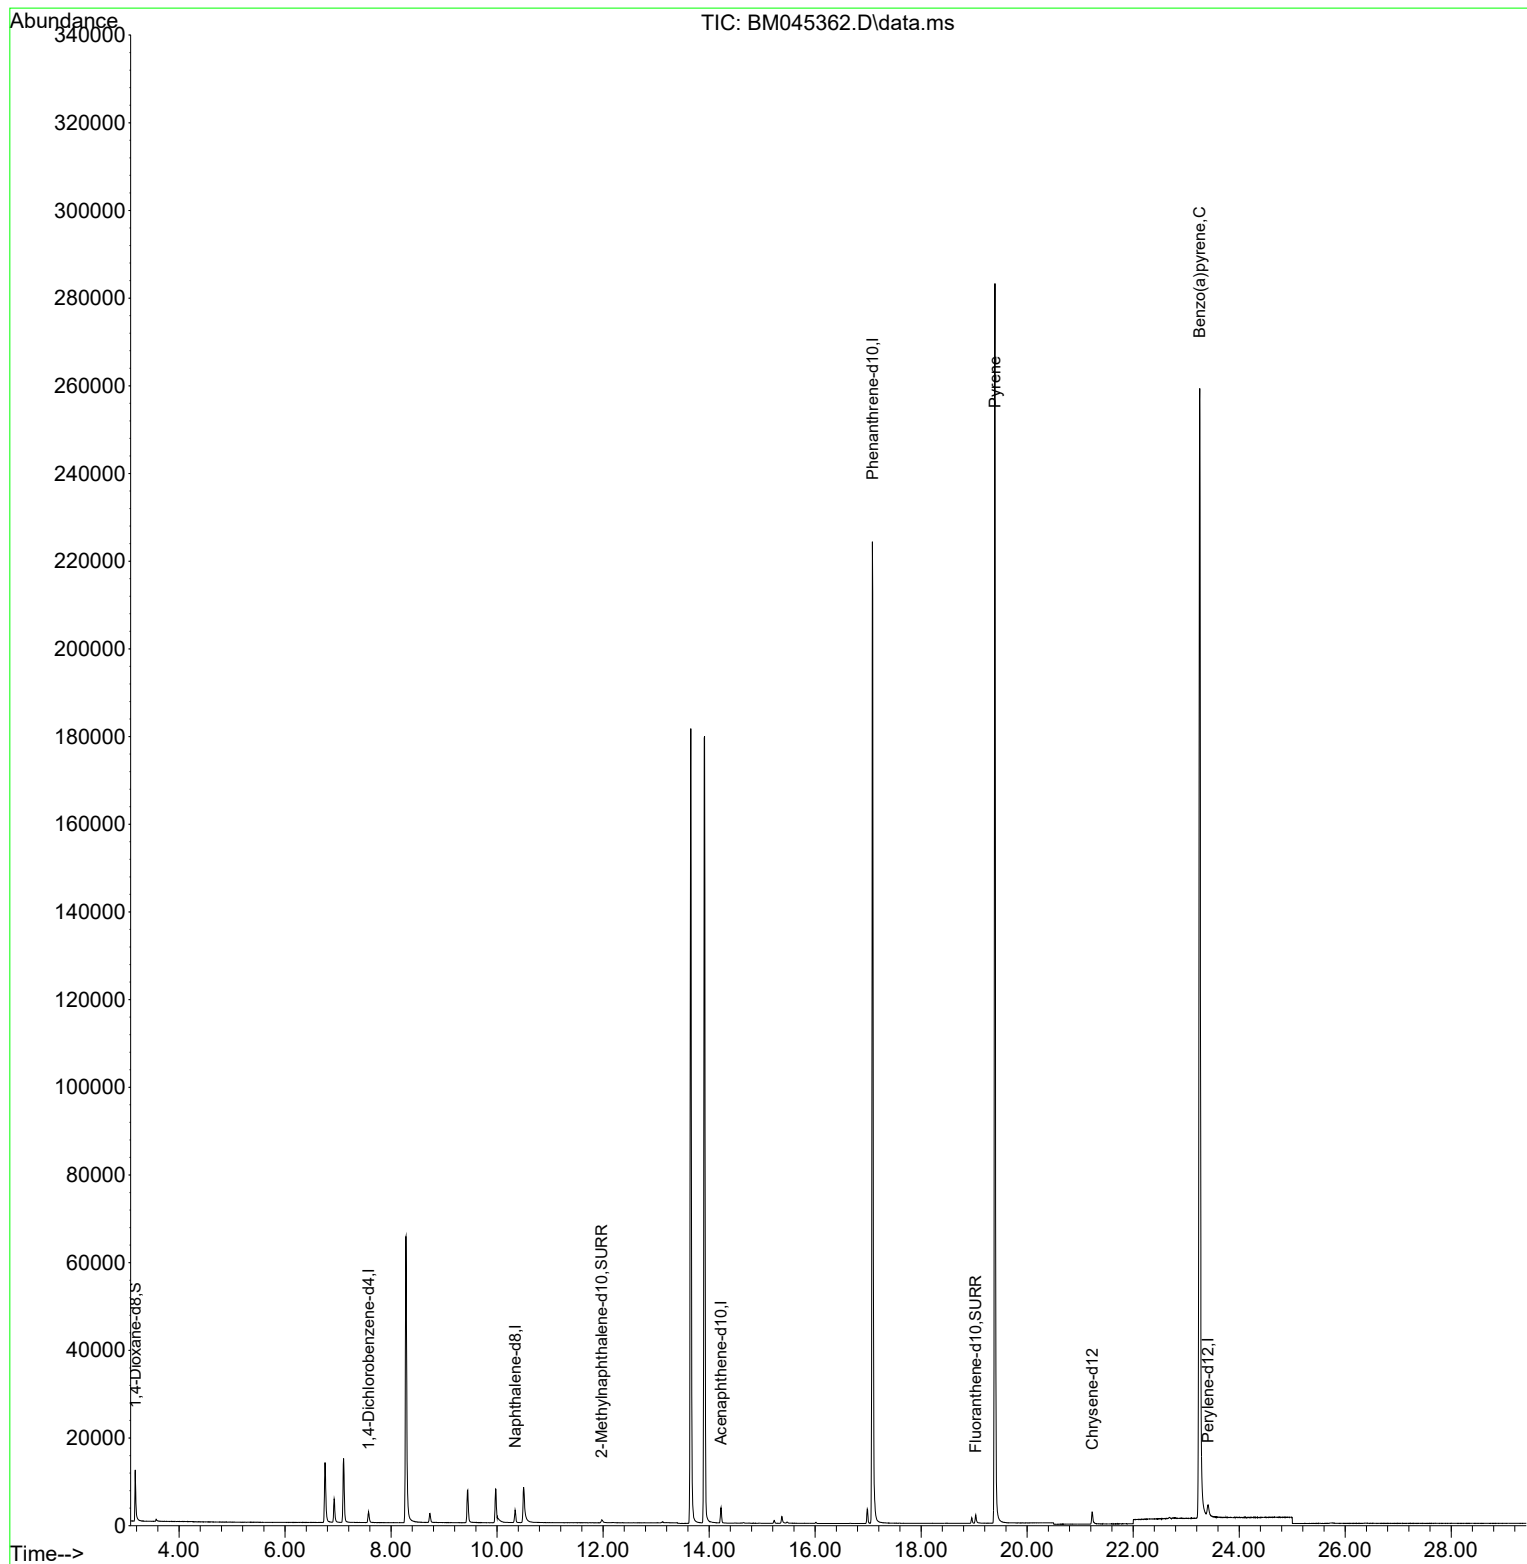

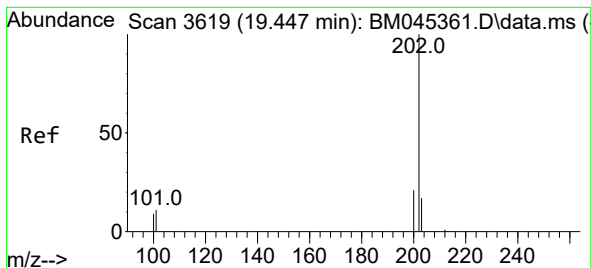

#20

Pyrene

Concen: 0.048 ng/ul

RT: 19.392 min Scan# 3

Delta R.T. -0.055 min

Lab File: BM045362.D

Acq: 18 Apr 2024 19:44

Instrument :

BNA_M

ClientSampleId :

SBLK255





Tgt Ion:202 Resp: 588

Ion Ratio Lower Upper

202 100

101 169.9 9.8 14.6#

100 1233.8 8.1 12.1#

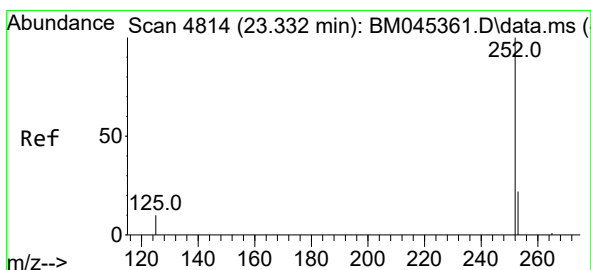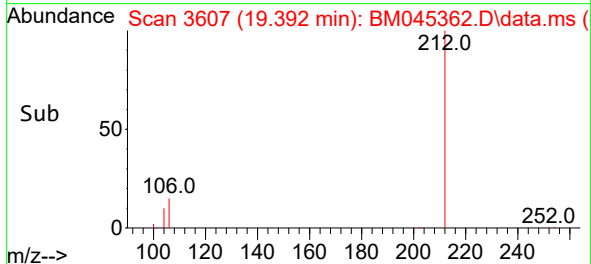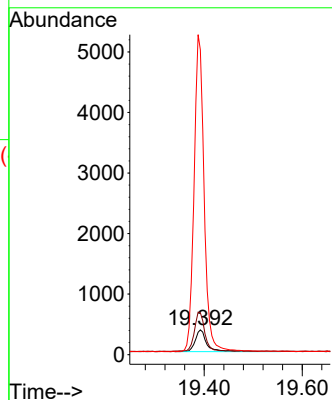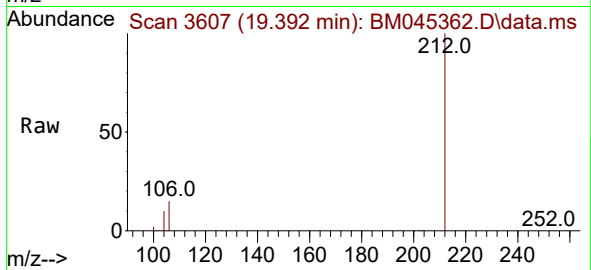

#26

Benzo(a)pyrene

Concen: 0.068 ng/ul

RT: 23.253 min Scan# 4787

Delta R.T. -0.080 min

Lab File: BM045362.D

Acq: 18 Apr 2024 19:44

Tgt Ion:252 Resp: 1428

Ion Ratio Lower Upper

252 100

253 60.0 24.6 37.0#

125 38.8 18.2 27.4#

