

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
 Data File : BM045363.D
 Acq On : 18 Apr 2024 20:20
 Operator : MA/JU
 Sample : PB160280BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK280

Quant Time: Apr 18 22:21:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 18 22:19:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.576	152	960	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.342	136	2670	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.223	164	1270	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	17.085	188	261860	0.400	ng/ul	# 0.07
17) Chrysene-d12	21.231	240	2125	0.400	ng/ul	# 0.01
23) Perylene-d12	23.414	264	4531	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	7380	5.852	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.980	152	1276	0.353	ng/ul	-0.02
18) Fluoranthene-d10	19.029	212	2392	0.445	ng/ul	-0.02
Target Compounds						
					Qvalue	
20) Pyrene	19.391	202	515	0.064	ng/ul#	1
26) Benzo(a)pyrene	23.254	252	1343	0.086	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045363.D
Acq On : 18 Apr 2024 20:20
Operator : MA/JU
Sample : PB160280BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK280

Quant Time: Apr 18 22:21:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

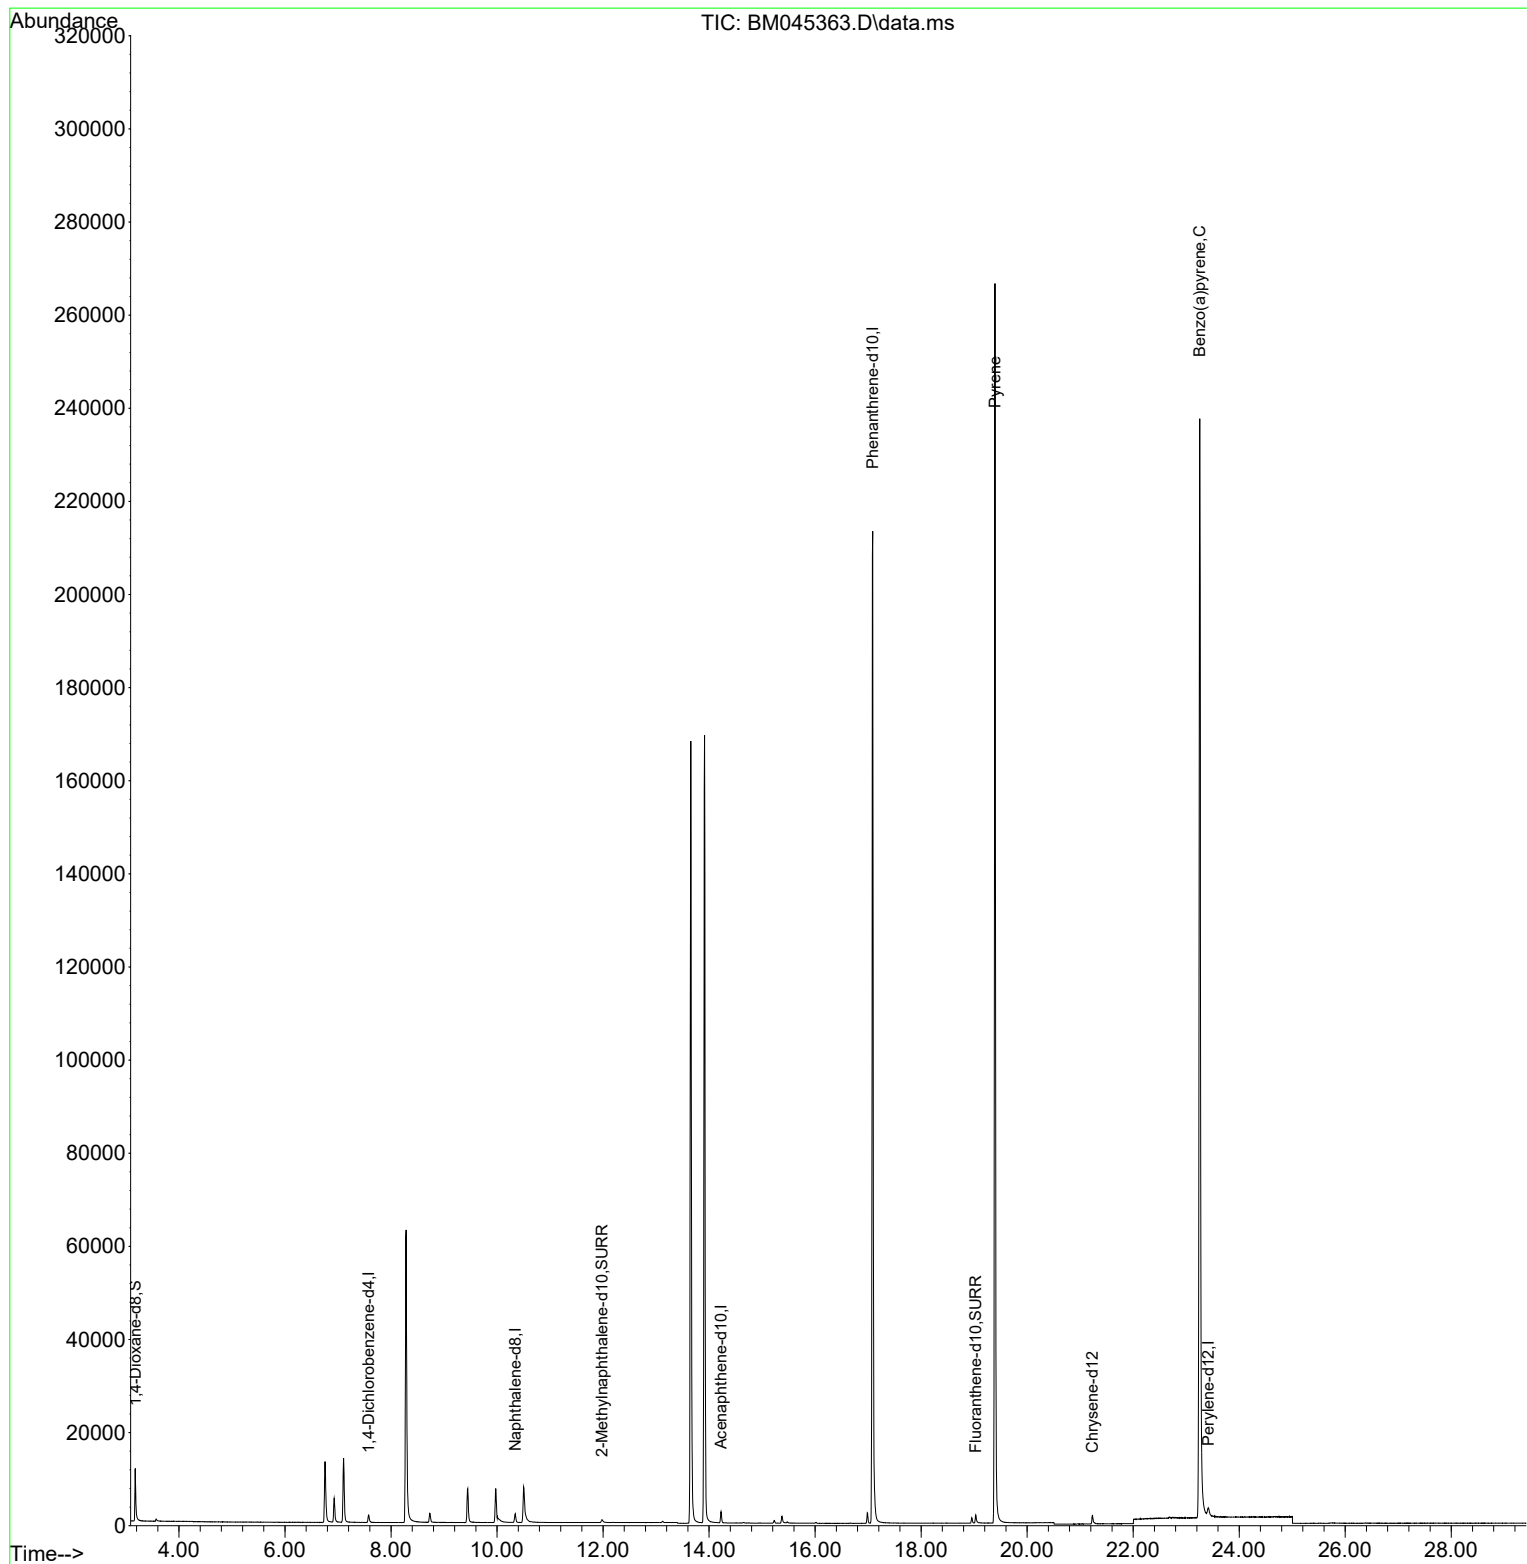

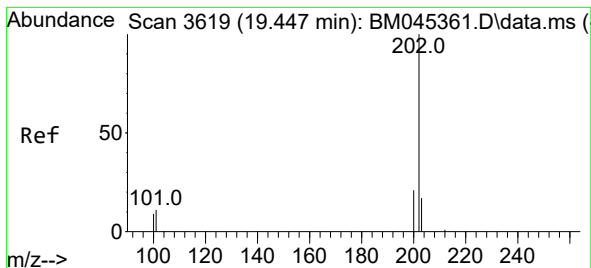

#20

Pyrene

Concen: 0.064 ng/ul

RT: 19.391 min Scan# 3

Delta R.T. -0.056 min

Lab File: BM045363.D

Acq: 18 Apr 2024 20:20

Instrument :





BNA_M

ClientSampleId :

SBLK280

Tgt Ion:202 Resp: 515

Ion	Ratio	Lower	Upper
202	100		
101	165.5	9.8	14.6#
100	1221.4	8.1	12.1#

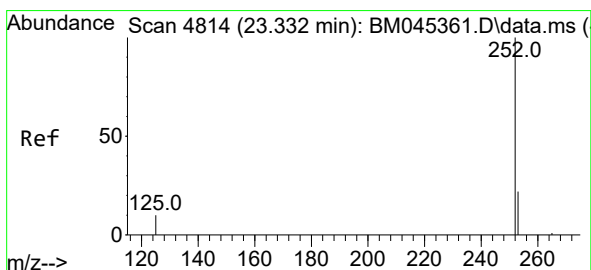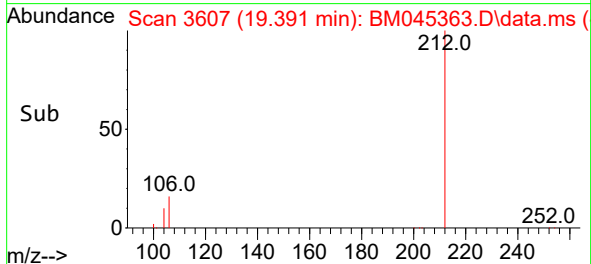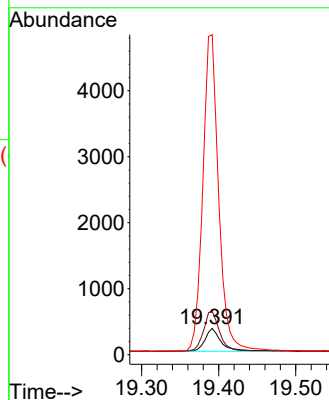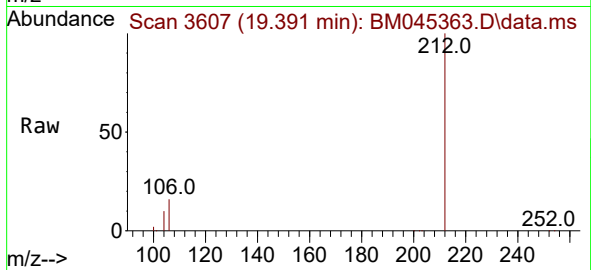

#26

Benzo(a)pyrene

Concen: 0.086 ng/ul

RT: 23.254 min Scan# 4787

Delta R.T. -0.079 min

Lab File: BM045363.D

Acq: 18 Apr 2024 20:20

Tgt Ion:252 Resp: 1343

Ion	Ratio	Lower	Upper
252	100		
253	62.8	24.6	37.0#
125	40.5	18.2	27.4#

