

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
 Data File : BM045397.D
 Acq On : 19 Apr 2024 18:19
 Operator : MA/JU
 Sample : P2032-06
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MF2

Quant Time: Apr 19 23:09:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 18 22:19:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.576	152	929	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.336	136	2730	0.400	ng/ul	#-0.05
9) Acenaphthene-d10	14.220	164	1319	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.078	188	310408	0.400	ng/ul	0.06
17) Chrysene-d12	21.222	240	2671	0.400	ng/ul	0.00
23) Perylene-d12	23.408	264	4964	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	4261	3.492	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.969	152	1338	0.362	ng/ul	-0.03
18) Fluoranthene-d10	19.025	212	3121	0.462	ng/ul	-0.03
Target Compounds						Qvalue
2) 1,4-Dioxane	3.188	88	54	0.046	ng/ul#	79
20) Pyrene	19.388	202	695	0.069	ng/ul#	1
26) Benzo(a)pyrene	23.250	252	1770	0.103	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045397.D
Acq On : 19 Apr 2024 18:19
Operator : MA/JU
Sample : P2032-06
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MF2

Quant Time: Apr 19 23:09:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration




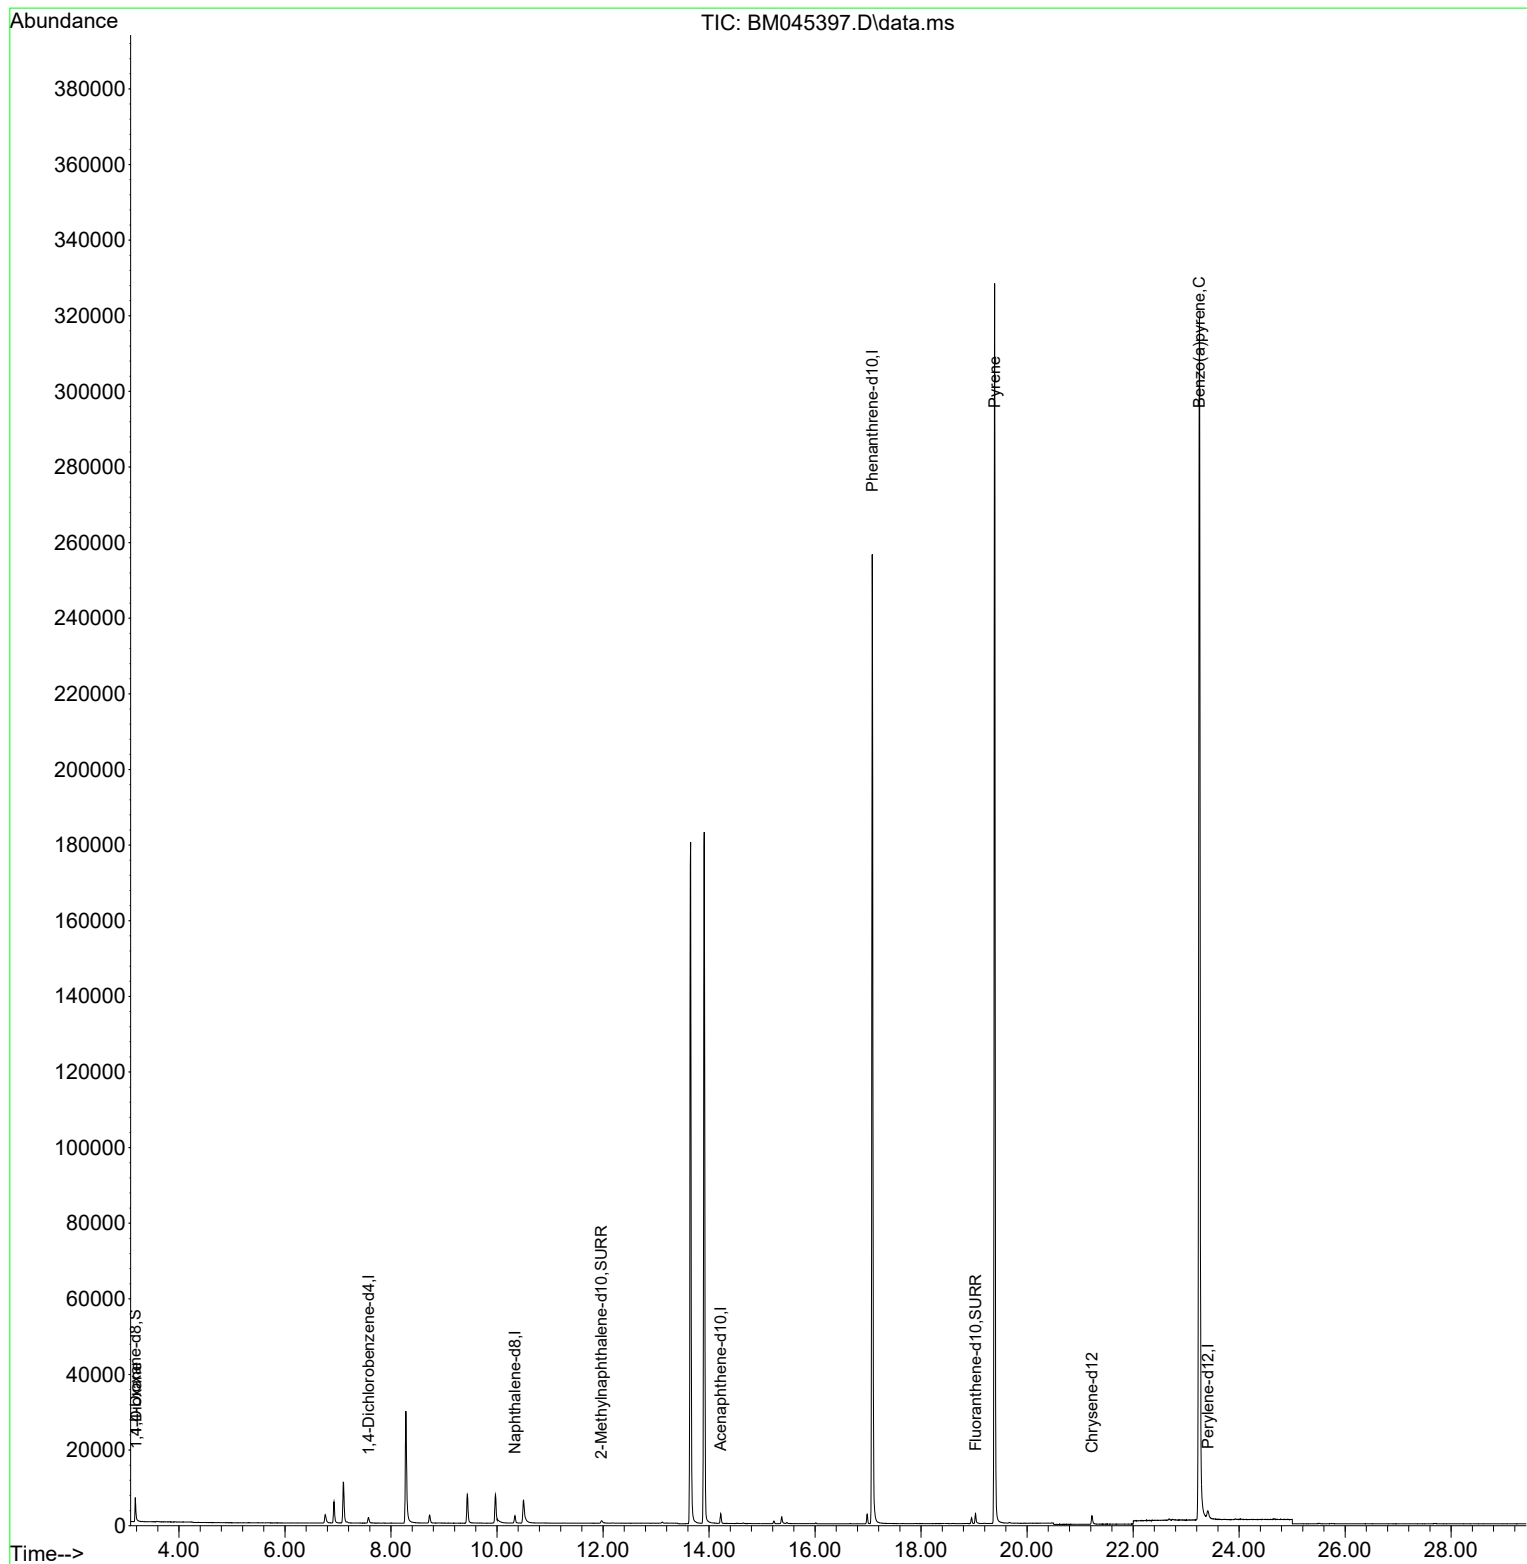


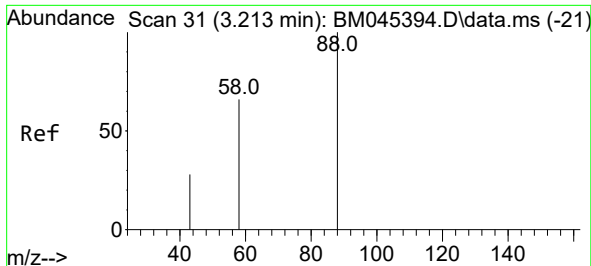

#2
1,4-Dioxane
Concen: 0.046 ng/ul
RT: 3.188 min Scan# 21
Delta R.T. -0.025 min
Lab File: BM045397.D
Acq: 19 Apr 2024 18:19




Instrument :
BNA_M
ClientSampleId :
EOMF2


Tgt Ion: 88 Resp: 54
Ion Ratio Lower Upper
88 100
43 49.5 30.6 46.0#
58 26.4 32.6 48.8#

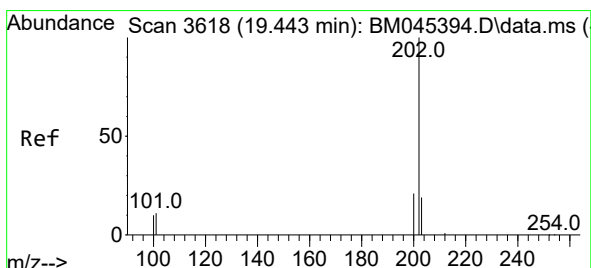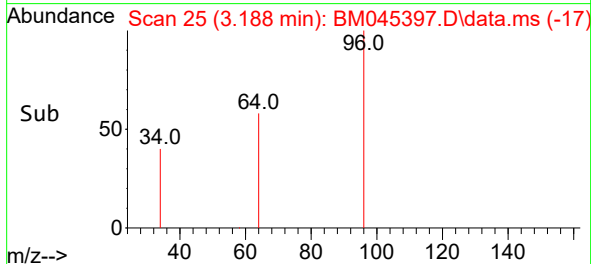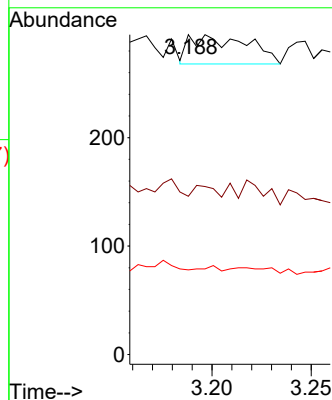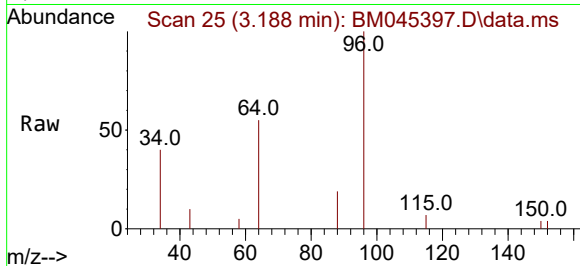

#20
Pyrene
Concen: 0.069 ng/ul
RT: 19.388 min Scan# 3606
Delta R.T. -0.060 min
Lab File: BM045397.D
Acq: 19 Apr 2024 18:19


Tgt Ion: 202 Resp: 695
Ion Ratio Lower Upper
202 100
101 181.8 9.8 14.6#
100 1337.0 8.1 12.1#

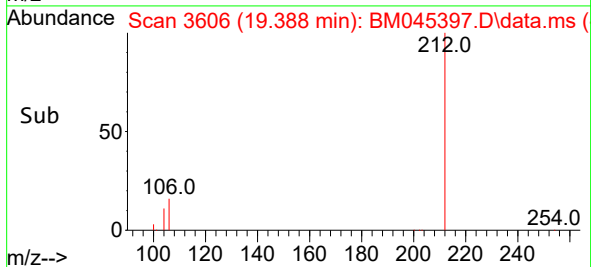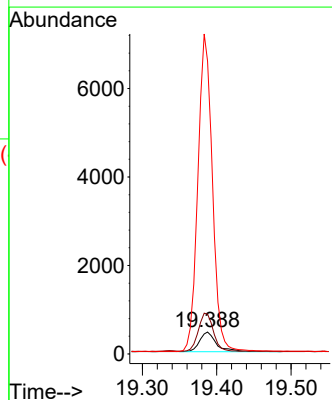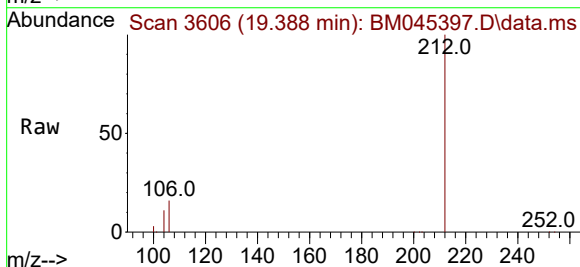

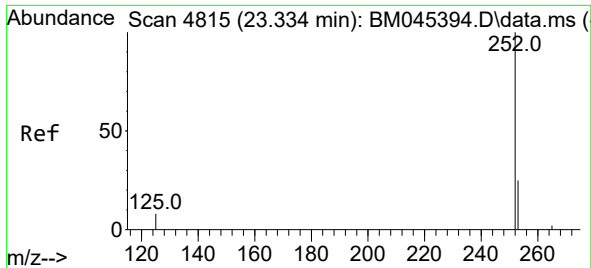

#26
Benzo(a)pyrene
Concen: 0.103 ng/ul
RT: 23.250 min Scan# 41
Delta R.T. -0.083 min
Lab File: BM045397.D
Acq: 19 Apr 2024 18:19

Instrument :
BNA_M
ClientSampleId :
E0MF2

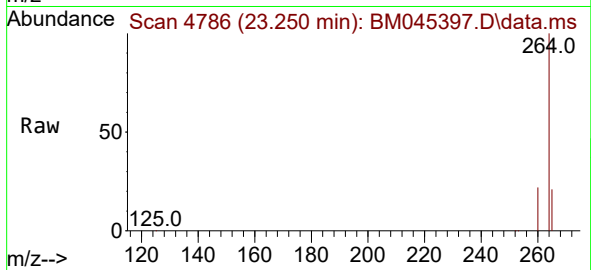

Tgt Ion:252 Resp: 1770
Ion Ratio Lower Upper
252 100
253 51.7 24.6 37.0#
125 42.5 18.2 27.4#

