

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
 Data File : BM045398.D
 Acq On : 19 Apr 2024 18:56
 Operator : MA/JU
 Sample : P2032-07
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MF3

Quant Time: Apr 19 23:09:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 18 22:19:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.572	152	977	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.336	136	2806	0.400	ng/ul	#-0.05
9) Acenaphthene-d10	14.219	164	1380	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	17.077	188	269585	0.400	ng/ul	0.06
17) Chrysene-d12	21.222	240	2309	0.400	ng/ul	# 0.00
23) Perylene-d12	23.408	264	4375	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	4574	3.564	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.975	152	1196	0.314	ng/ul	-0.02
18) Fluoranthene-d10	19.029	212	2554	0.438	ng/ul	-0.02
Target Compounds						Qvalue
20) Pyrene	19.387	202	531	0.061	ng/ul#	1
26) Benzo(a)pyrene	23.245	252	1346	0.089	ng/ul#	56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045398.D
Acq On : 19 Apr 2024 18:56
Operator : MA/JU
Sample : P2032-07
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MF3

Quant Time: Apr 19 23:09:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

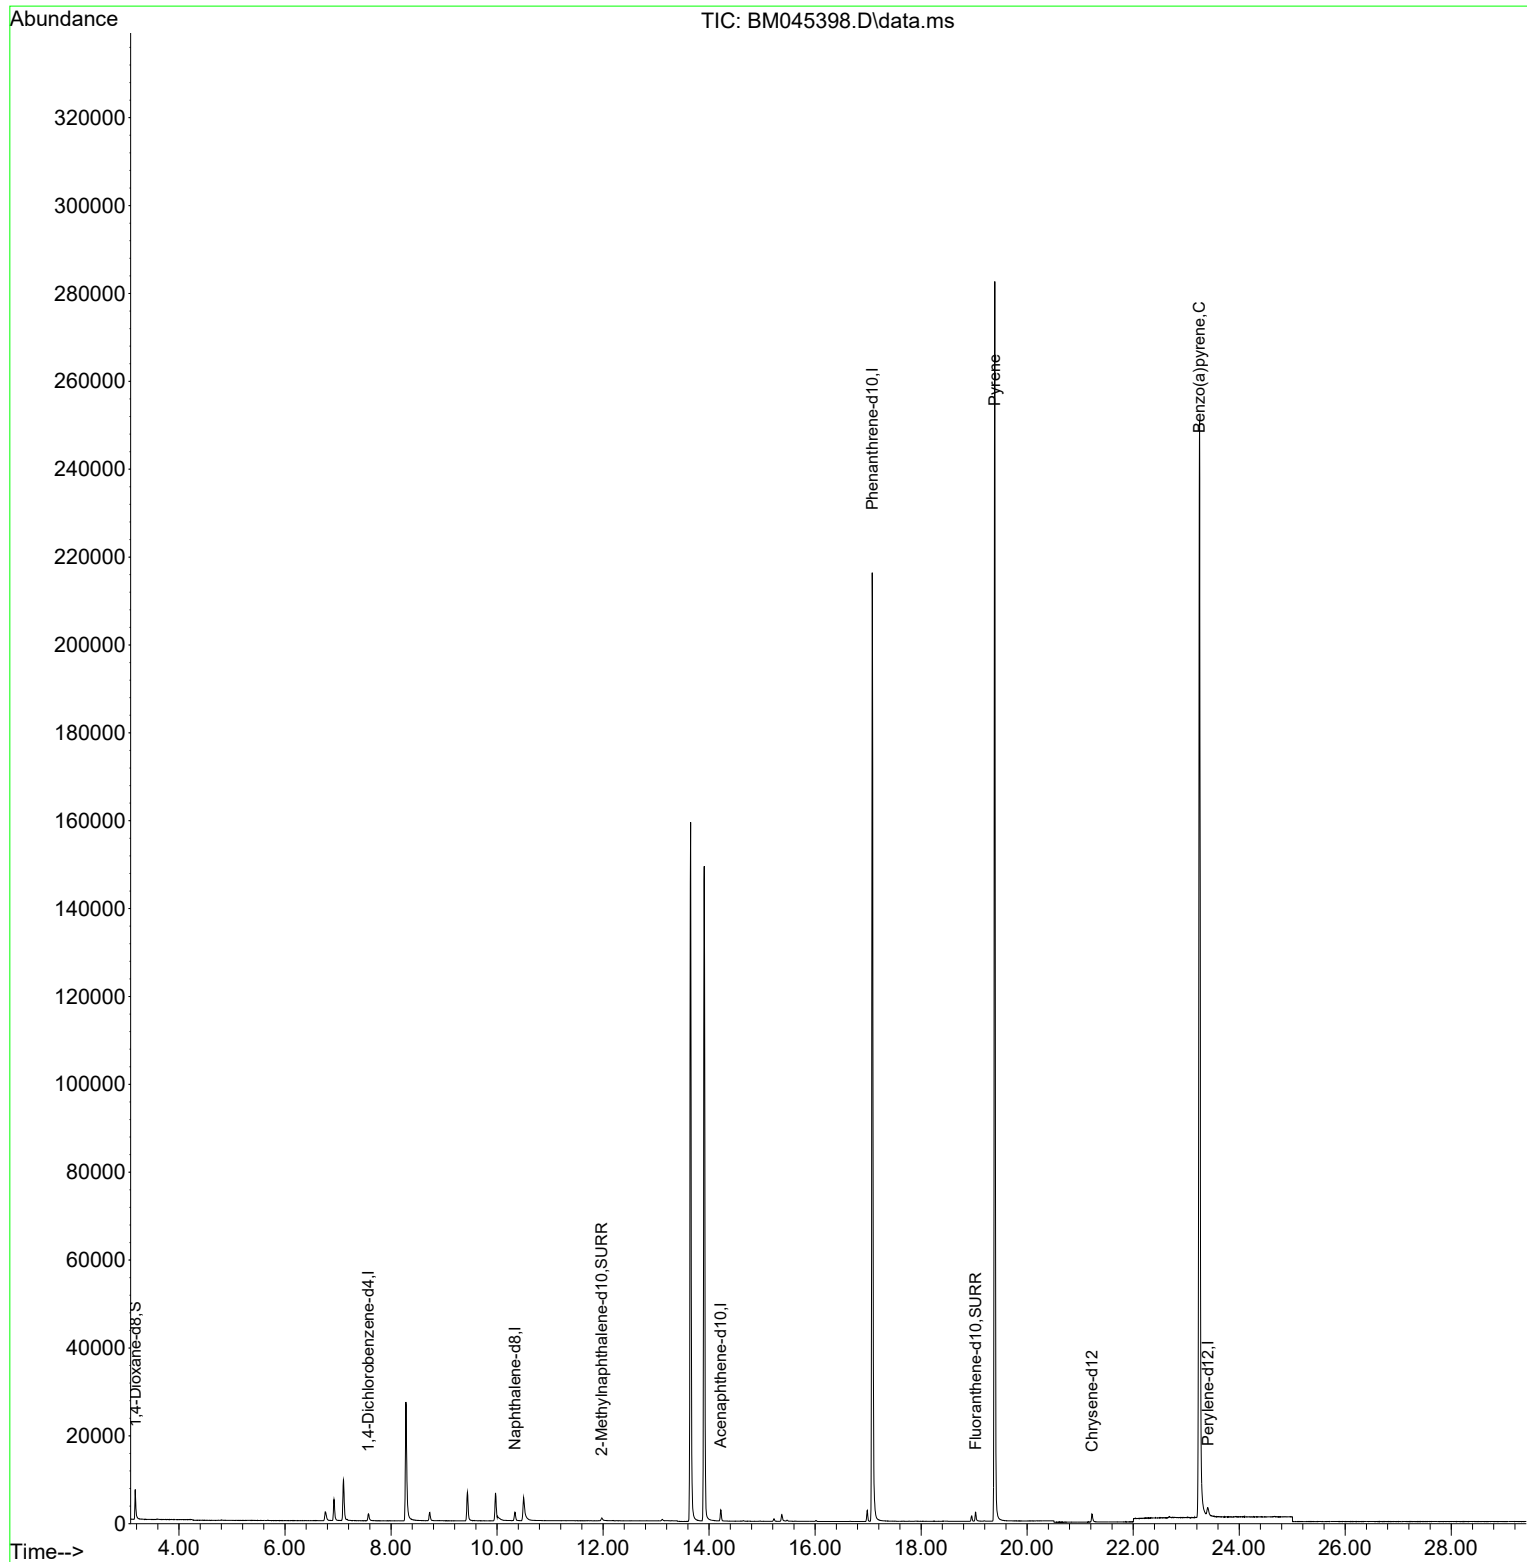

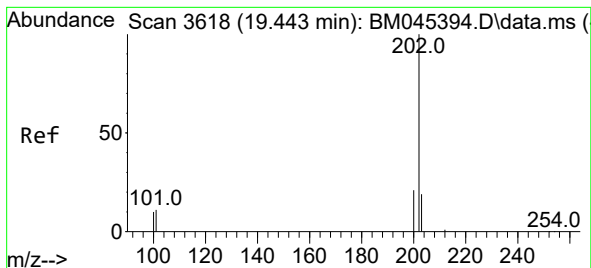

#20

Pyrene

Concen: 0.061 ng/ul

RT: 19.387 min Scan# 3

Delta R.T. -0.060 min

Lab File: BM045398.D

Acq: 19 Apr 2024 18:56

Instrument :

BNA_M

ClientSampleId :

EOMF3





Tgt Ion:202 Resp: 531

Ion Ratio Lower Upper

202 100

101 184.5 9.8 14.6#

100 1442.1 8.1 12.1#

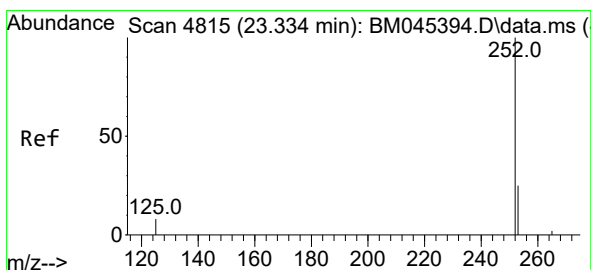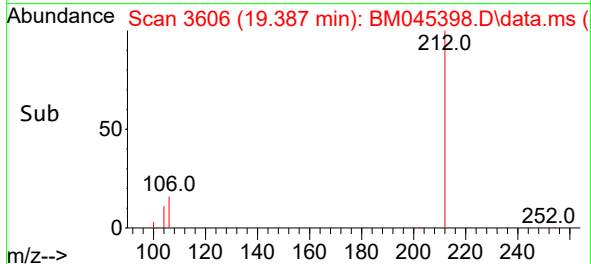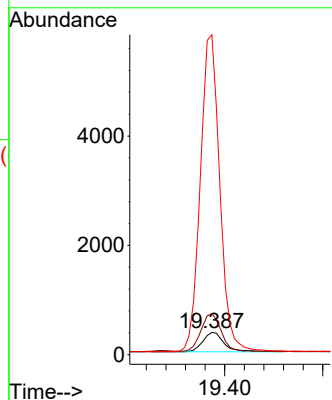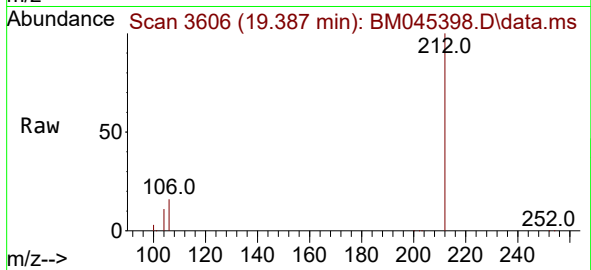

#26

Benzo(a)pyrene

Concen: 0.089 ng/ul

RT: 23.245 min Scan# 4784

Delta R.T. -0.088 min

Lab File: BM045398.D

Acq: 19 Apr 2024 18:56

Tgt Ion:252 Resp: 1346

Ion Ratio Lower Upper

252 100

253 56.0 24.6 37.0#

125 42.6 18.2 27.4#

