

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
 Data File : BM045399.D
 Acq On : 19 Apr 2024 19:32
 Operator : MA/JU
 Sample : P2032-10
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MF6

Quant Time: Apr 19 23:09:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 18 22:19:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.572	152	1001	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.336	136	2879	0.400	ng/ul	-0.05
9) Acenaphthene-d10	14.220	164	1372	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.078	188	300339	0.400	ng/ul	# 0.06
17) Chrysene-d12	21.221	240	2329	0.400	ng/ul	# 0.00
23) Perylene-d12	23.408	264	4721	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	4665	3.548	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.969	152	1383	0.354	ng/ul	-0.03
18) Fluoranthene-d10	19.025	212	3027	0.514	ng/ul	-0.03
Target Compounds						
					Qvalue	
20) Pyrene	19.388	202	597	0.068	ng/ul#	1
26) Benzo(a)pyrene	23.247	252	1571	0.097	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045399.D
Acq On : 19 Apr 2024 19:32
Operator : MA/JU
Sample : P2032-10
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOMF6

Quant Time: Apr 19 23:09:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

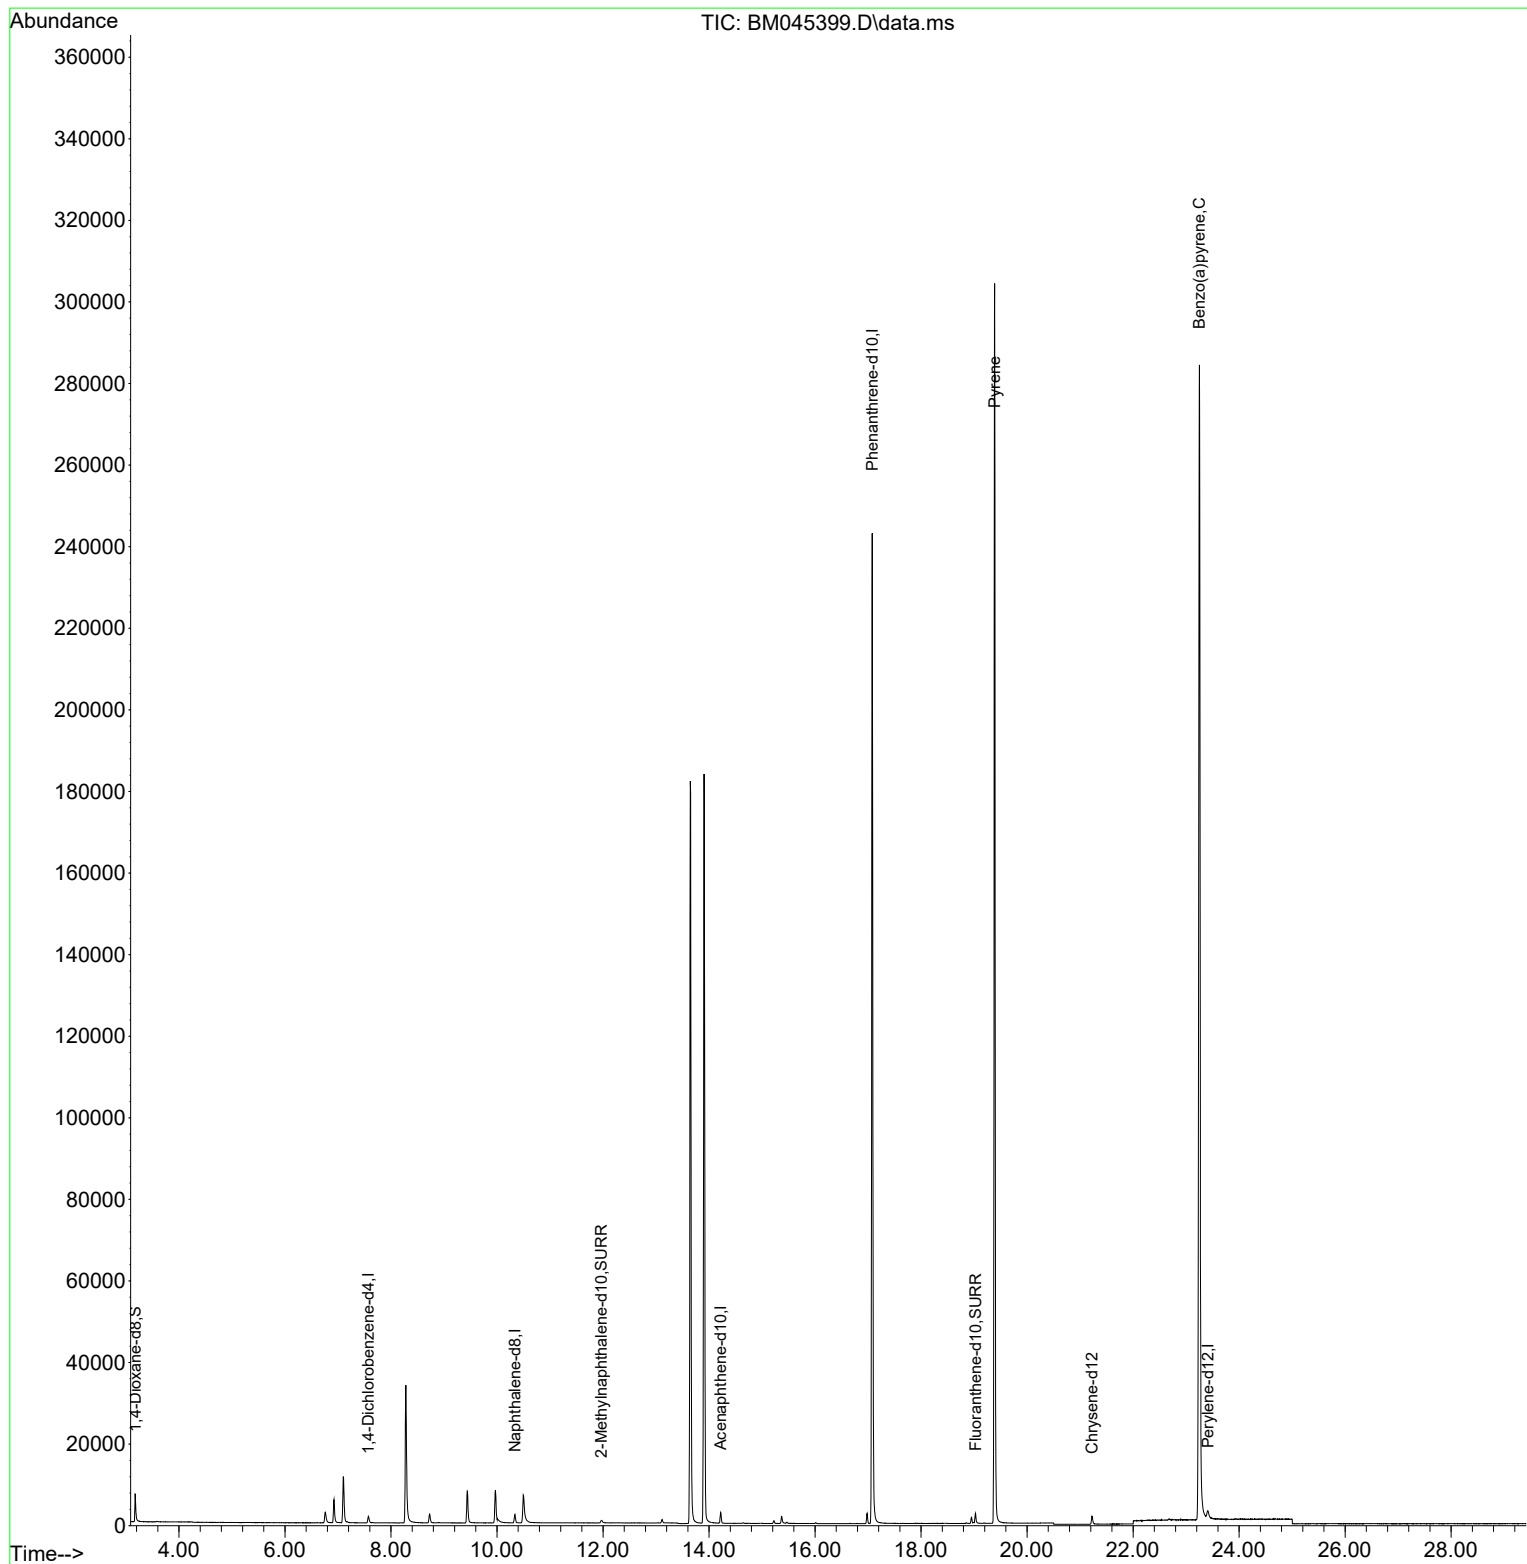

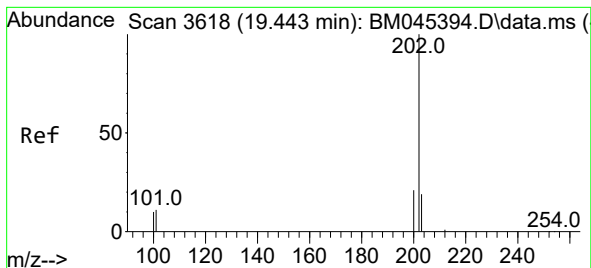

#20

Pyrene

Concen: 0.068 ng/ul

RT: 19.388 min Scan# 3

Delta R.T. -0.060 min

Lab File: BM045399.D

Acq: 19 Apr 2024 19:32

Instrument :





BNA_M

ClientSampleId :

EOMF6

Tgt Ion:202 Resp: 597

Ion	Ratio	Lower	Upper
202	100		
101	188.9	9.8	14.6#
100	1360.8	8.1	12.1#

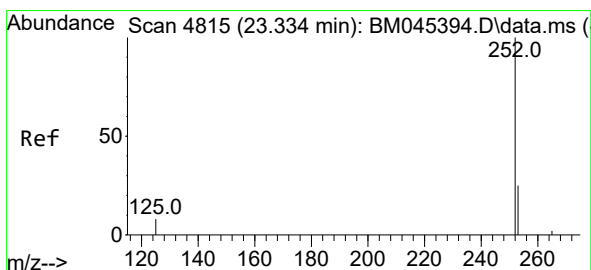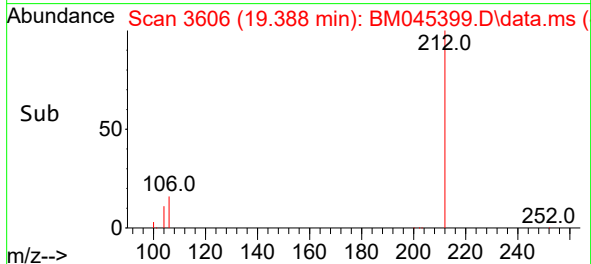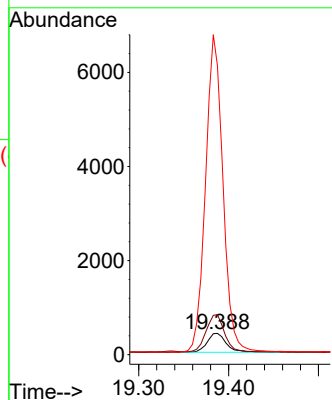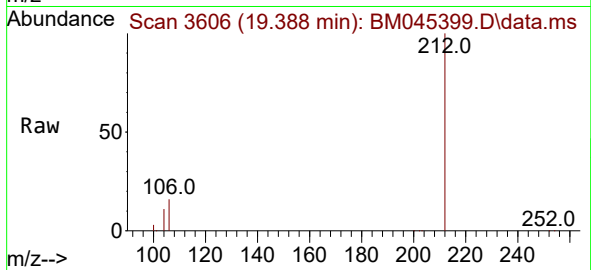

#26

Benzo(a)pyrene

Concen: 0.097 ng/ul

RT: 23.247 min Scan# 4785

Delta R.T. -0.086 min

Lab File: BM045399.D

Acq: 19 Apr 2024 19:32

Tgt Ion:252 Resp: 1571

Ion	Ratio	Lower	Upper
252	100		
253	54.9	24.6	37.0#
125	40.5	18.2	27.4#

