

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN031019.D
 Acq On : 18 Apr 2024 21:53
 Operator : MA/JU
 Sample : P2037-14
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Apr 18 22:44:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 17 22:24:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	102645	20.000	ng/ul	0.00
20) Naphthalene-d8	10.416	136	473365	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.281	164	339332	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.034	188	777246	20.000	ng/ul	0.00
79) Chrysene-d12	21.263	240	837607	20.000	ng/ul	-0.01
88) Perylene-d12	24.163	264	1029753	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	8127	3.712	ng/uL	0.00
4) Pyridine-d5	3.564	84	35701	5.439	ng/ul	0.00
7) Phenol-d5	6.817	99	3001	0.361	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.981	67	113616	22.153	ng/ul	0.00
11) 2-Chlorophenol-d4	7.169	132	8080	1.283	ng/ul	0.00
15) 4-Methylphenol-d8	8.346	113	10011	1.439	ng/ul	0.00
21) Nitrobenzene-d5	8.793	128	69011	21.016	ng/ul	0.00
24) 2-Nitrophenol-d4	9.511	143	64669	21.528	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.046	165	4267	0.649	ng/ul	0.00
31) 4-Chloroaniline-d4	10.563	131	18418	1.701	ng/ul	0.00
46) Dimethylphthalate-d6	13.699	166	579400	25.574	ng/ul	0.00
49) Acenaphthylene-d8	13.975	160	12326	0.473	ng/ul	0.00
54) 4-Nitrophenol-d4	14.504	143	11355	2.620	ng/ul	0.00
60) Fluorene-d10	15.281	176	229670	11.585	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.398	200	38590	11.248	ng/ul	-0.01
73) Anthracene-d10	17.128	188	25621	0.765	ng/ul	0.00
81) Pyrene-d10	19.428	212	6173	0.137	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.963	264	3372	0.071	ng/ul	-0.01
Target Compounds						
55) 4-Nitrophenol	14.510	109	30994	9.027	ng/ul#	2


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031019.D
Acq On : 18 Apr 2024 21:53
Operator : MA/JU
Sample : P2037-14
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Apr 18 22:44:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 17 22:24:16 2024
Response via : Initial Calibration

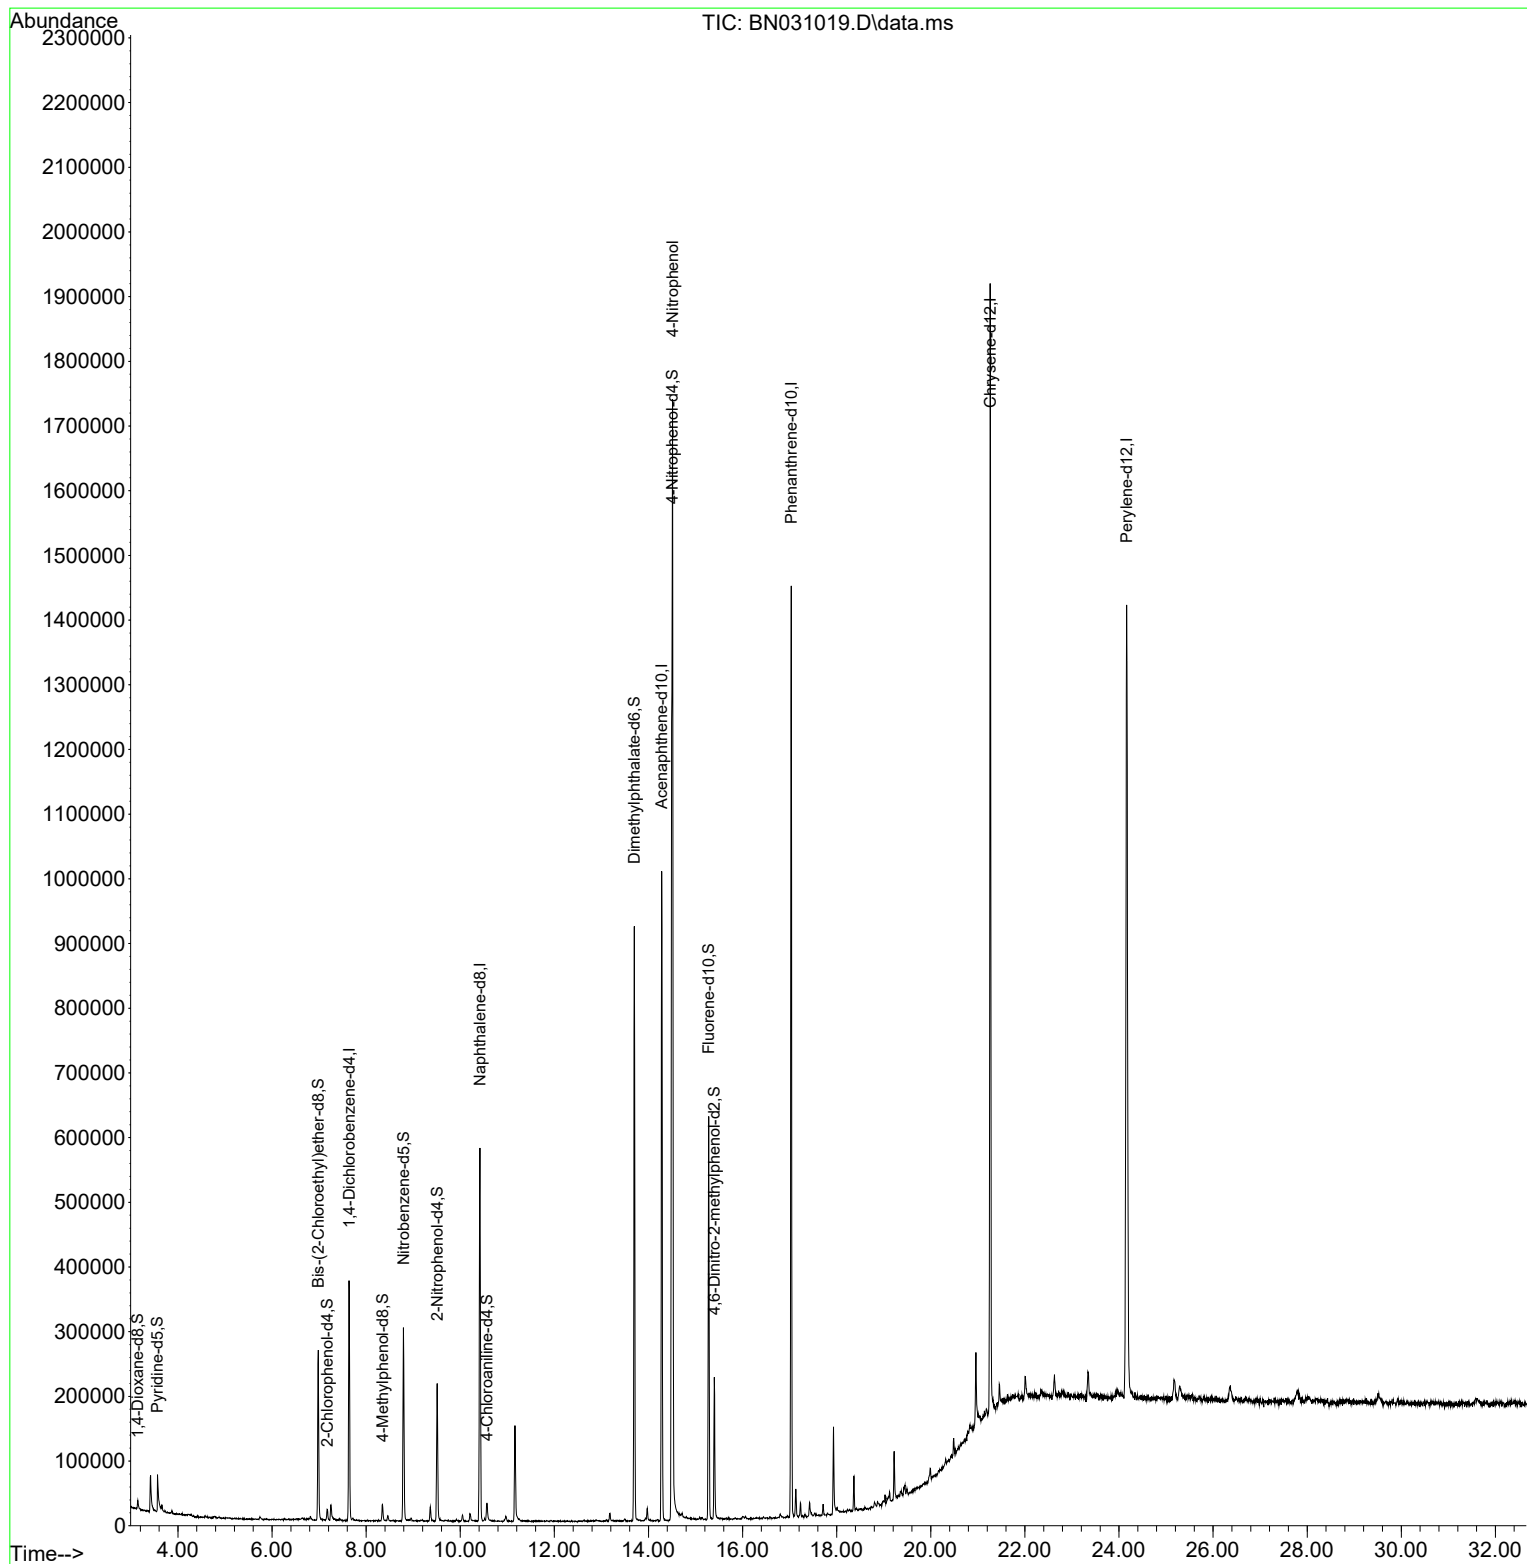

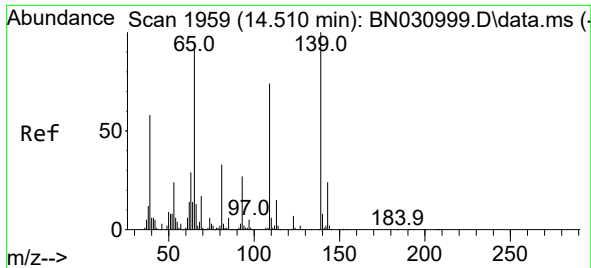

#55
 4-Nitrophenol
 Concen: 9.027 ng/ul
 RT: 14.510 min Scan# 14
 Delta R.T. 0.000 min
 Lab File: BN031019.D
 Acq: 18 Apr 2024 21:53

Instrument :
 BNA_M
 ClientSampleId :

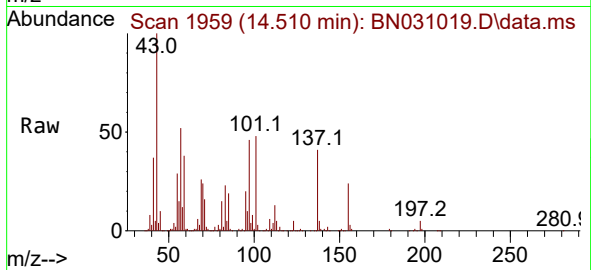

Tgt Ion:109 Resp: 30994
 Ion Ratio Lower Upper
 109 100
 139 12.3 111.8 167.6#
 65 22.4 98.7 148.1#

