




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
 Data File : BM045369.D
 Acq On : 18 Apr 2024 23:58
 Operator : MA/JU
 Sample : P2077-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:31:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 18 22:19:59 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/19/2024
 Supervised By :mohammad ahmed 04/22/2024

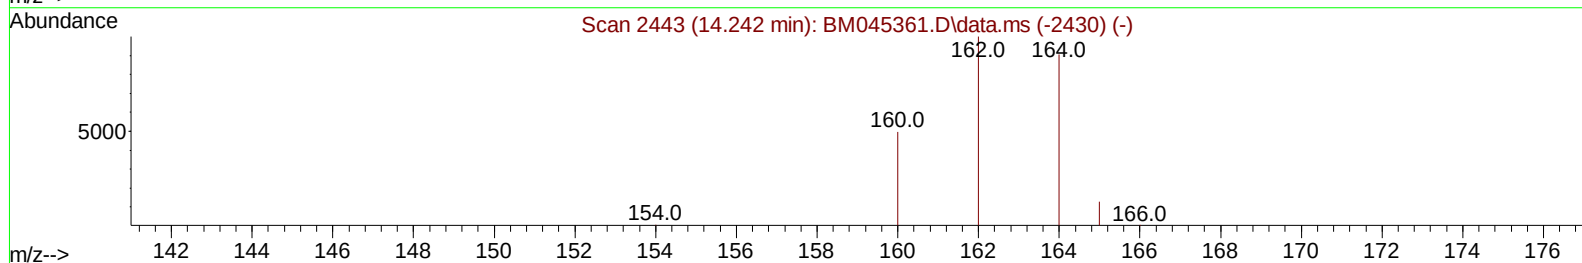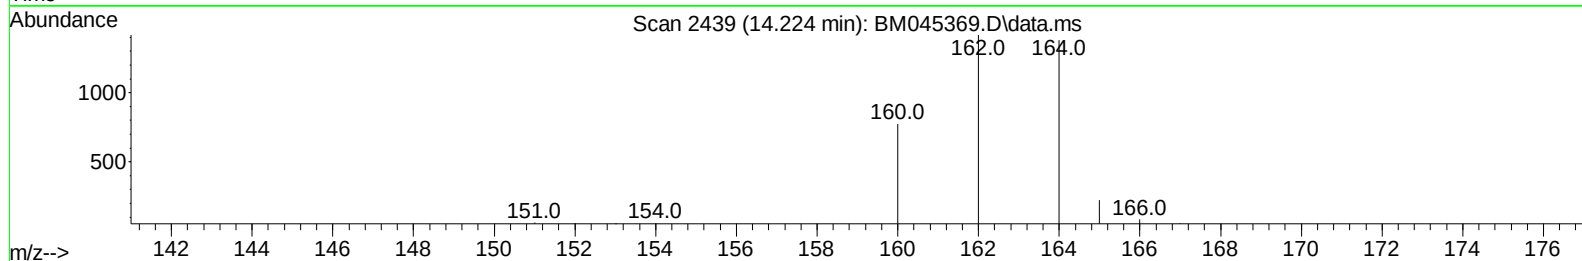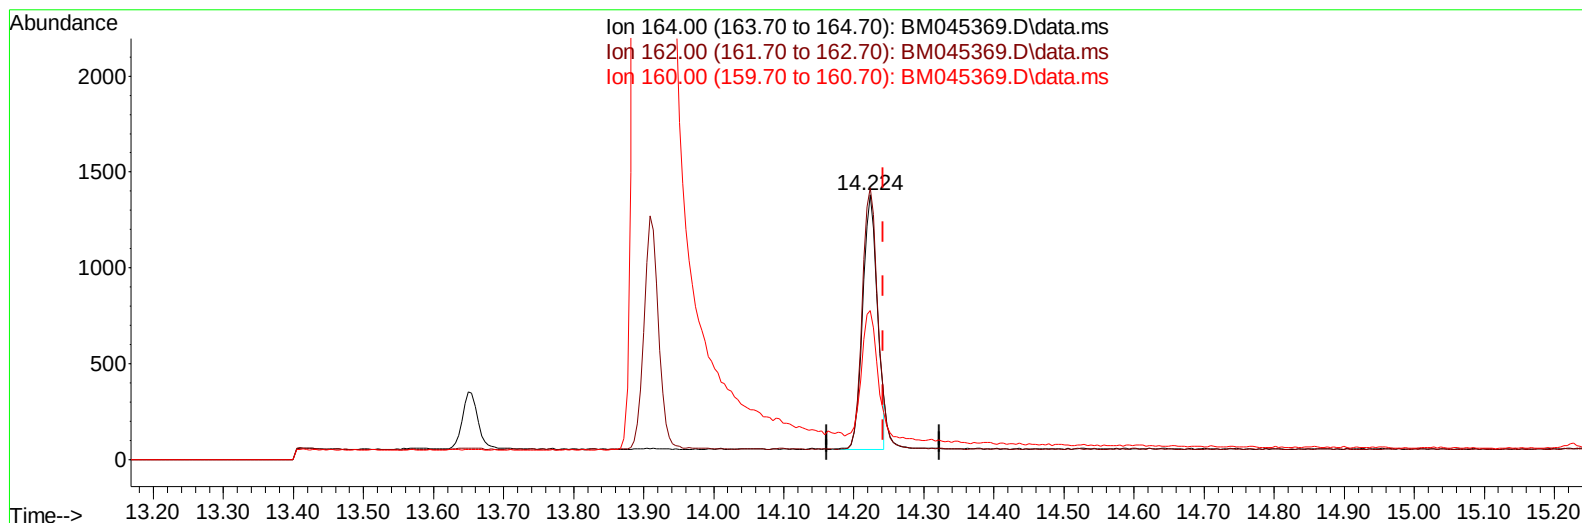

TIC: BM045369.D\data.ms

(9) Acenaphthene-d10 (I)

14.224min (-0.018) 0.40 ng/u1

response 1933

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	103.00	102.61
160.00	50.00	56.12
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045369.D
Acq On : 18 Apr 2024 23:58
Operator : MA/JU
Sample : P2077-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF6

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:31:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/22/2024

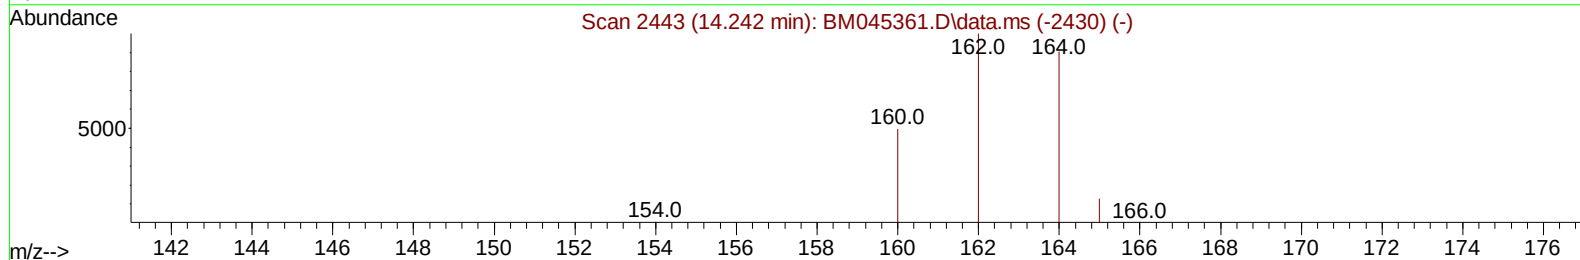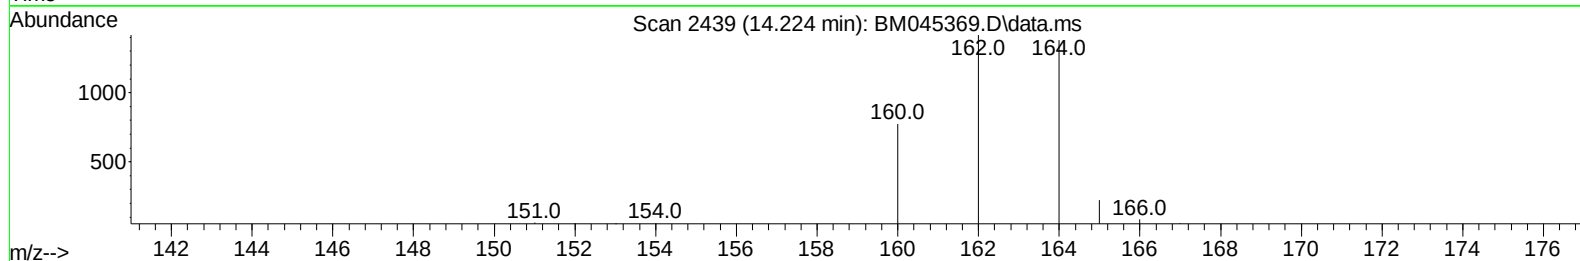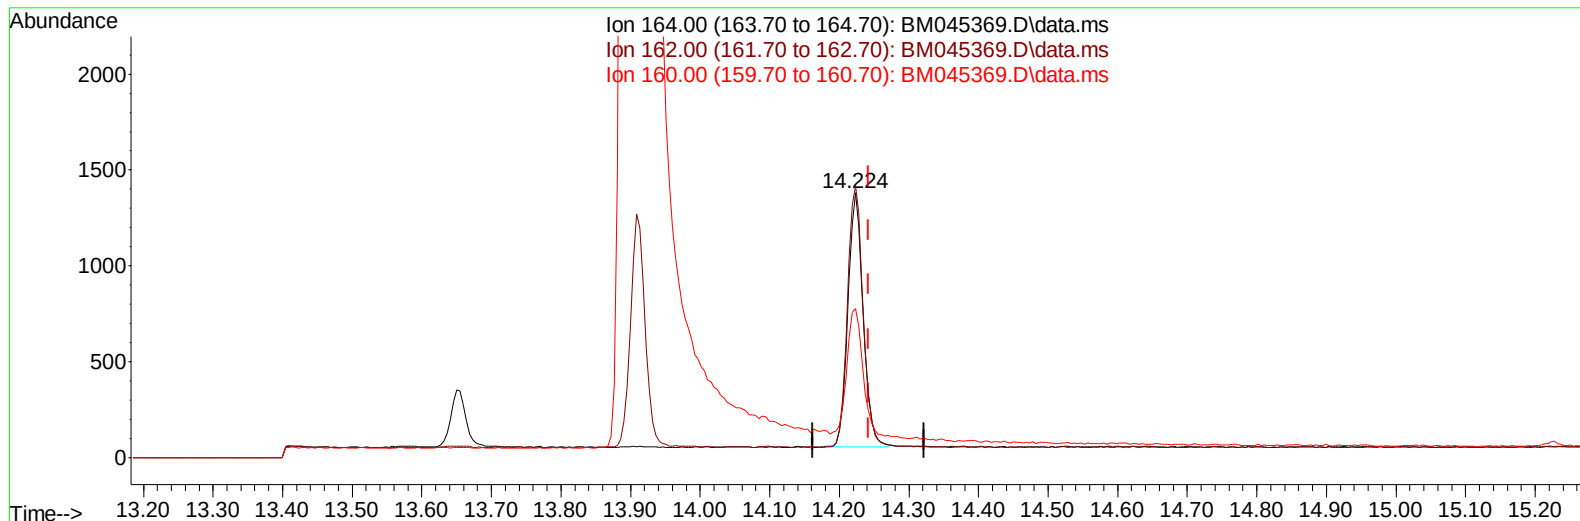

TIC: BM045369.D\data.ms

(9) Acenaphthene-d10 (I)

14.224min (-0.018) 0.40 ng/ul m

response 2003

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	103.00	102.61
160.00	50.00	56.12
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045369.D
Acq On : 18 Apr 2024 23:58
Operator : MA/JU
Sample : P2077-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF6

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:31:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/22/2024

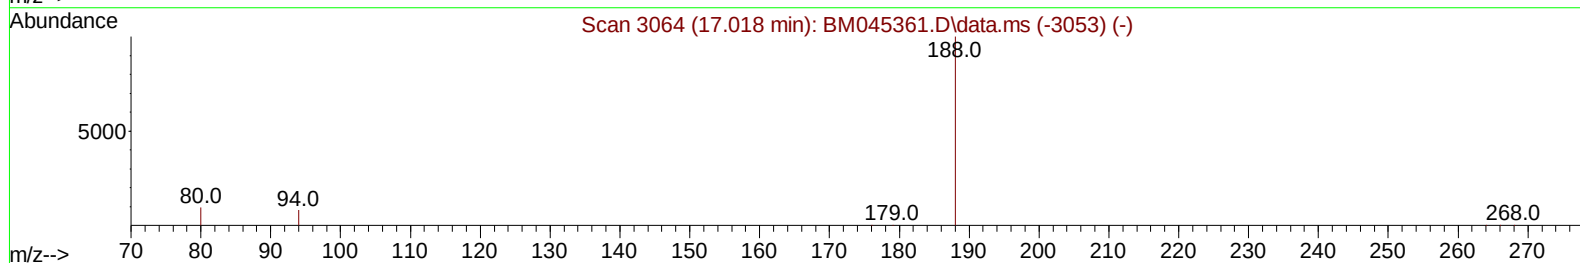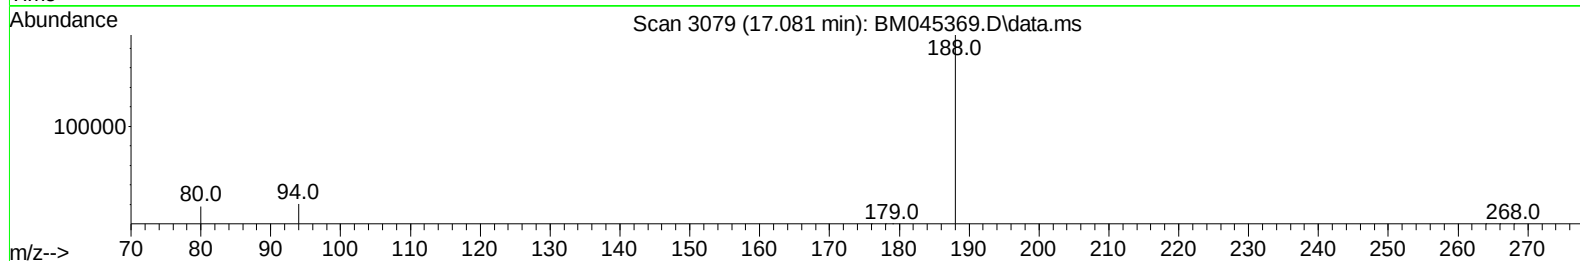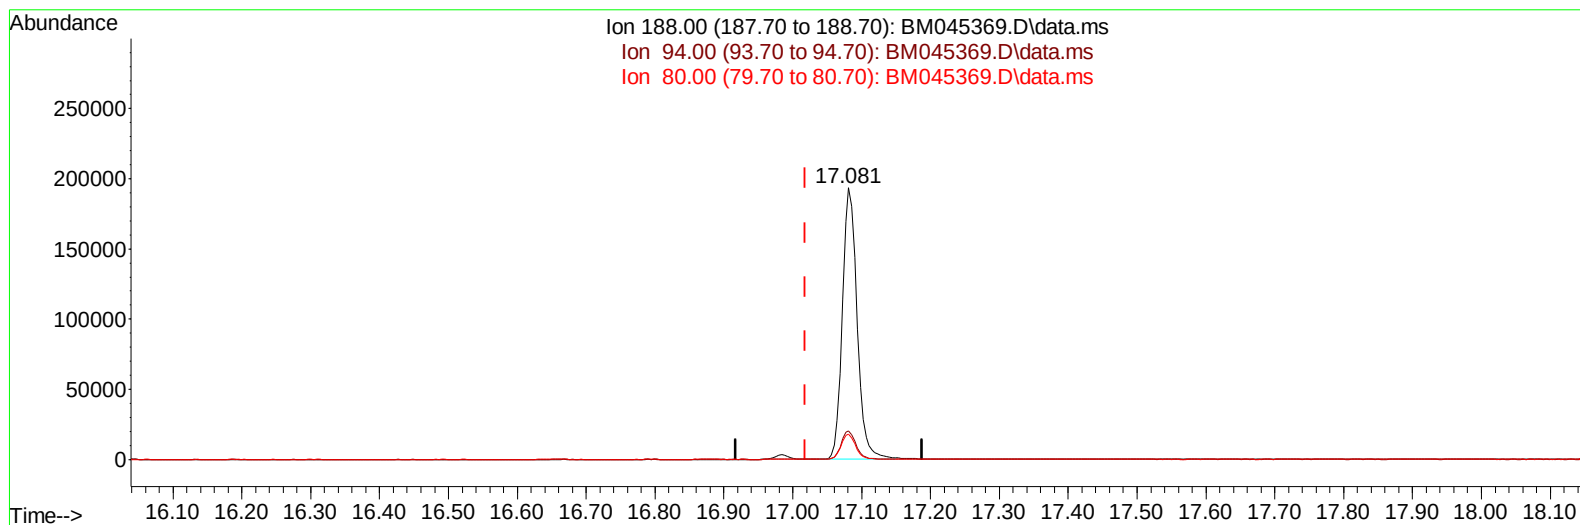

TIC: BM045369.D\data.ms

(13) Phenanthrene-d10 (I)

17.081min (+ 0.063) 0.40 ng/u1

response 285858

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.00	10.61
80.00	11.80	9.26#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045369.D
Acq On : 18 Apr 2024 23:58
Operator : MA/JU
Sample : P2077-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF6

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:31:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/22/2024

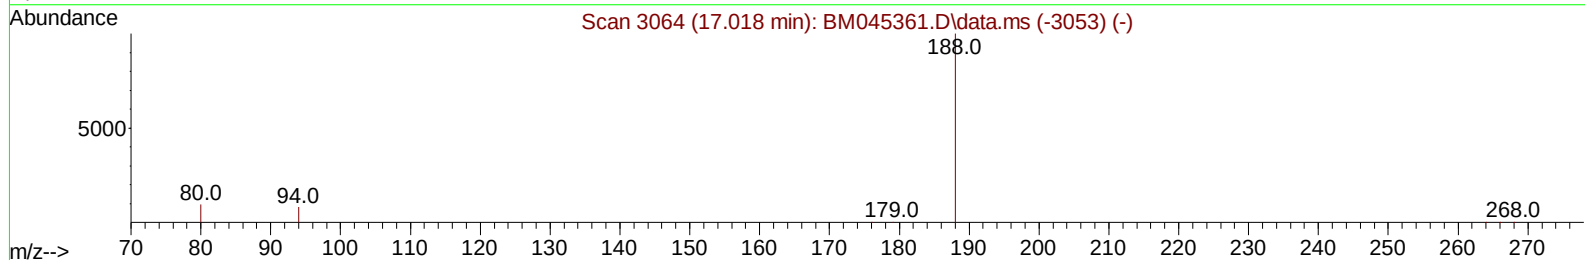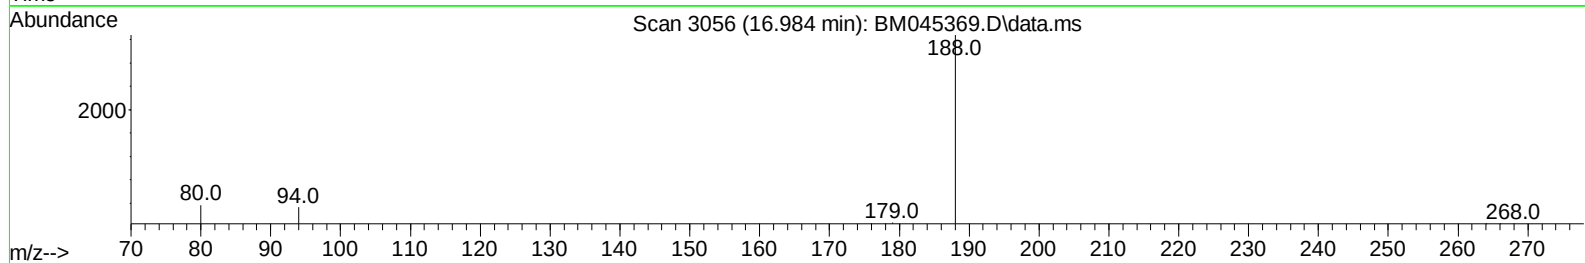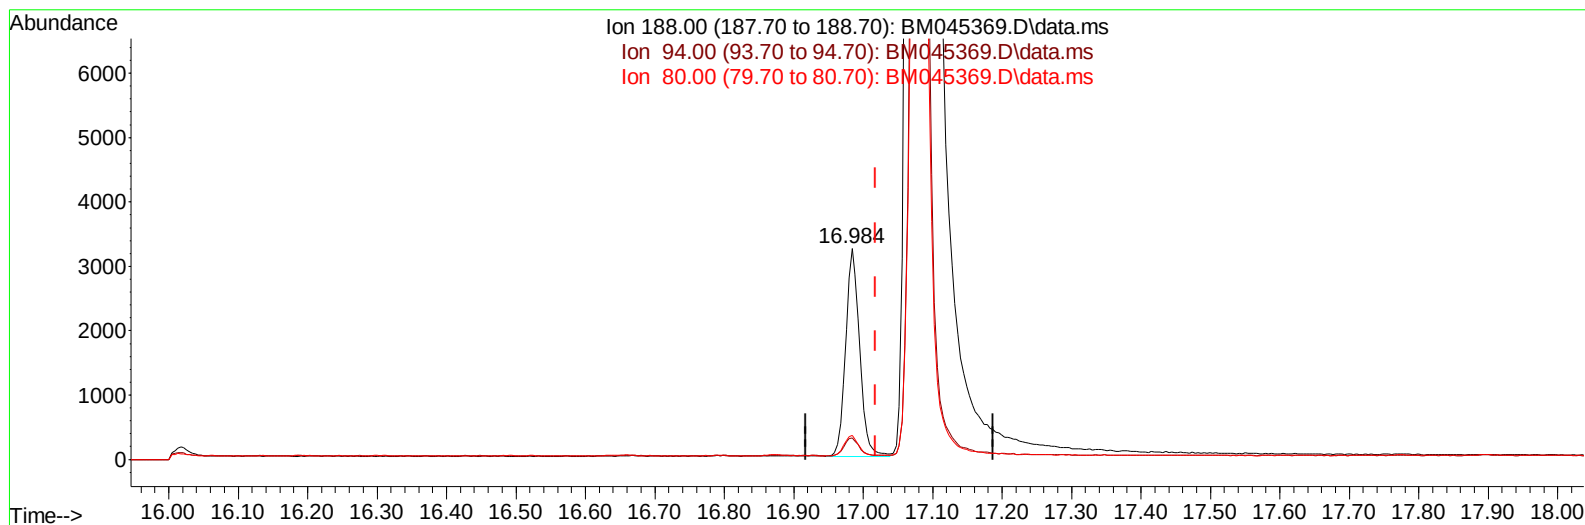

TIC: BM045369.D\data.ms

(13) Phenanthrene-d10 (I)

16.984min (-0.034) 0.40 ng/ul m

response 4548

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.00	10.10
80.00	11.80	11.29
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045369.D
Acq On : 18 Apr 2024 23:58
Operator : MA/JU
Sample : P2077-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF6

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:31:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/22/2024

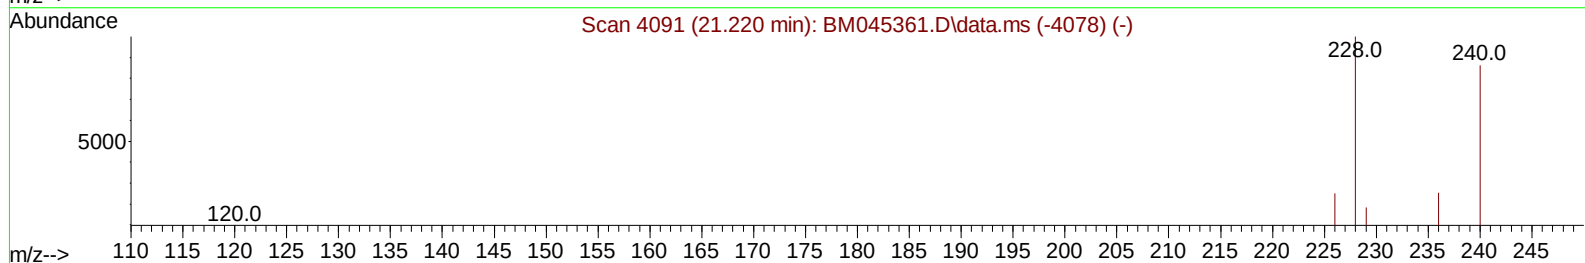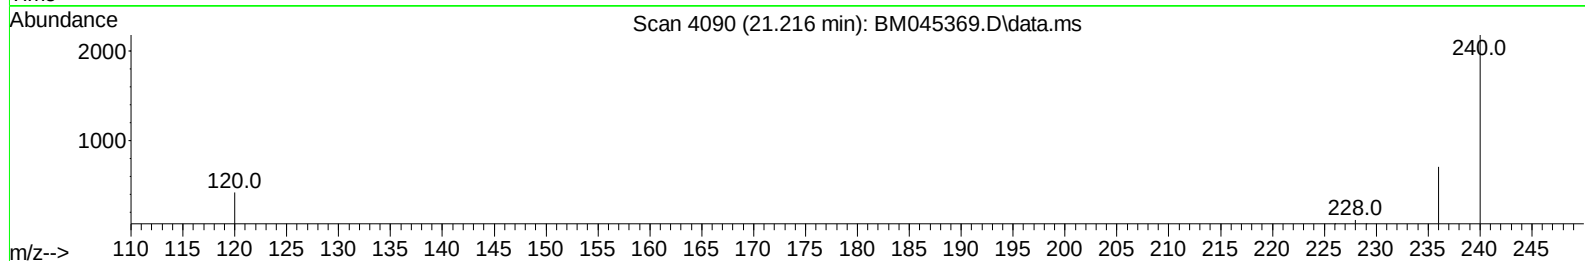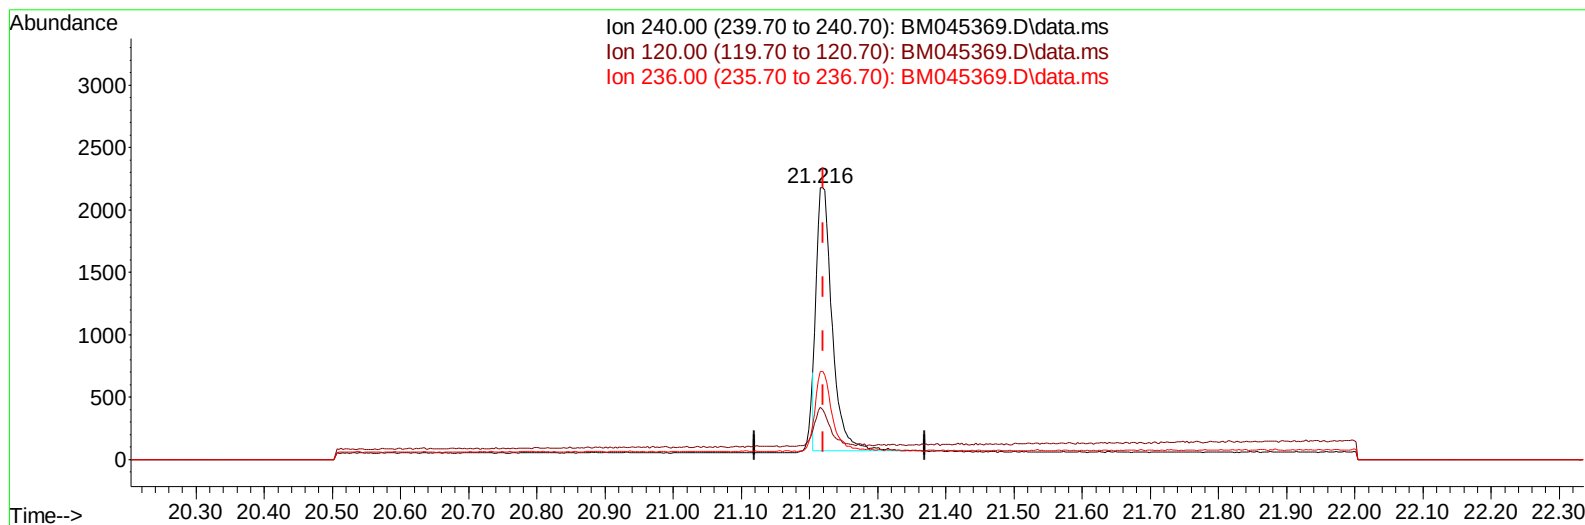

TIC: BM045369.D\data.ms

(17) Chrysene-d12

21.216min (-0.003) 0.40 ng/u1

response 3392

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.80	19.15
236.00	31.10	32.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045369.D
Acq On : 18 Apr 2024 23:58
Operator : MA/JU
Sample : P2077-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF6

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:31:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/22/2024

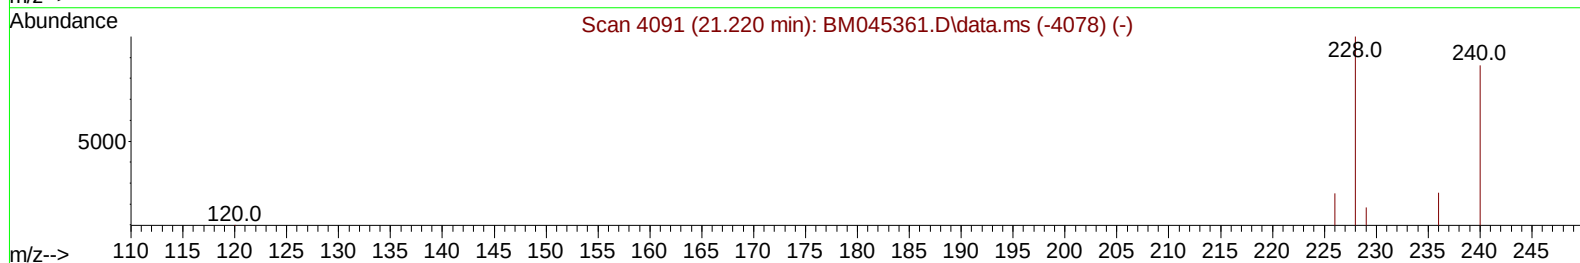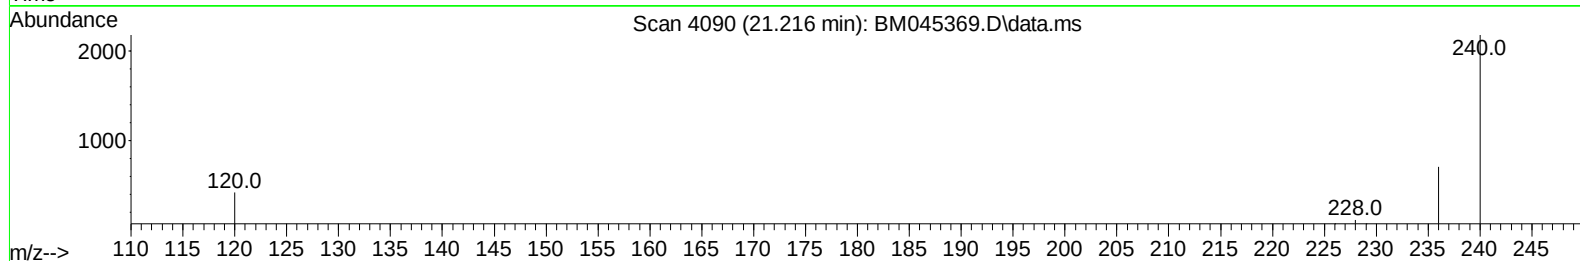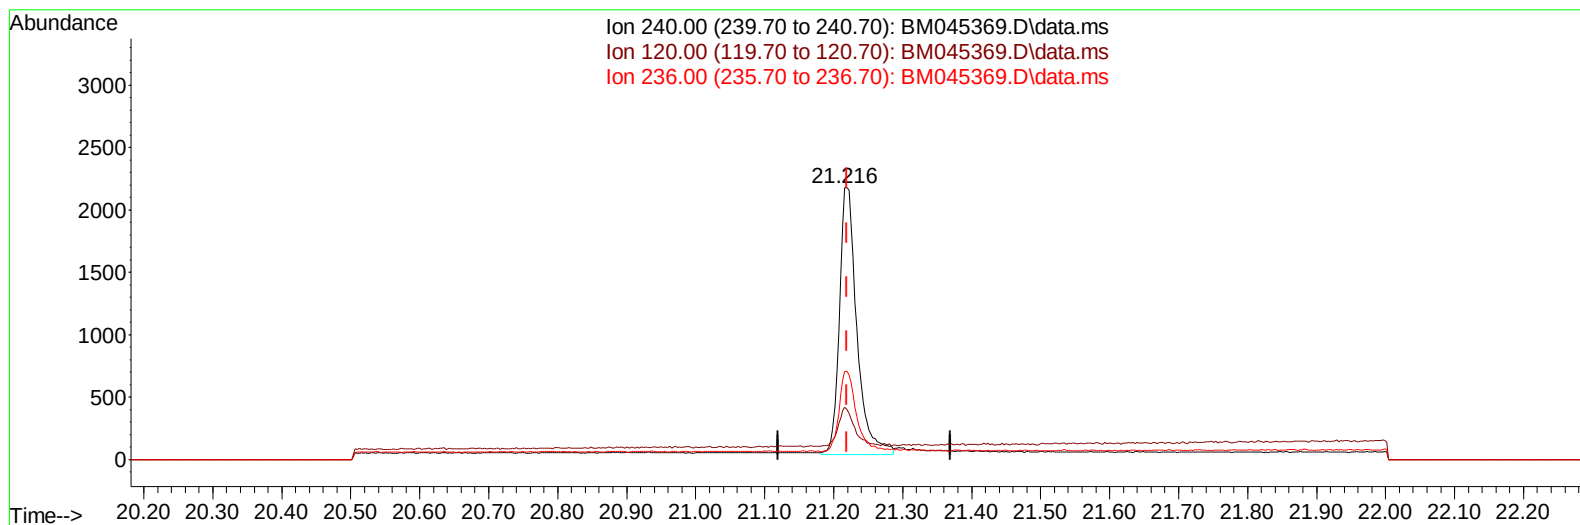

TIC: BM045369.D\data.ms

(17) Chrysene-d12

21.216min (-0.003) 0.40 ng/ul m

response 3750

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.80	19.15
236.00	31.10	32.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045369.D
Acq On : 18 Apr 2024 23:58
Operator : MA/JU
Sample : P2077-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF6

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:31:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/22/2024

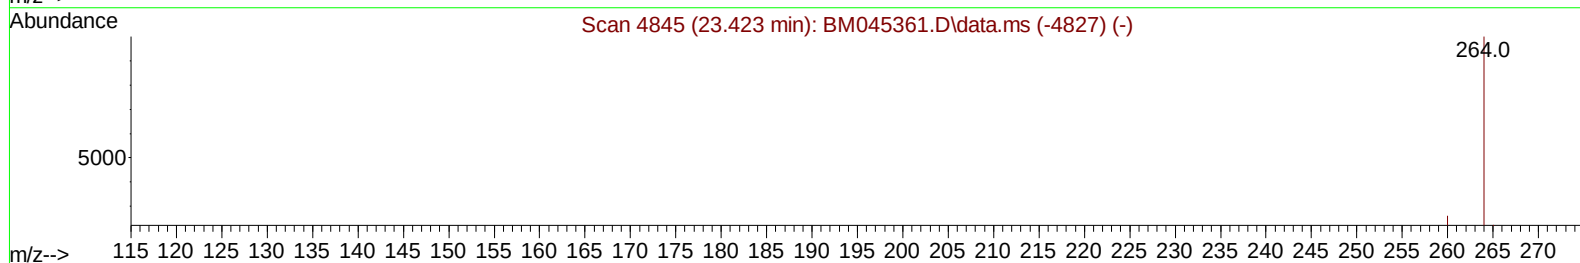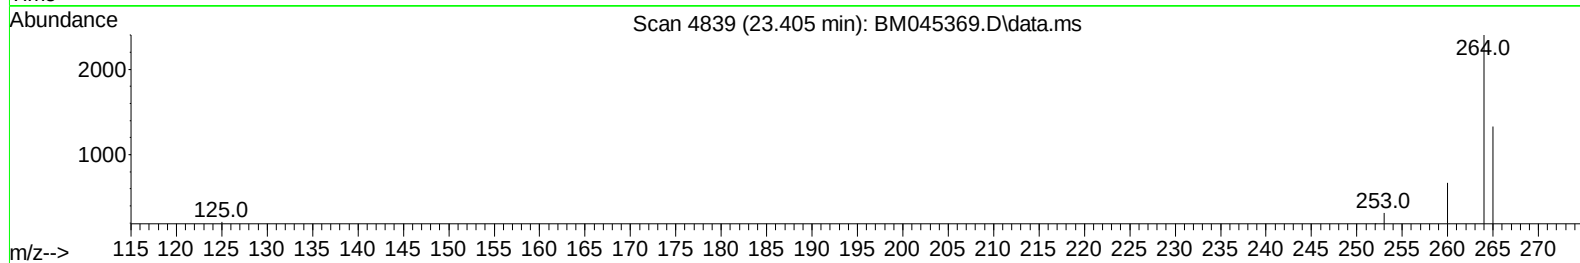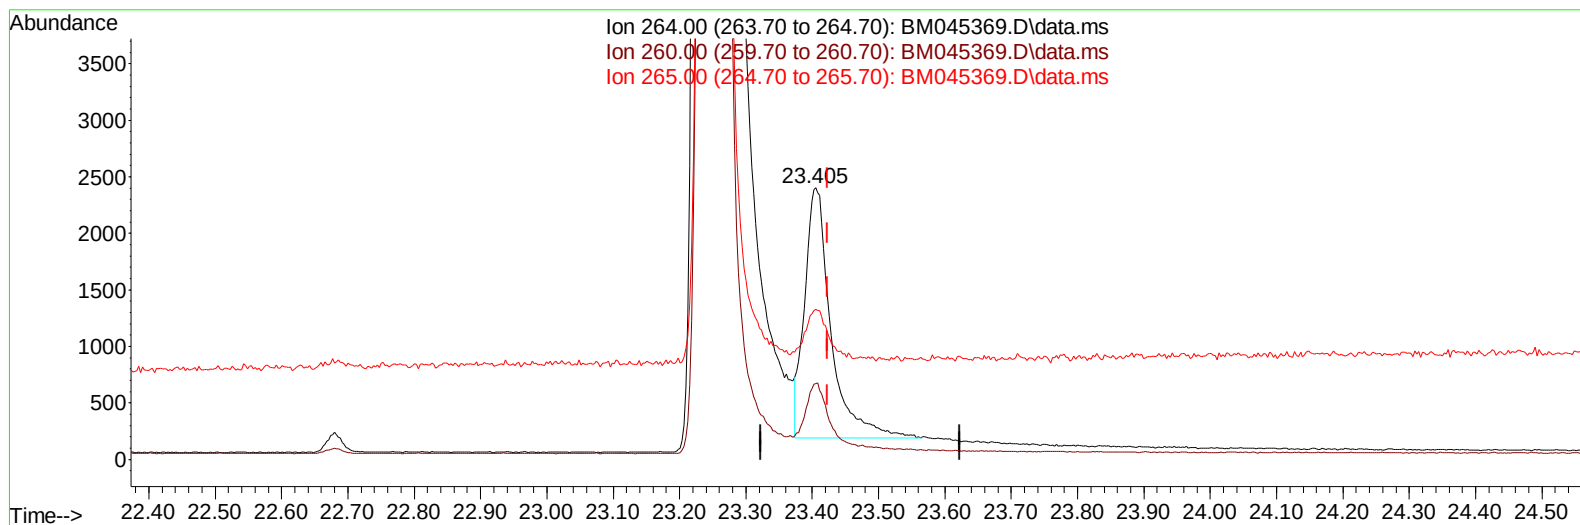

TIC: BM045369.D\data.ms

(23) Perylene-d12 (I)

23.405min (-0.018) 0.40 ng/u1

response 6193

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	27.91
265.00	70.40	55.39#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045369.D
Acq On : 18 Apr 2024 23:58
Operator : MA/JU
Sample : P2077-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF6

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:31:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/22/2024

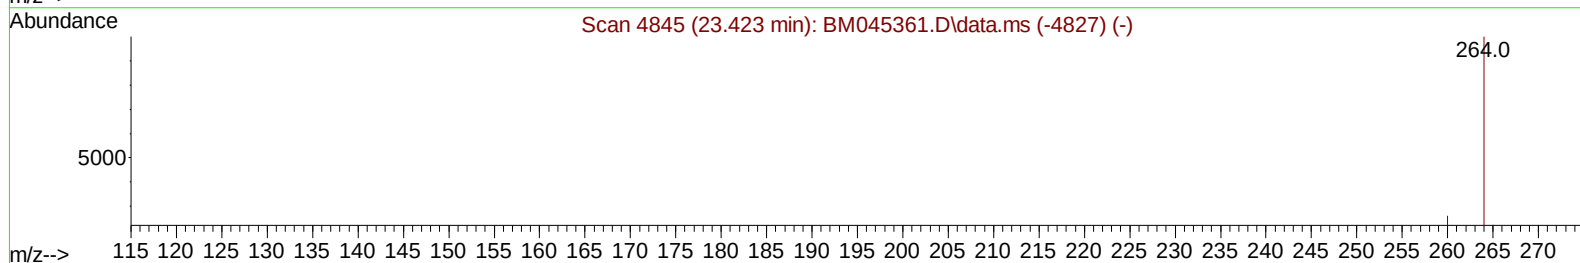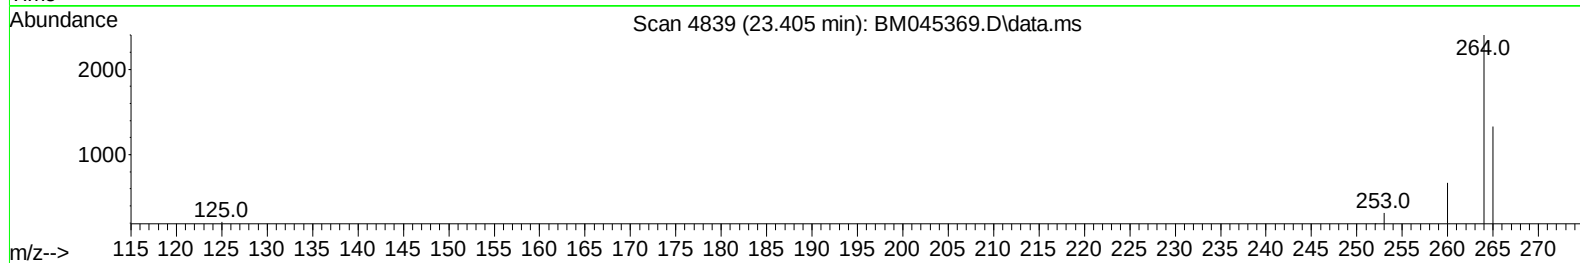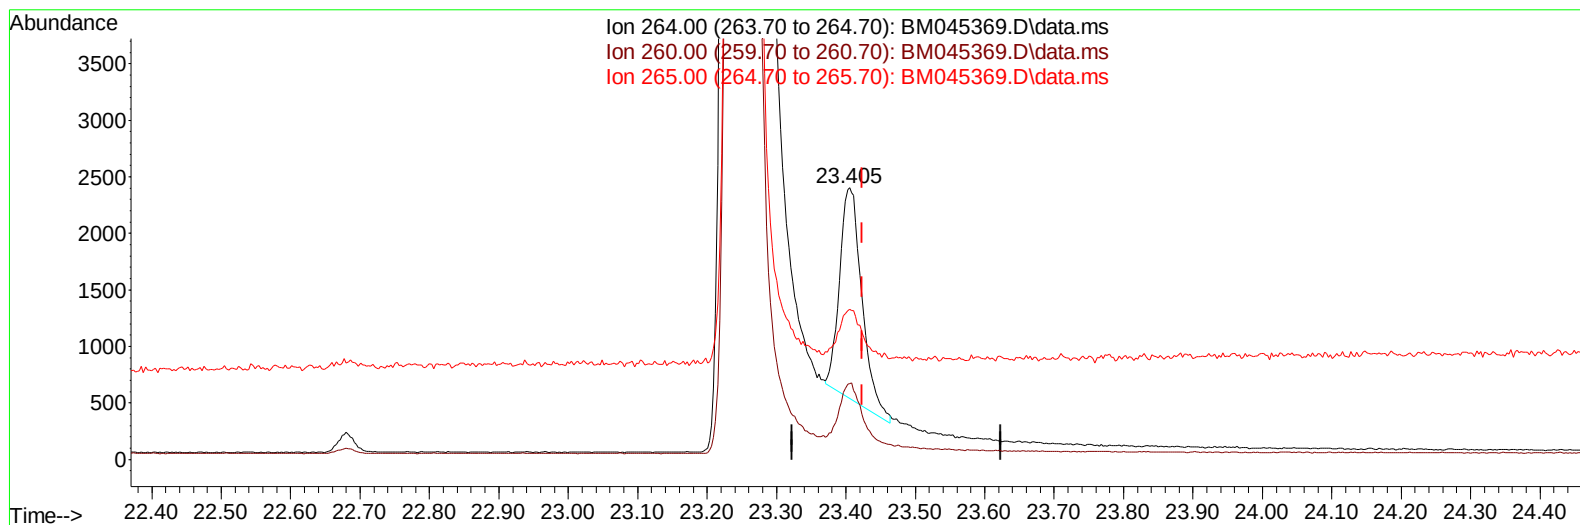

TIC: BM045369.D\data.ms

(23) Perylene-d12 (I)

23.405min (-0.018) 0.40 ng/ul m

response 4134

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	27.91
265.00	70.40	55.39#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
 Data File : BM045369.D
 Acq On : 18 Apr 2024 23:58
 Operator : MA/JU
 Sample : P2077-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/19/2024
 Supervised By :mohammad ahmed 04/22/2024

Quant Time: Apr 19 00:31:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 18 22:19:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.576	152	1247	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.342	136	3609	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.224	164	2003m	0.400	ng/ul	-0.02
13) Phenanthrene-d10	16.984	188	4548m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.216	240	3750m	0.400	ng/ul	0.00
23) Perylene-d12	23.405	264	4134m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.176	96	4077	2.489	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.975	152	1094	0.224	ng/ul	-0.02
18) Fluoranthene-d10	19.029	212	2941	0.310	ng/ul	-0.02

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045369.D
Acq On : 18 Apr 2024 23:58
Operator : MA/JU
Sample : P2077-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF6

Manual IntegrationsAPPROVED

Quant Time: Apr 19 00:31:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/22/2024

