




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045394.D
Acq On : 19 Apr 2024 15:38
Operator : MA/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
LabSampleId :
SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Apr 19 16:16:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/22/2024
Supervised By :mohammad ahmed 04/22/2024

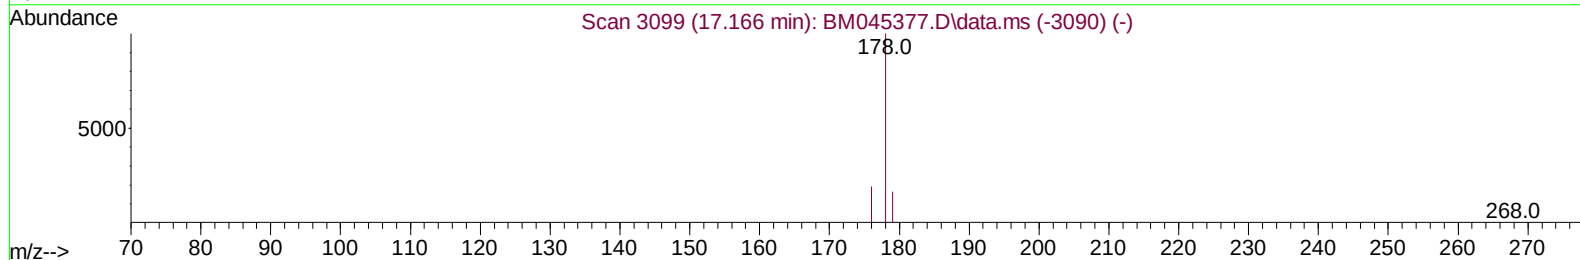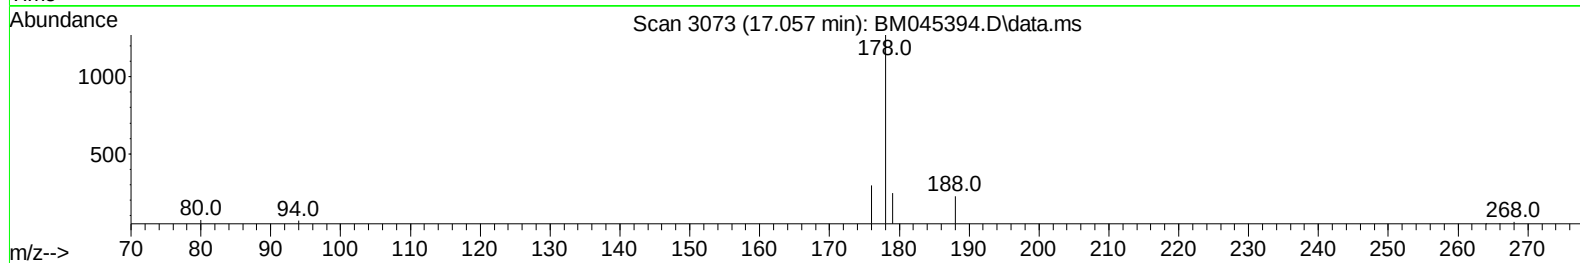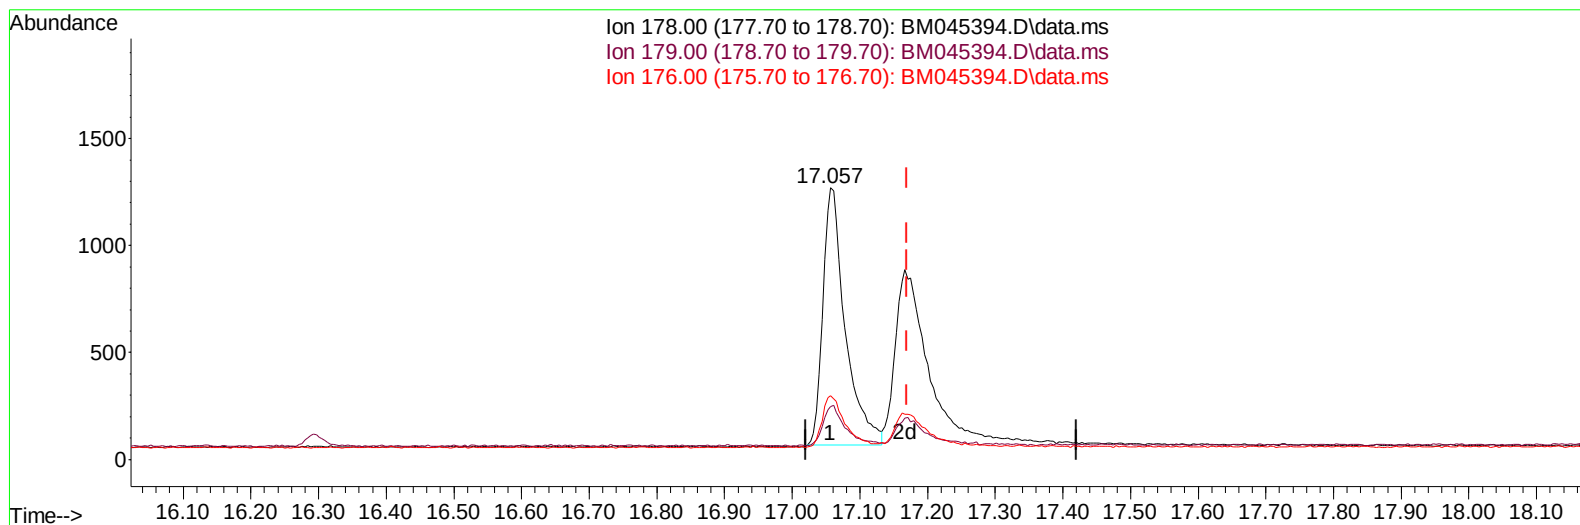

TIC: BM045394.D\data.ms

(16) Anthracene

17.057min (-0.113) 0.39 ng/u1

response 2761

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.30	19.39
176.00	20.30	23.40
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
 Data File : BM045394.D
 Acq On : 19 Apr 2024 15:38
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Apr 19 16:16:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 18 22:19:59 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/22/2024
 Supervised By :mohammad ahmed 04/22/2024

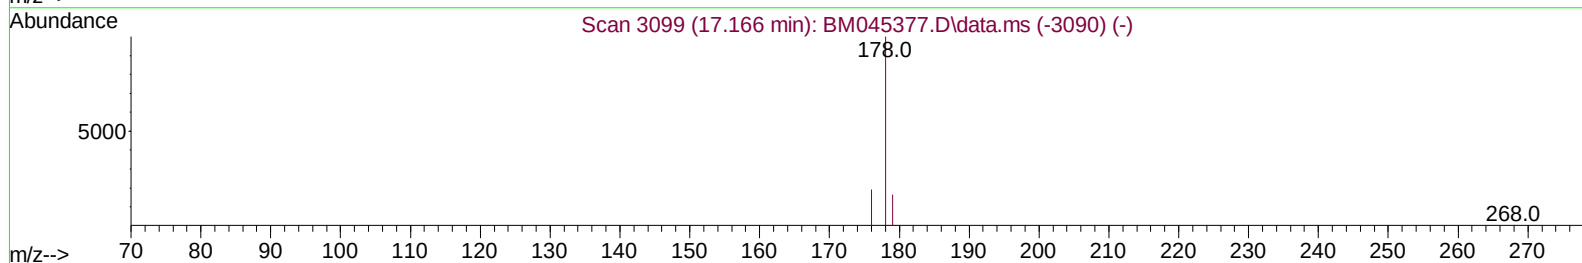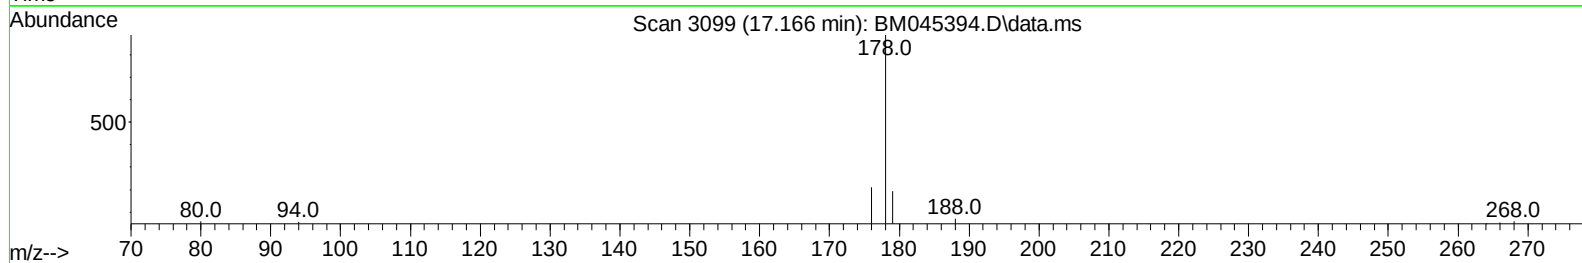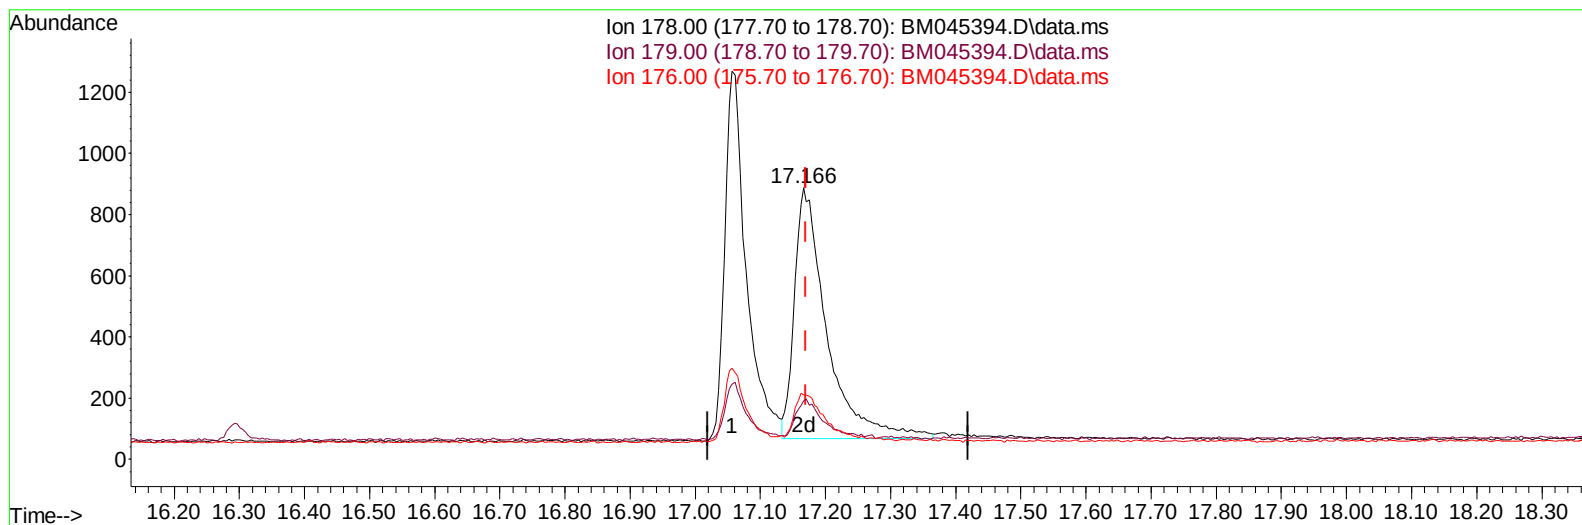

TIC: BM045394.D\data.ms

(16) Anthracene

17.166min (-0.003) 0.40 ng/ul m

response 2847

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.30	21.65#
176.00	20.30	23.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
 Data File : BM045394.D
 Acq On : 19 Apr 2024 15:38
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/22/2024
 Supervised By :mohammad ahmed 04/22/2024

Quant Time: Apr 19 16:16:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 18 22:19:59 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.606	152		886	0.400	ng/ul	0.00
4) Naphthalene-d8	10.380	136		2572	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.238	164		1215	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.014	188		2572	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.219	240		1936	0.400	ng/ul	# 0.00
23) Perylene-d12	23.419	264		2767	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.184	96		487	0.418	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.991	152		1317	0.378	ng/ul	0.00
18) Fluoranthene-d10	19.048	212		2258	0.462	ng/ul	0.00
Target Compounds							
						Qvalue	
2) 1,4-Dioxane	3.213	88		471	0.422	ng/ul#	82
5) Naphthalene	10.435	128		2729	0.400	ng/ul#	94
7) 2-Methylnaphthalene	12.074	142		1539	0.378	ng/ul	97
8) 1-Methylnaphthalene	12.272	142		1712	0.385	ng/ul	97
10) Acenaphthylene	13.961	152		2473	0.408	ng/ul	96
11) Acenaphthene	14.303	153		1848	0.426	ng/ul	99
12) Fluorene	15.321	166		1936	0.398	ng/ul#	99
14) Pentachlorophenol	16.689	266		212	0.352	ng/ul	99
15) Phenanthrene	17.057	178		2830	0.391	ng/ul	95
16) Anthracene	17.166	178		2847m	0.399	ng/ul	
19) Fluoranthene	19.081	202		3231	0.467	ng/ul#	94
20) Pyrene	19.443	202		3419	0.468	ng/ul#	94
21) Benzo(a)anthracene	21.213	228		2612	0.388	ng/ul	97
22) Chrysene	21.257	228		3686	0.438	ng/ul	97
24) Benzo(b)fluoranthene	22.759	252		3732	0.373	ng/ul	96
25) Benzo(k)fluoranthene	22.805	252		4660	0.416	ng/ul#	92
26) Benzo(a)pyrene	23.334	252		3808	0.399	ng/ul#	88
27) Indeno(1,2,3-cd)pyrene	25.628	276		5447	0.417	ng/ul#	100
28) Dibenzo(a,h)anthracene	25.658	278		4295	0.415	ng/ul#	87
29) Benzo(g,h,i)perylene	26.298	276		4908	0.435	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045394.D
Acq On : 19 Apr 2024 15:38
Operator : MA/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
LabSampleId :
SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Apr 19 16:16:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/22/2024
Supervised By :mohammad ahmed 04/22/2024

