




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045404.D
Acq On : 19 Apr 2024 22:35
Operator : MA/JU
Sample : P2032-13
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MF9

Manual IntegrationsAPPROVED

Quant Time: Apr 19 23:38:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/22/2024
Supervised By :mohammad ahmed 04/22/2024

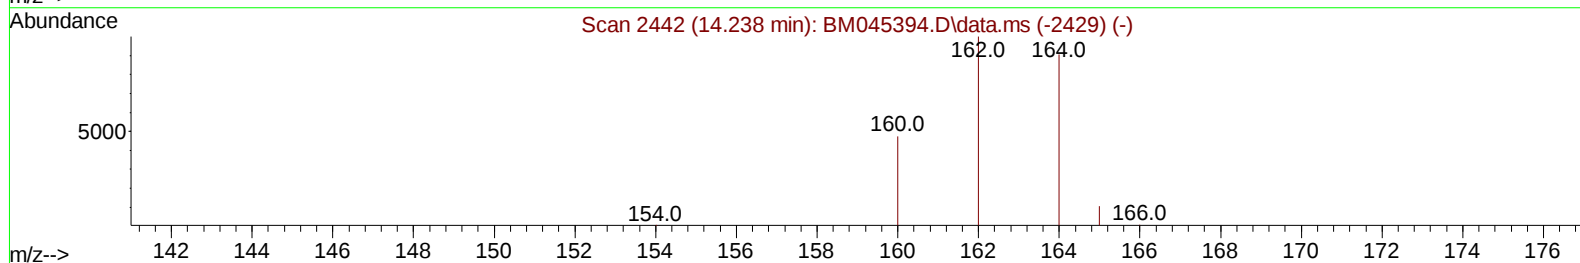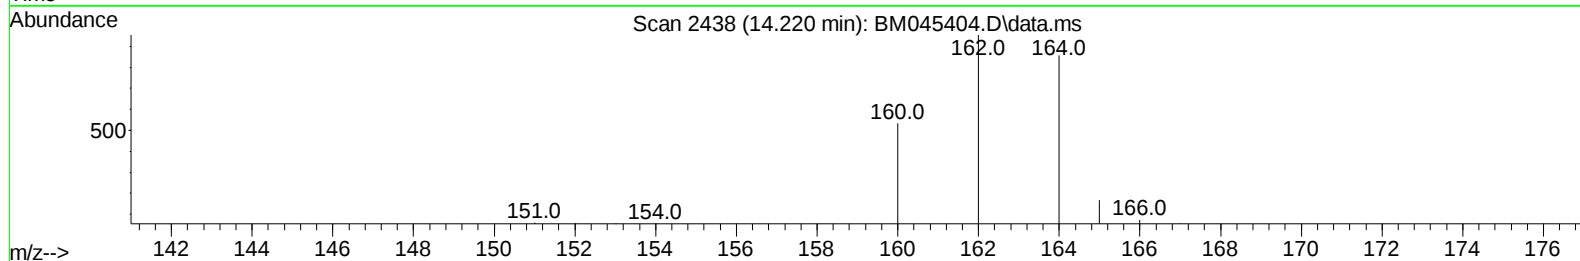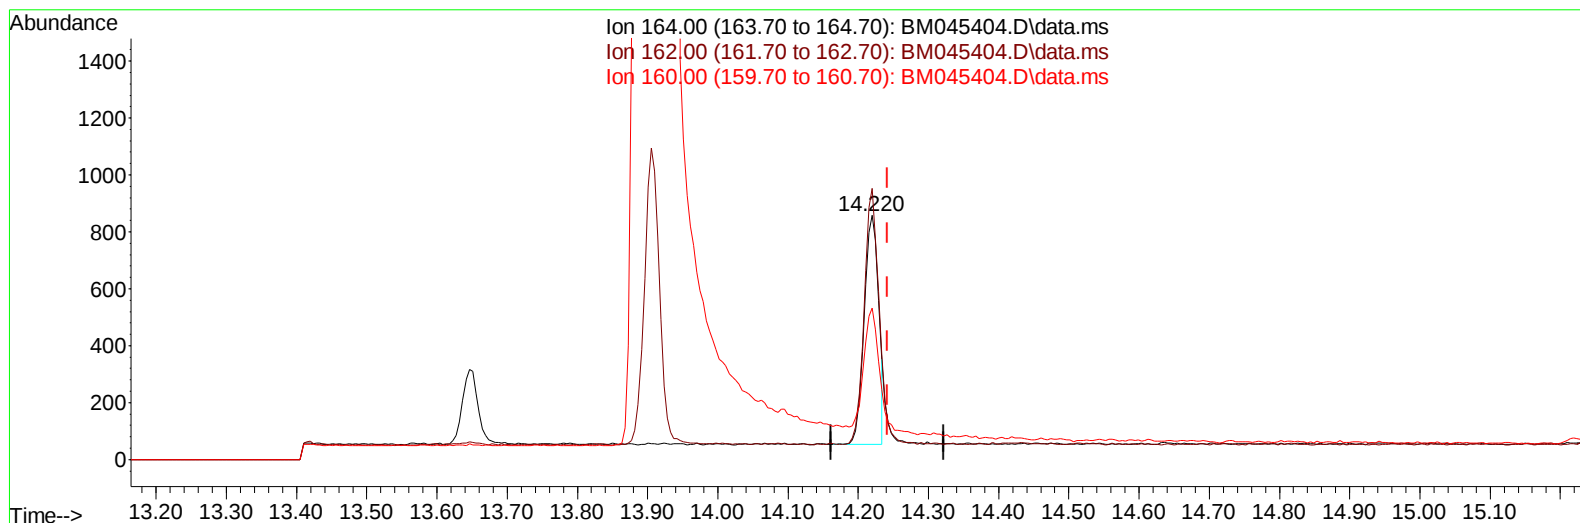

TIC: BM045404.D\data.ms

(9) Acenaphthene-d10 (I)

14.220min (-0.022) 0.40 ng/u1

response 1163

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	103.00	111.19
160.00	50.00	62.12#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045404.D
Acq On : 19 Apr 2024 22:35
Operator : MA/JU
Sample : P2032-13
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOMF9

Manual IntegrationsAPPROVED

Quant Time: Apr 19 23:38:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/22/2024
Supervised By :mohammad ahmed 04/22/2024

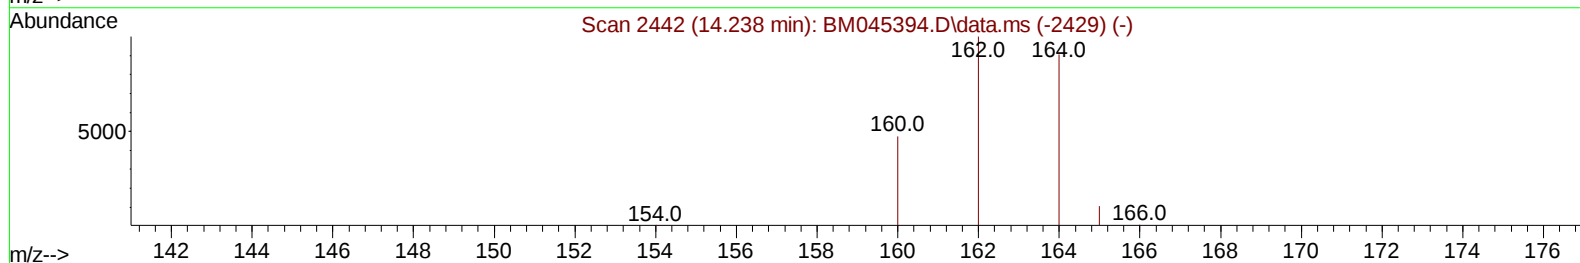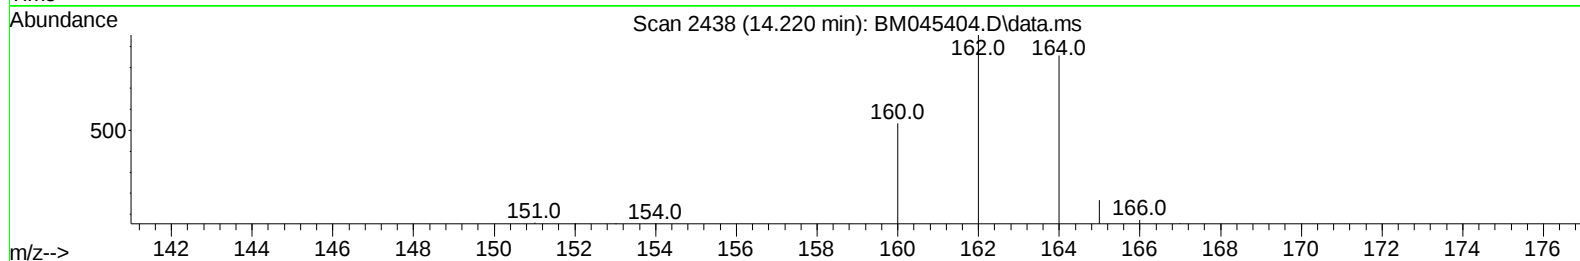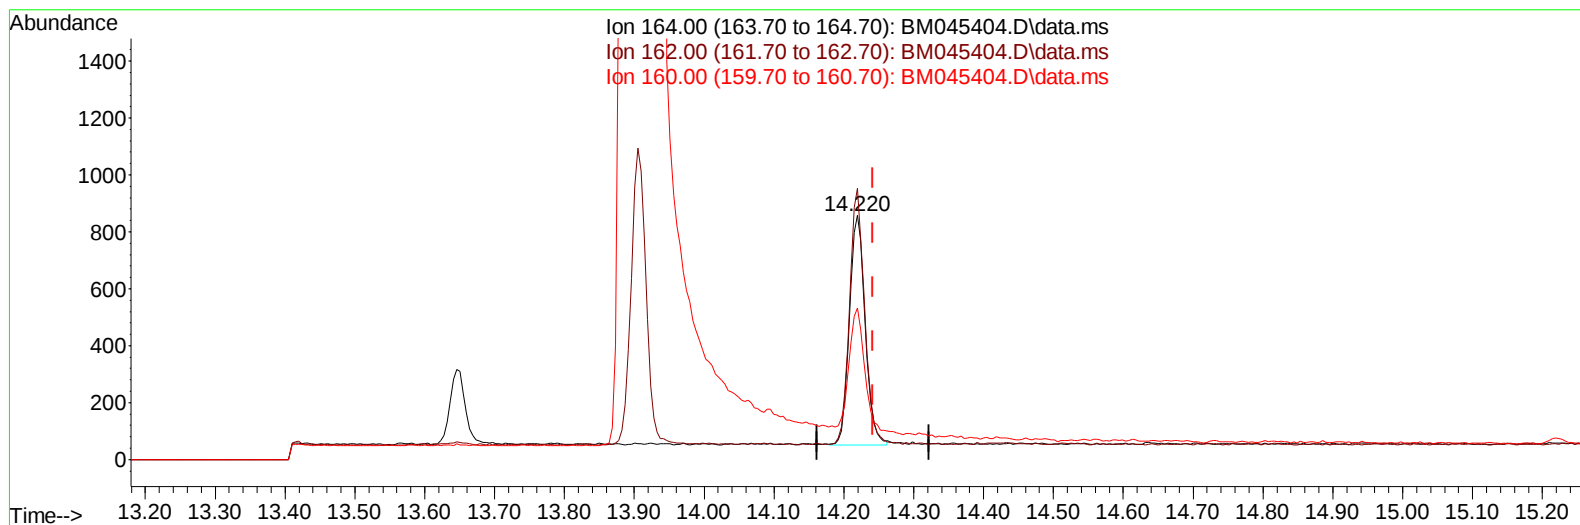

TIC: BM045404.D\data.ms

(9) Acenaphthene-d10 (I)

14.220min (-0.022) 0.40 ng/u1 m

response 1258

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	103.00	111.19
160.00	50.00	62.12#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045404.D
Acq On : 19 Apr 2024 22:35
Operator : MA/JU
Sample : P2032-13
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MF9

Manual IntegrationsAPPROVED

Quant Time: Apr 19 23:38:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/22/2024
Supervised By :mohammad ahmed 04/22/2024

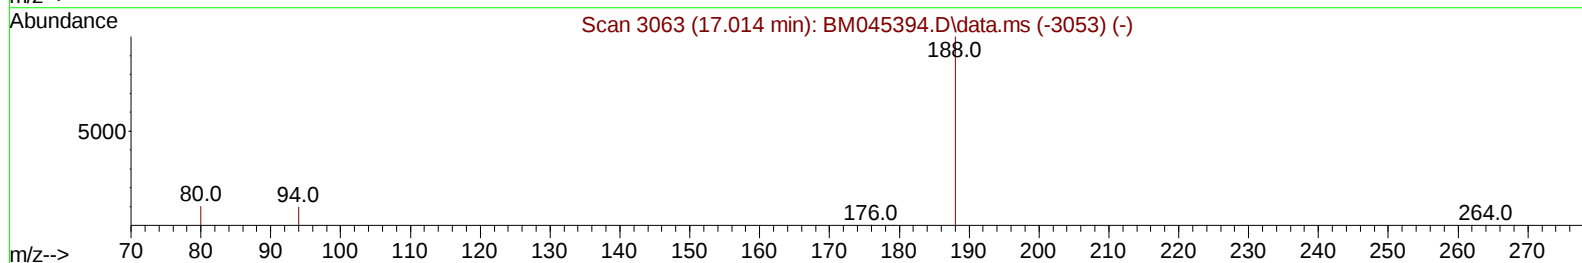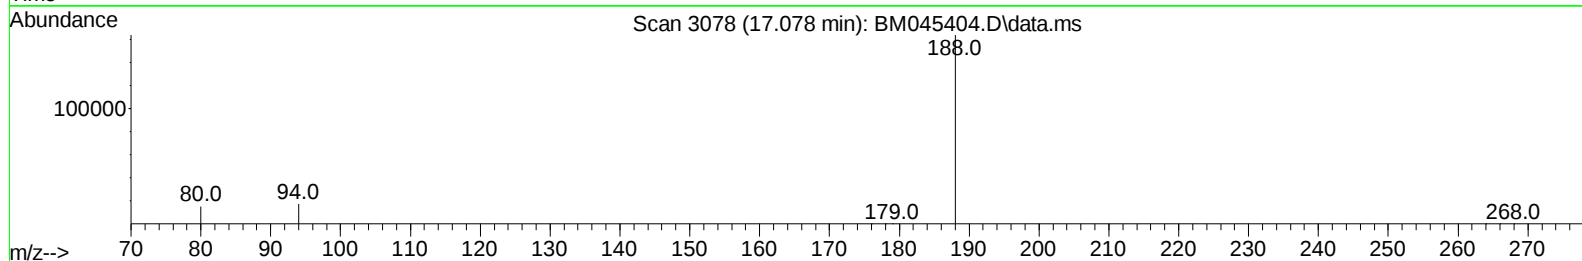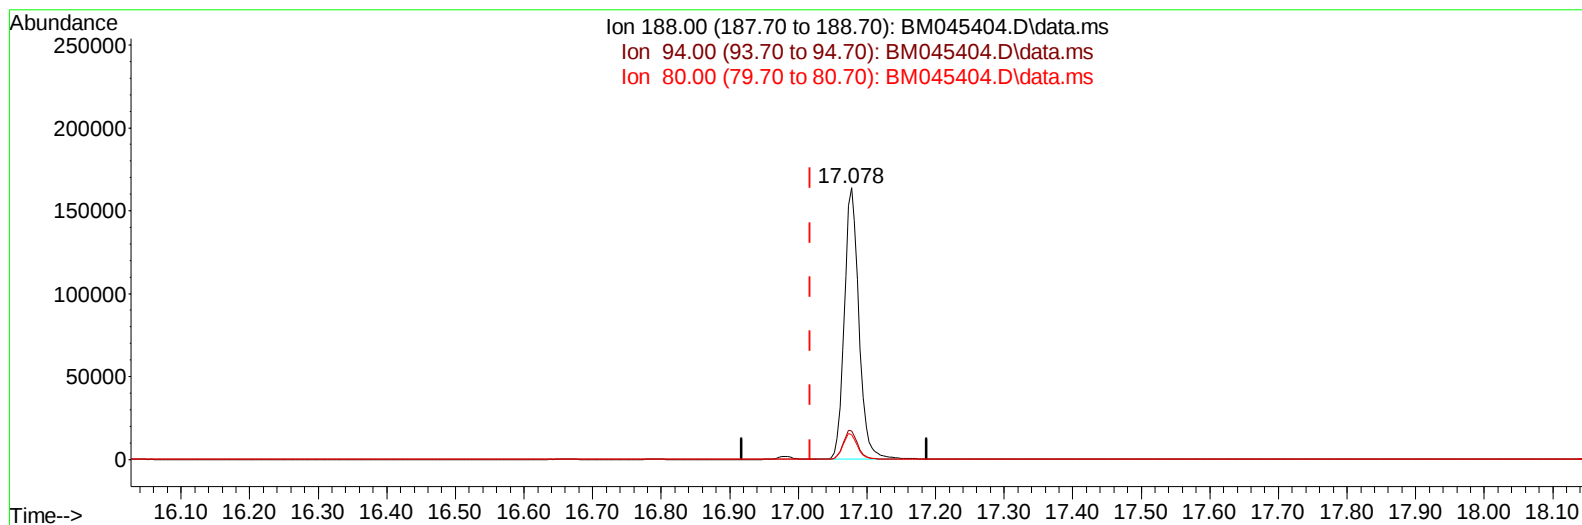

TIC: BM045404.D\data.ms

(13) Phenanthrene-d10 (I)

17.078min (+ 0.060) 0.40 ng/u1

response 241692

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.00	10.55
80.00	11.80	9.22#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
 Data File : BM045404.D
 Acq On : 19 Apr 2024 22:35
 Operator : MA/JU
 Sample : P2032-13
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MF9

Manual IntegrationsAPPROVED

Quant Time: Apr 19 23:38:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 18 22:19:59 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/22/2024
 Supervised By :mohammad ahmed 04/22/2024

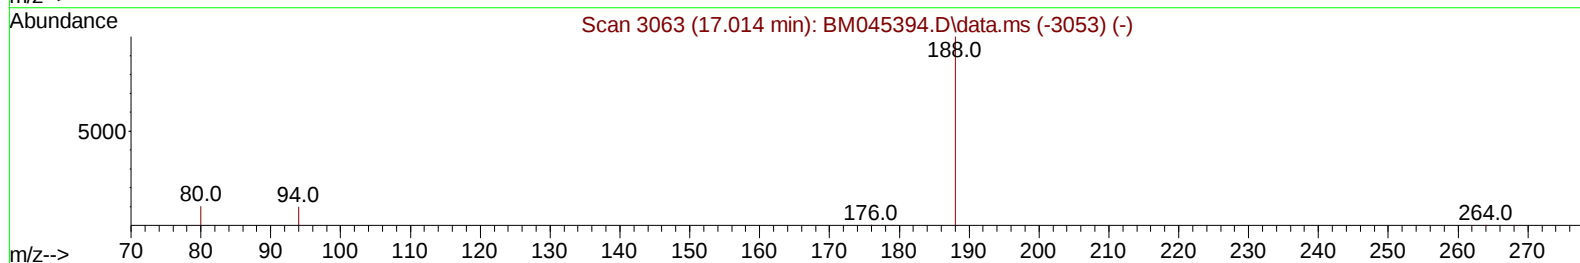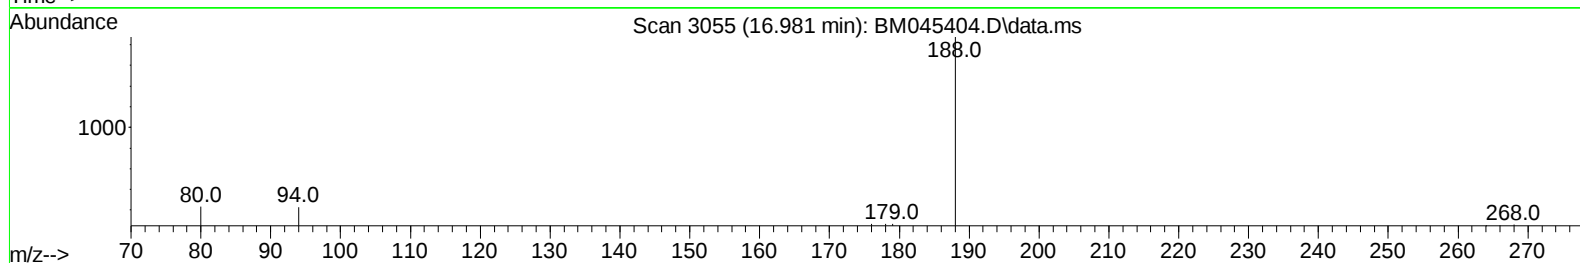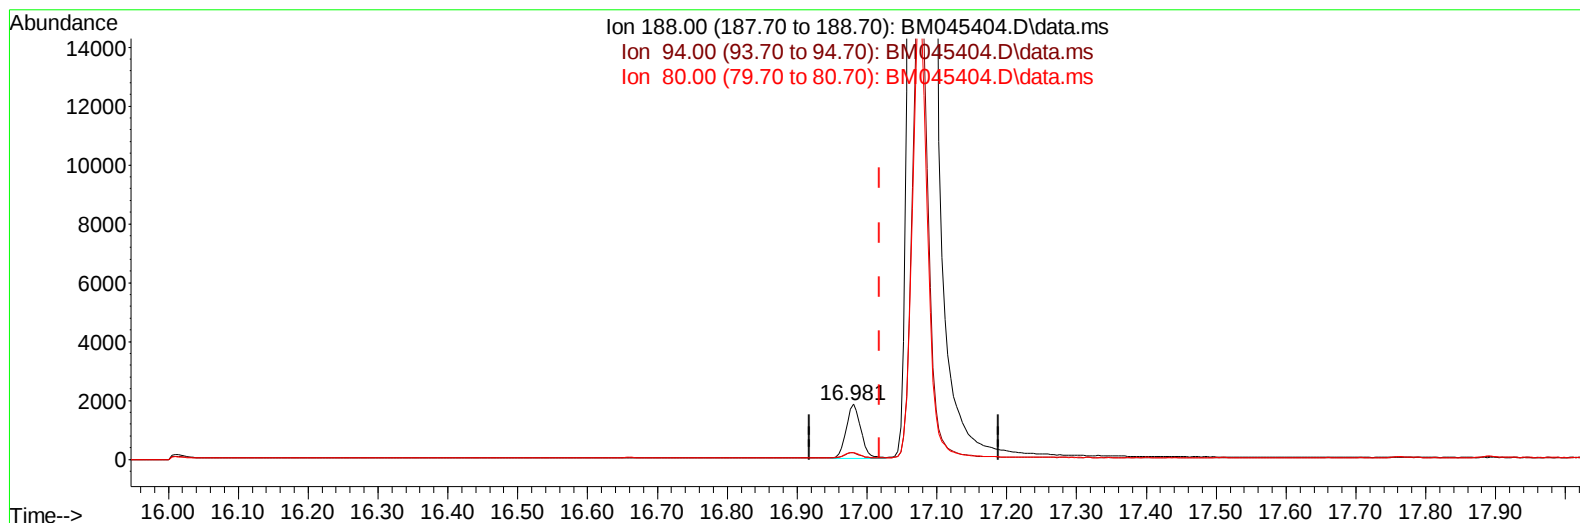

TIC: BM045404.D\data.ms

(13) Phenanthrene-d10 (I)

16.981min (-0.037) 0.40 ng/ul m

response 2703

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.00	12.27
80.00	11.80	12.33
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045404.D
Acq On : 19 Apr 2024 22:35
Operator : MA/JU
Sample : P2032-13
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MF9

Manual IntegrationsAPPROVED

Quant Time: Apr 19 23:38:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/22/2024
Supervised By :mohammad ahmed 04/22/2024

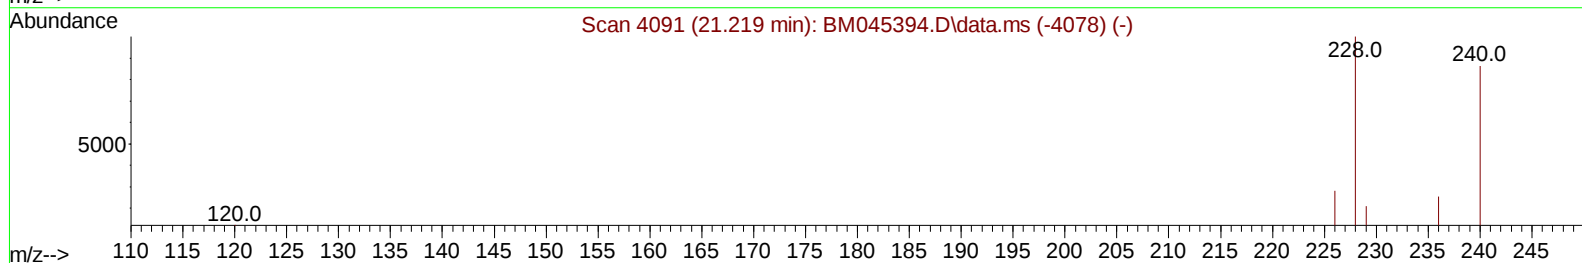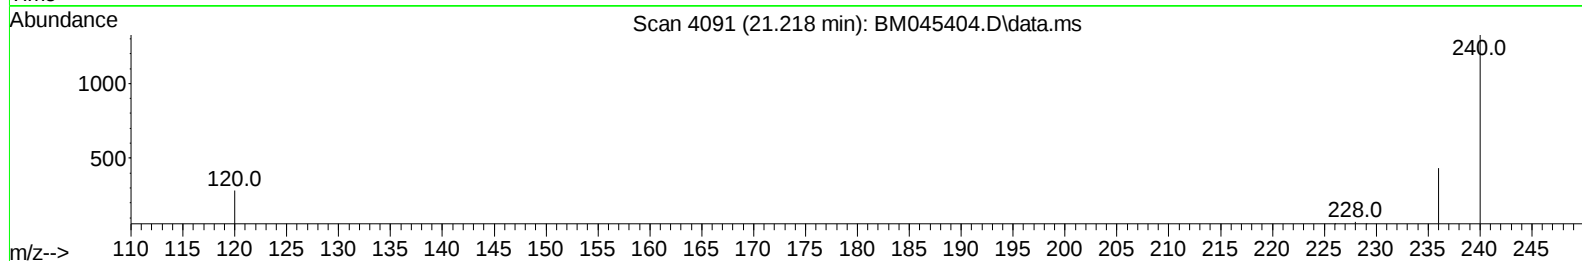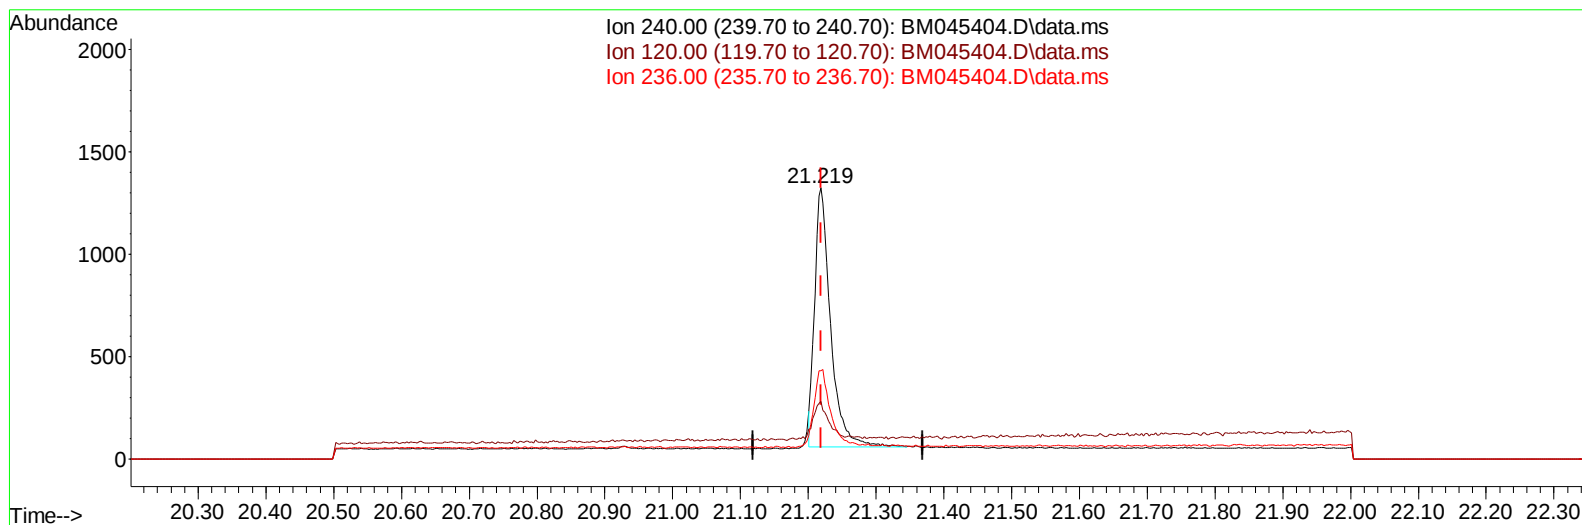

TIC: BM045404.D\data.ms

(17) Chrysene-d12

21.218min (-0.001) 0.40 ng/u1

response 2076

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.80	21.28#
236.00	31.10	32.75
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045404.D
Acq On : 19 Apr 2024 22:35
Operator : MA/JU
Sample : P2032-13
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MF9

Manual IntegrationsAPPROVED

Quant Time: Apr 19 23:38:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/22/2024
Supervised By :mohammad ahmed 04/22/2024

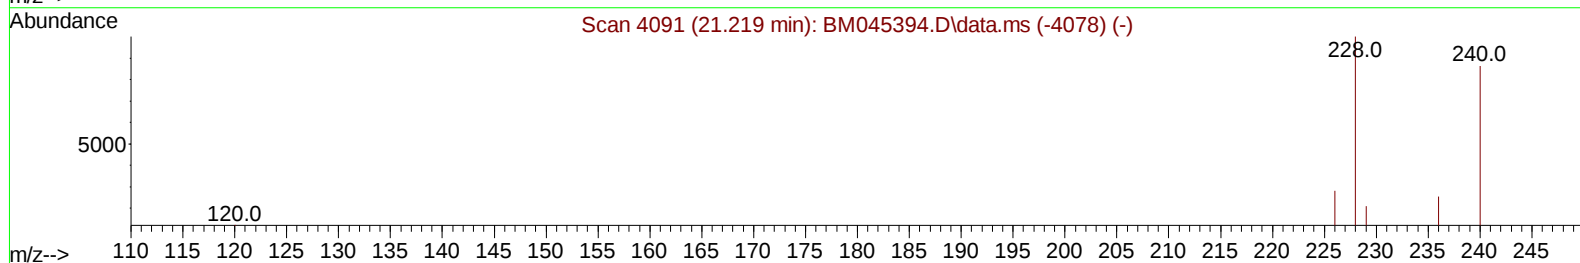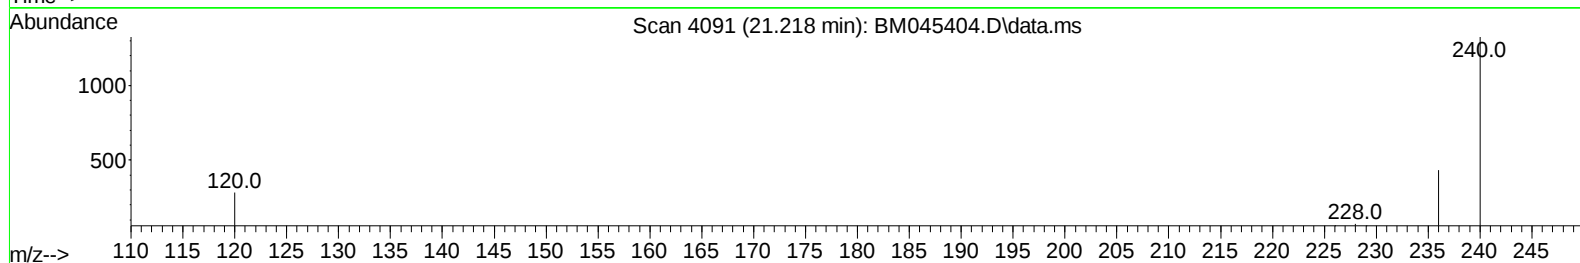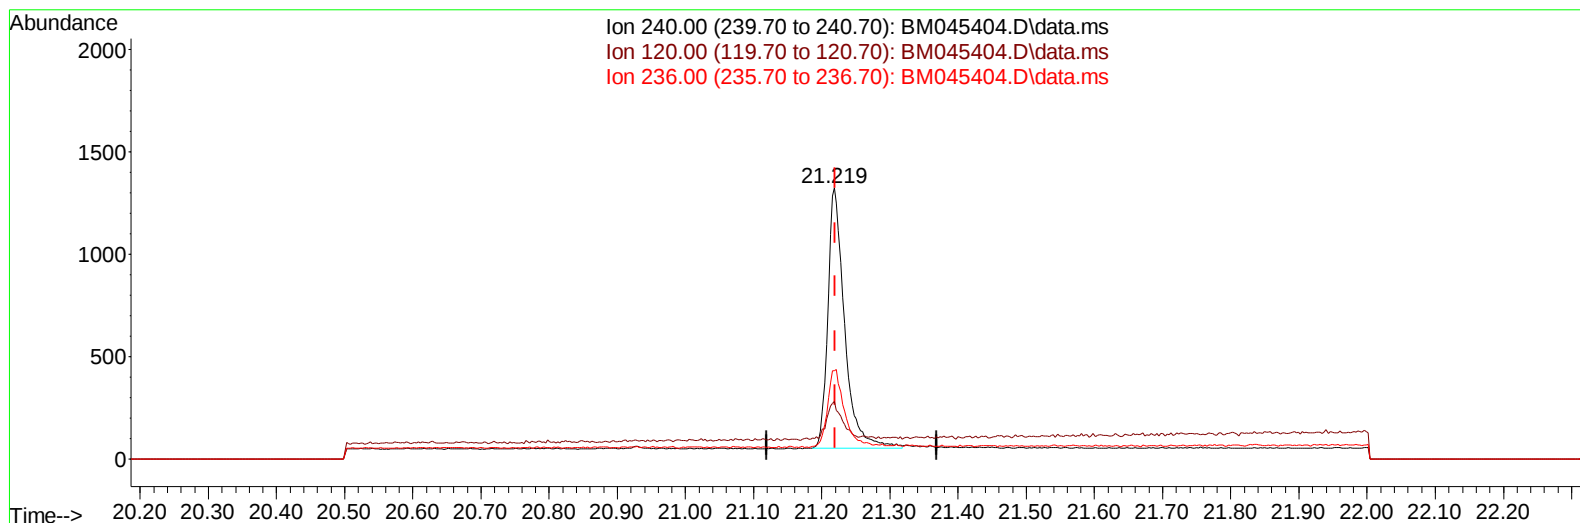

TIC: BM045404.D\data.ms

(17) Chrysene-d12

21.218min (-0.001) 0.40 ng/u1 m

response 2181

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.80	21.28#
236.00	31.10	32.75
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045404.D
Acq On : 19 Apr 2024 22:35
Operator : MA/JU
Sample : P2032-13
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOMF9

Manual IntegrationsAPPROVED

Quant Time: Apr 19 23:38:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/22/2024
Supervised By :mohammad ahmed 04/22/2024

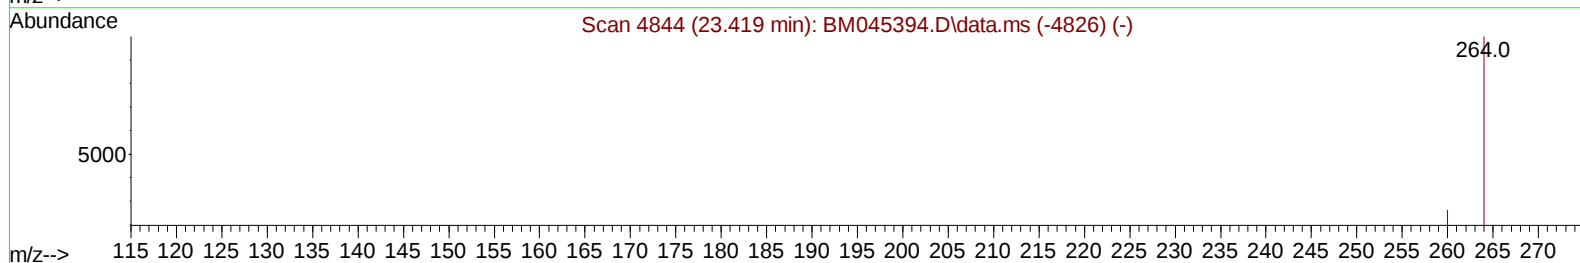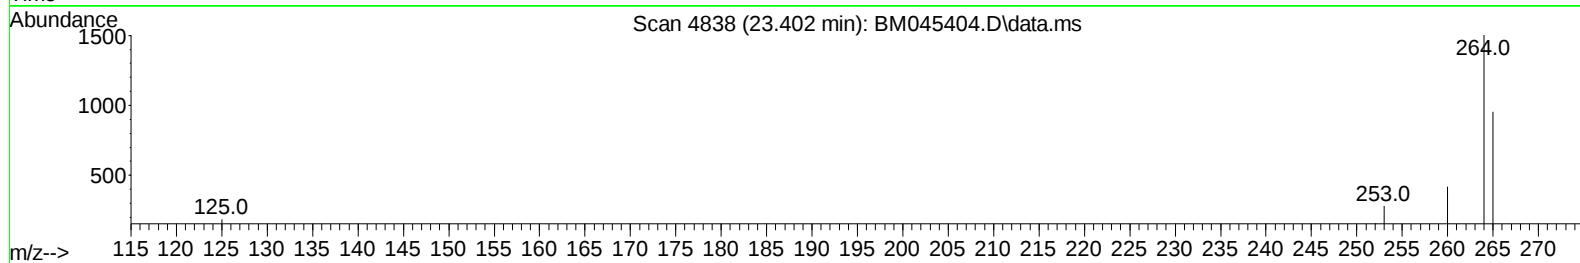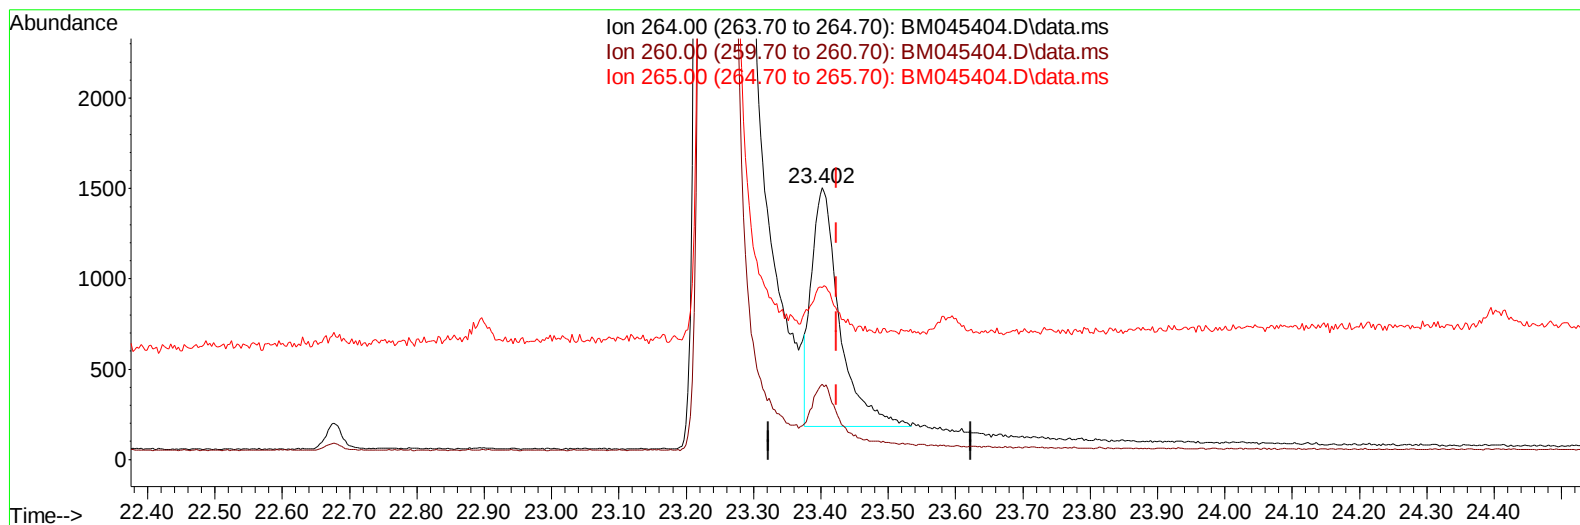

TIC: BM045404.D\data.ms

(23) Perylene-d12 (I)

23.402min (-0.021) 0.40 ng/u1

response 3827

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	27.74
265.00	70.40	63.34
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045404.D
Acq On : 19 Apr 2024 22:35
Operator : MA/JU
Sample : P2032-13
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOMF9

Manual IntegrationsAPPROVED

Quant Time: Apr 19 23:38:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/22/2024
Supervised By :mohammad ahmed 04/22/2024

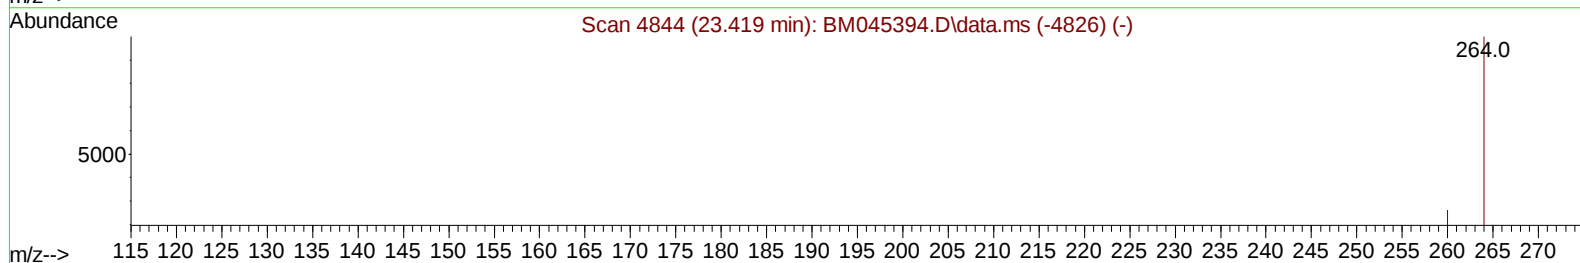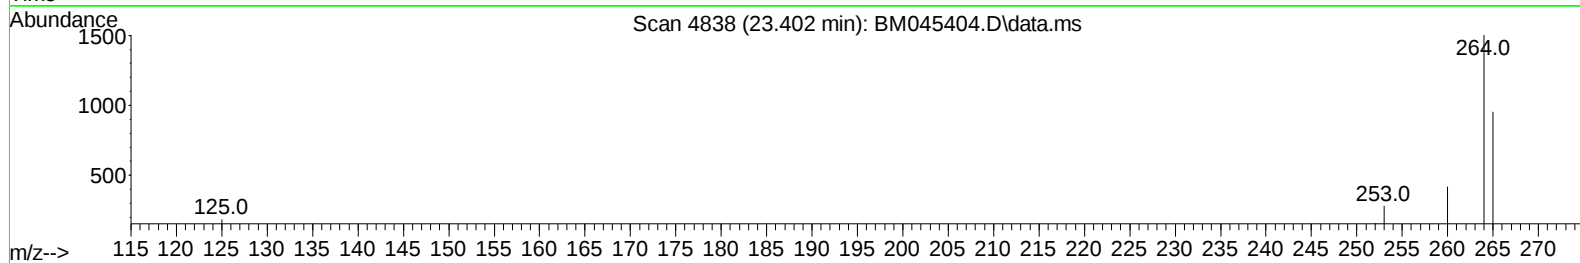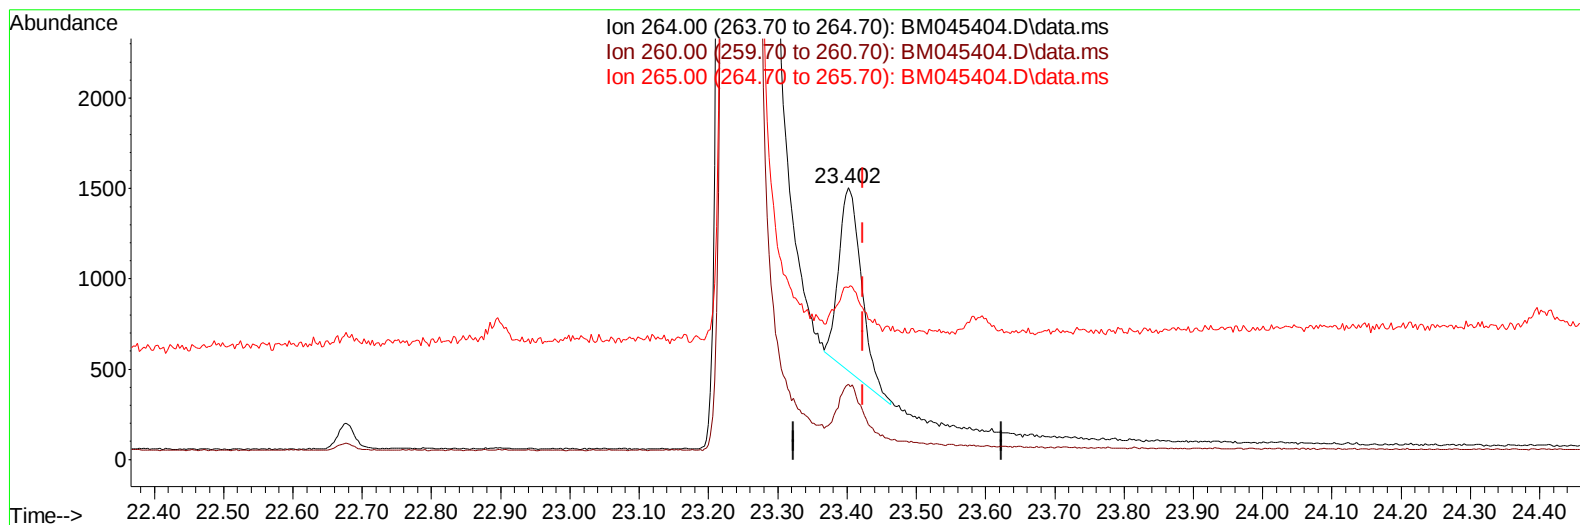

TIC: BM045404.D\data.ms

(23) Perylene-d12 (I)

23.402min (-0.021) 0.40 ng/ul m

response 2291

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	27.74
265.00	70.40	63.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
 Data File : BM045404.D
 Acq On : 19 Apr 2024 22:35
 Operator : MA/JU
 Sample : P2032-13
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MF9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/22/2024
 Supervised By :mohammad ahmed 04/22/2024

Quant Time: Apr 19 23:38:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 18 22:19:59 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.572	152		806	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.336	136		2395	0.400	ng/ul	#-0.05
9) Acenaphthene-d10	14.220	164		1258m	0.400	ng/ul	-0.02
13) Phenanthrene-d10	16.981	188		2703m	0.400	ng/ul	-0.04
17) Chrysene-d12	21.218	240		2181m	0.400	ng/ul	0.00
23) Perylene-d12	23.402	264		2291m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.175	96		3615	3.414	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.964	152		1046	0.322	ng/ul	-0.03
18) Fluoranthene-d10	19.025	212		2445	0.444	ng/ul	-0.03

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045404.D
Acq On : 19 Apr 2024 22:35
Operator : MA/JU
Sample : P2032-13
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MF9

Manual IntegrationsAPPROVED

Quant Time: Apr 19 23:38:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/22/2024
Supervised By :mohammad ahmed 04/22/2024

