

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
 Data File : BM045375.D
 Acq On : 19 Apr 2024 03:34
 Operator : MA/JU
 Sample : P2036-16
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCSY8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/19/2024
 Supervised By :mohammad ahmed 04/22/2024

Quant Time: Apr 19 04:03:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 18 22:19:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.576	152	858	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.341	136	2504	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.223	164	1368m	0.400	ng/ul	-0.02
13) Phenanthrene-d10	16.984	188	2955m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.222	240	2295m	0.400	ng/ul	0.00
23) Perylene-d12	23.405	264	2269m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	3564	3.162	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.975	152	1180	0.348	ng/ul	-0.02
18) Fluoranthene-d10	19.029	212	2857	0.493	ng/ul	-0.02
Target Compounds						Qvalue
2) 1,4-Dioxane	3.209	88	418	0.387	ng/ul#	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041824\
Data File : BM045375.D
Acq On : 19 Apr 2024 03:34
Operator : MA/JU
Sample : P2036-16
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCSY8


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/22/2024


Quant Time: Apr 19 04:03:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 22:19:59 2024
Response via : Initial Calibration

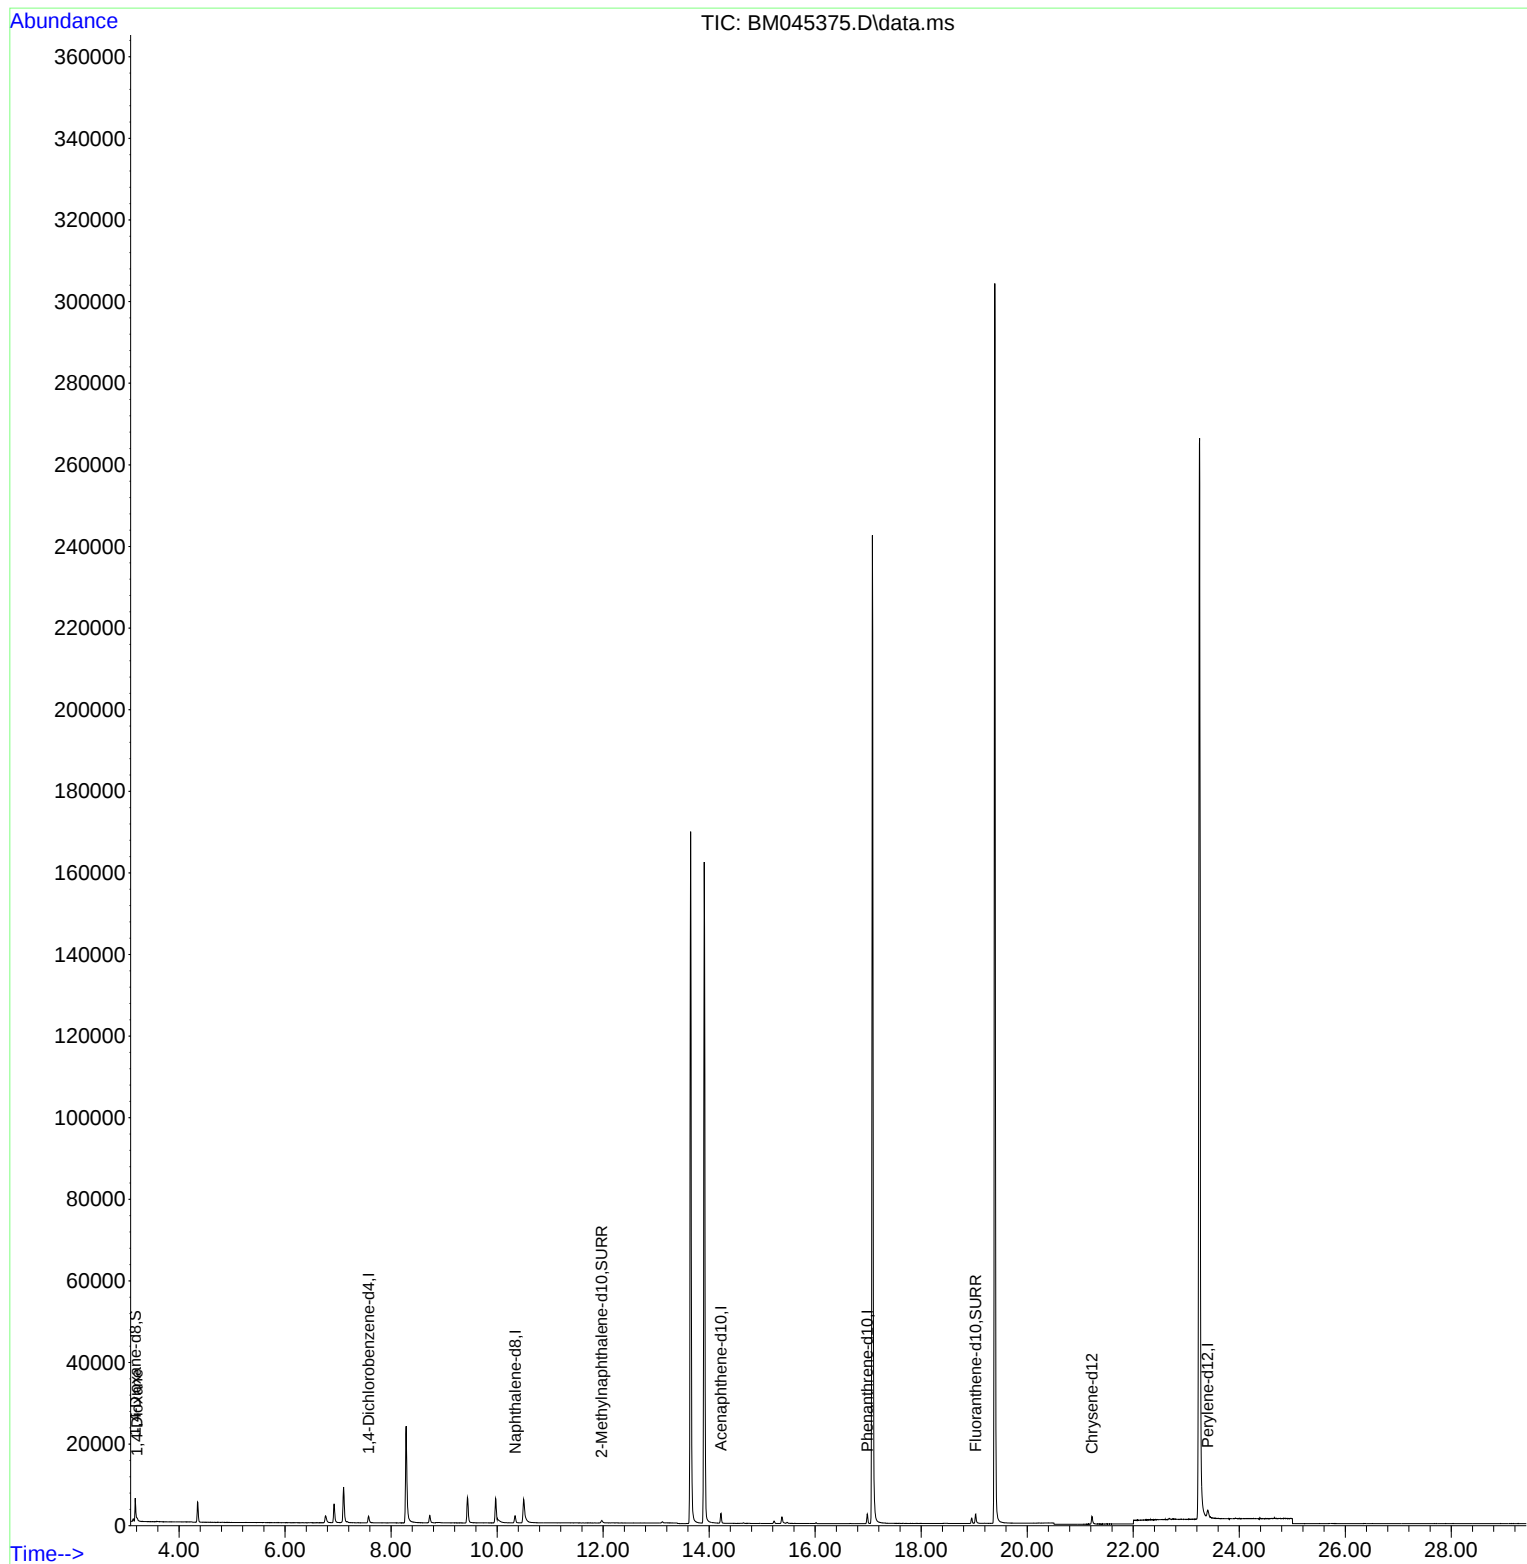


Abundance Scan 31 (3.213 min): BM045361.D\data.ms (-23)

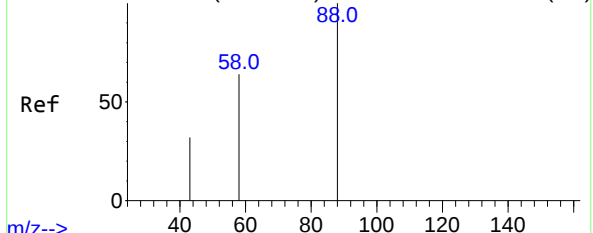

Abundance Scan 30 (3.209 min): BM045375.D\data.ms

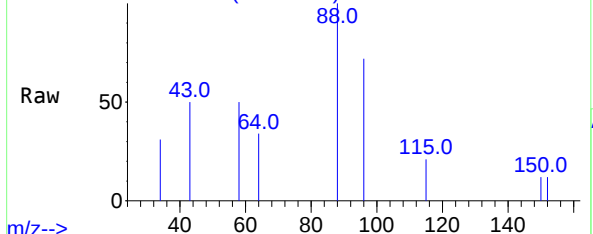

Abundance Scan 30 (3.209 min): BM045375.D\data.ms (-17)

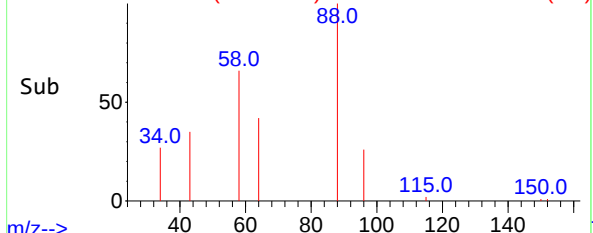

#2
1,4-Dioxane
Concen: 0.387 ng/ul
RT: 3.209 min Scan# 30
Delta R.T. -0.004 min
Lab File: BM045375.D
Acq: 19 Apr 2024 03:34

Tgt Ion: 88	Resp: 418
Ion Ratio	Lower Upper
88	100
43	49.8 30.6 46.0
58	50.2 32.6 48.8

Instrument :
BNA_M
ClientSampleId :
YCSY8

Manual Integrations
APPROVED
Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/22/2024

