
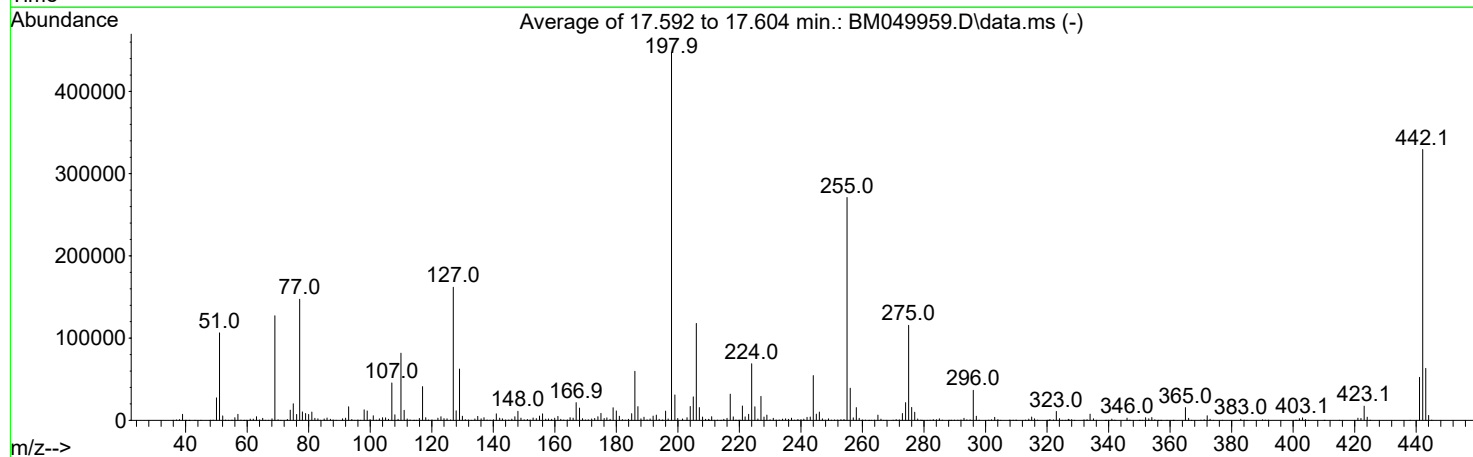


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041825\
Data File : BM049959.D
Acq On : 18 Apr 2025 10:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 09 04:00:55 2025

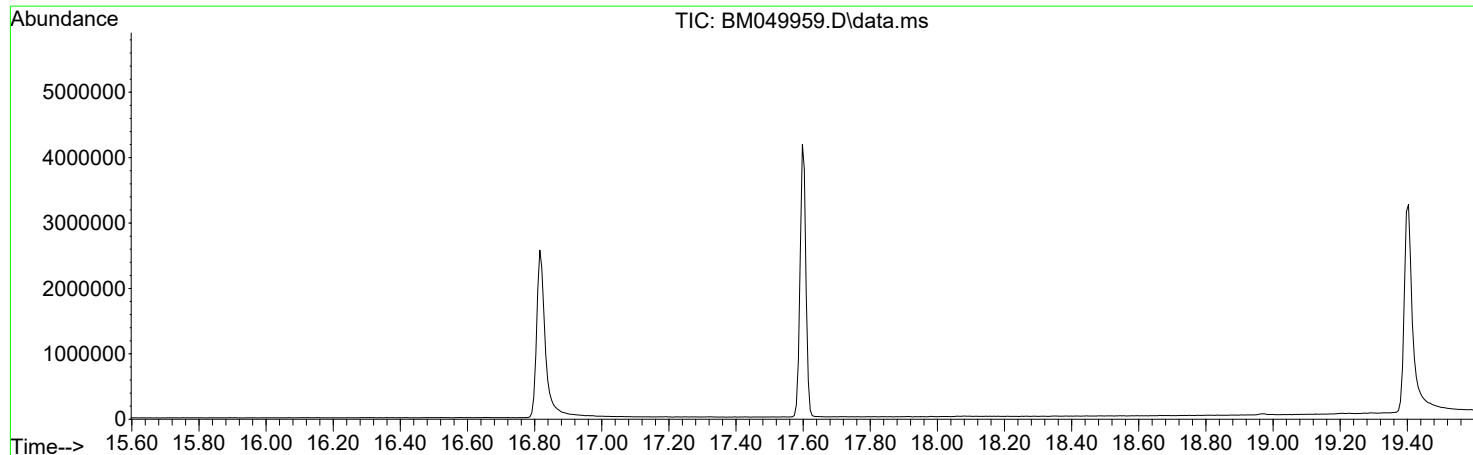

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.8	106519	PASS
68	69	0.00	2	1.5	1959	PASS
69	198	0.00	100	28.5	127371	PASS
70	69	0.00	2	0.6	807	PASS
127	198	10	80	36.2	161941	PASS
197	198	0.00	2	0.4	1774	PASS
198	198	100	100	100.0	447381	PASS
199	198	5	9	6.9	30877	PASS
275	198	10	60	25.8	115619	PASS
365	198	1	100	3.5	15652	PASS
441	198	0.01	100	11.7	52392	PASS
442	442	50	100	100.0	329536	PASS
443	442	15	24	19.2	63181	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/18/2025	BNA_M	<u>BM049959.D</u>
Compound Name	Response	Retention Time
DDT	1285864	20.633
DDD	24366	20.197
DDE	4286	19.686
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28652	1314516	2.18

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041825\
Data File : BM049959.D
Acq On : 18 Apr 2025 10:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 18 11:54:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

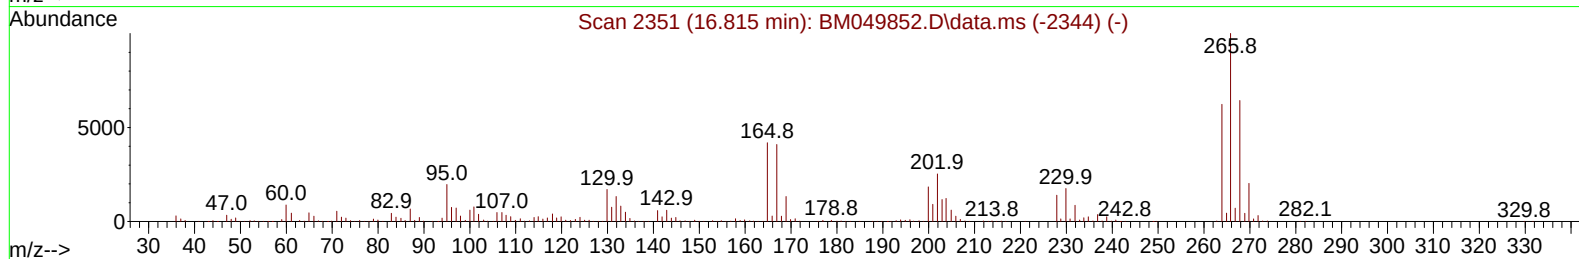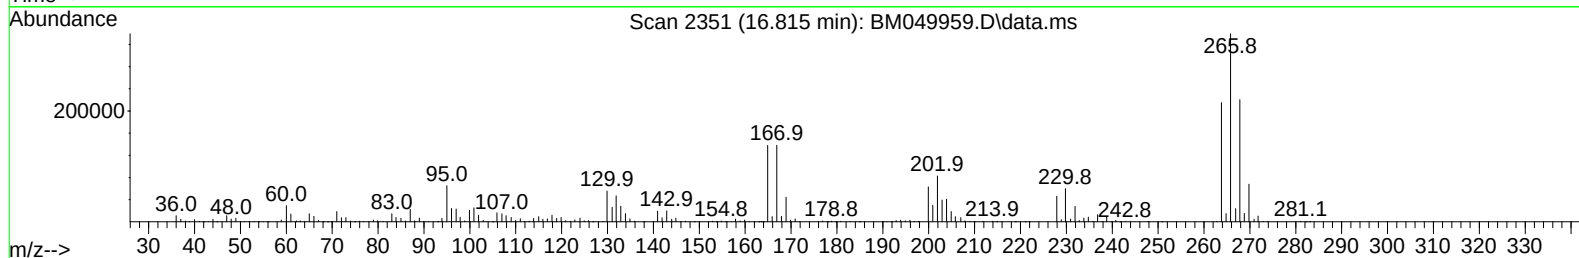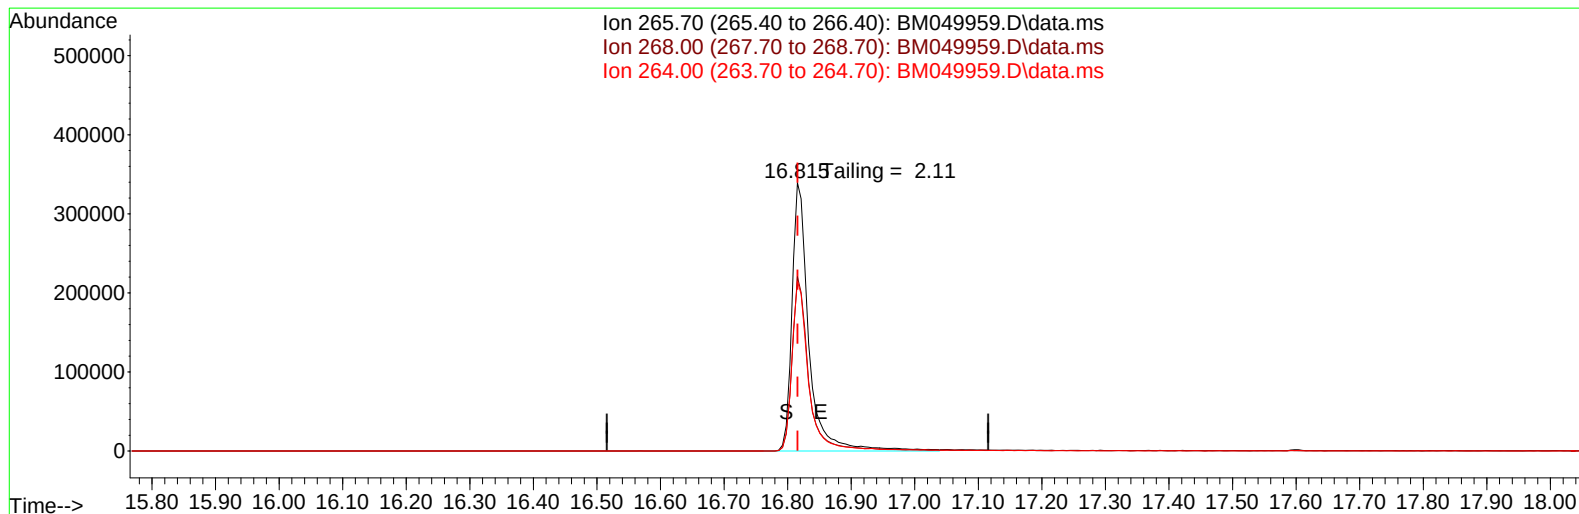

TIC: BM049959.D\data.ms

(70) Pentachlorophenol (C)

16.815min (-0.000) 0.00 ng




response 629116

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	64.95
264.00	62.30	63.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041825\
Data File : BM049959.D
Acq On : 18 Apr 2025 10:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 18 11:54:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

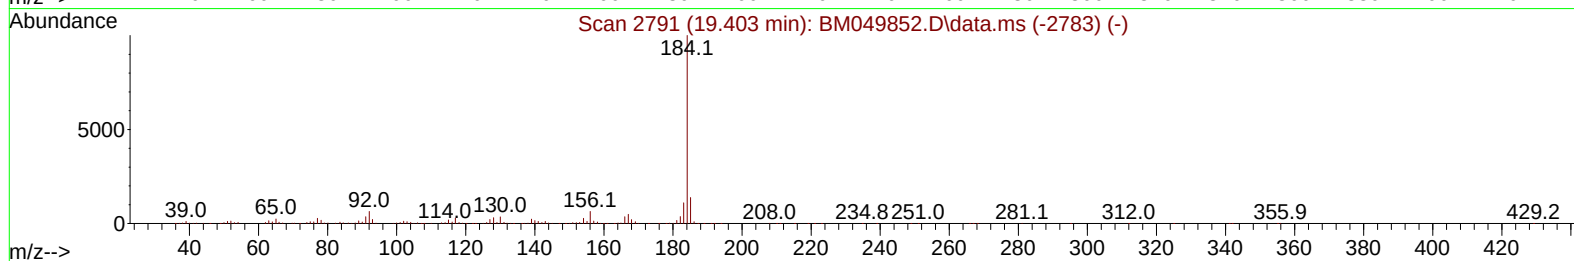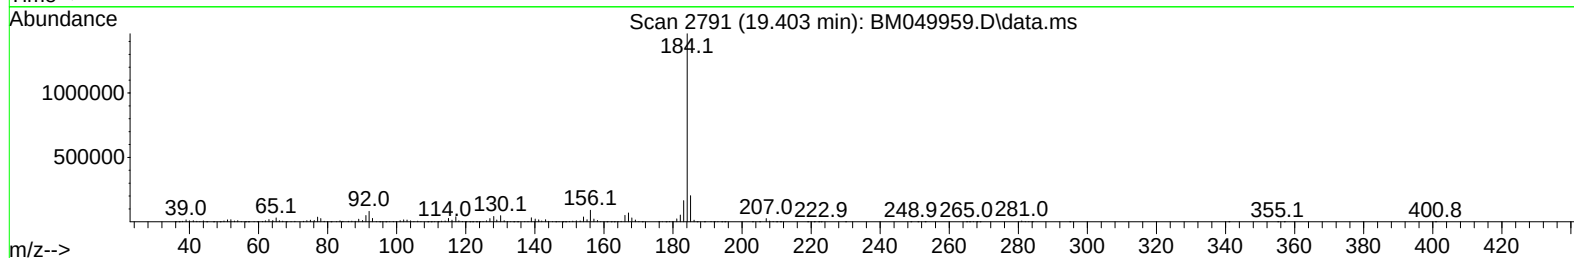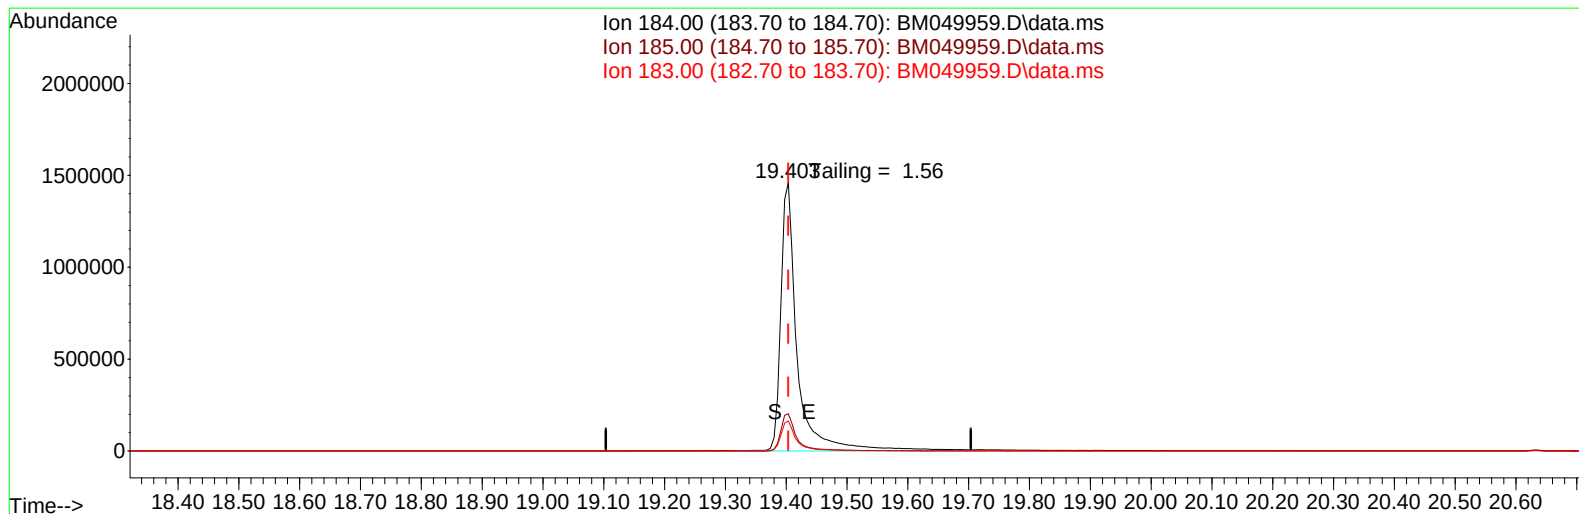

TIC: BM049959.D\data.ms

(77) Benzidine

19.403min (-0.000) 248612.04 ng

response 2724306

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.91
183.00	11.00	11.22
0.00	0.00	0.00