

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041919\
 Data File : BM019999.D
 Acq On : 20 Apr 2019 09:06
 Operator : JU/SJ
 Sample : K2475-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP-TRACK-74-75

Quant Time: Apr 21 22:08:49 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 19 00:56:08 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.50	152	87604	20.00	ng	0.00
21) Naphthalene-d8	10.29	136	323349	20.00	ng	0.00
39) Acenaphthene-d10	14.17	164	201176	20.00	ng	0.00
64) Phenanthrene-d10	16.94	188	475500	20.00	ng	0.00
76) Chrysene-d12	21.16	240	528315	20.00	ng	0.00
87) Perylene-d12	23.35	264	651291	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.12	112	715414	132.35	ng	-0.01
7) Phenol-d6	6.70	99	848707	104.33	ng	0.00
23) Nitrobenzene-d5	8.68	82	671086	92.82	ng	0.00
42) 2,4,6-Tribromophenol	15.69	330	448200	138.40	ng	0.00
45) 2-Fluorobiphenyl	12.78	172	1423605	88.19	ng	0.00
79) Terphenyl-d14	19.59	244	2984218	99.63	ng	0.00
Target Compounds						
9) Benzaldehyde	6.65	77	398	Below Cal	Qvalue #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041919\
Data File : BM019999.D
Acq On : 20 Apr 2019 09:06
Operator : JU/SJ
Sample : K2475-06
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-TRACK-74-75

Quant Time: Apr 21 22:08:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 19 00:56:08 2019
Response via : Initial Calibration

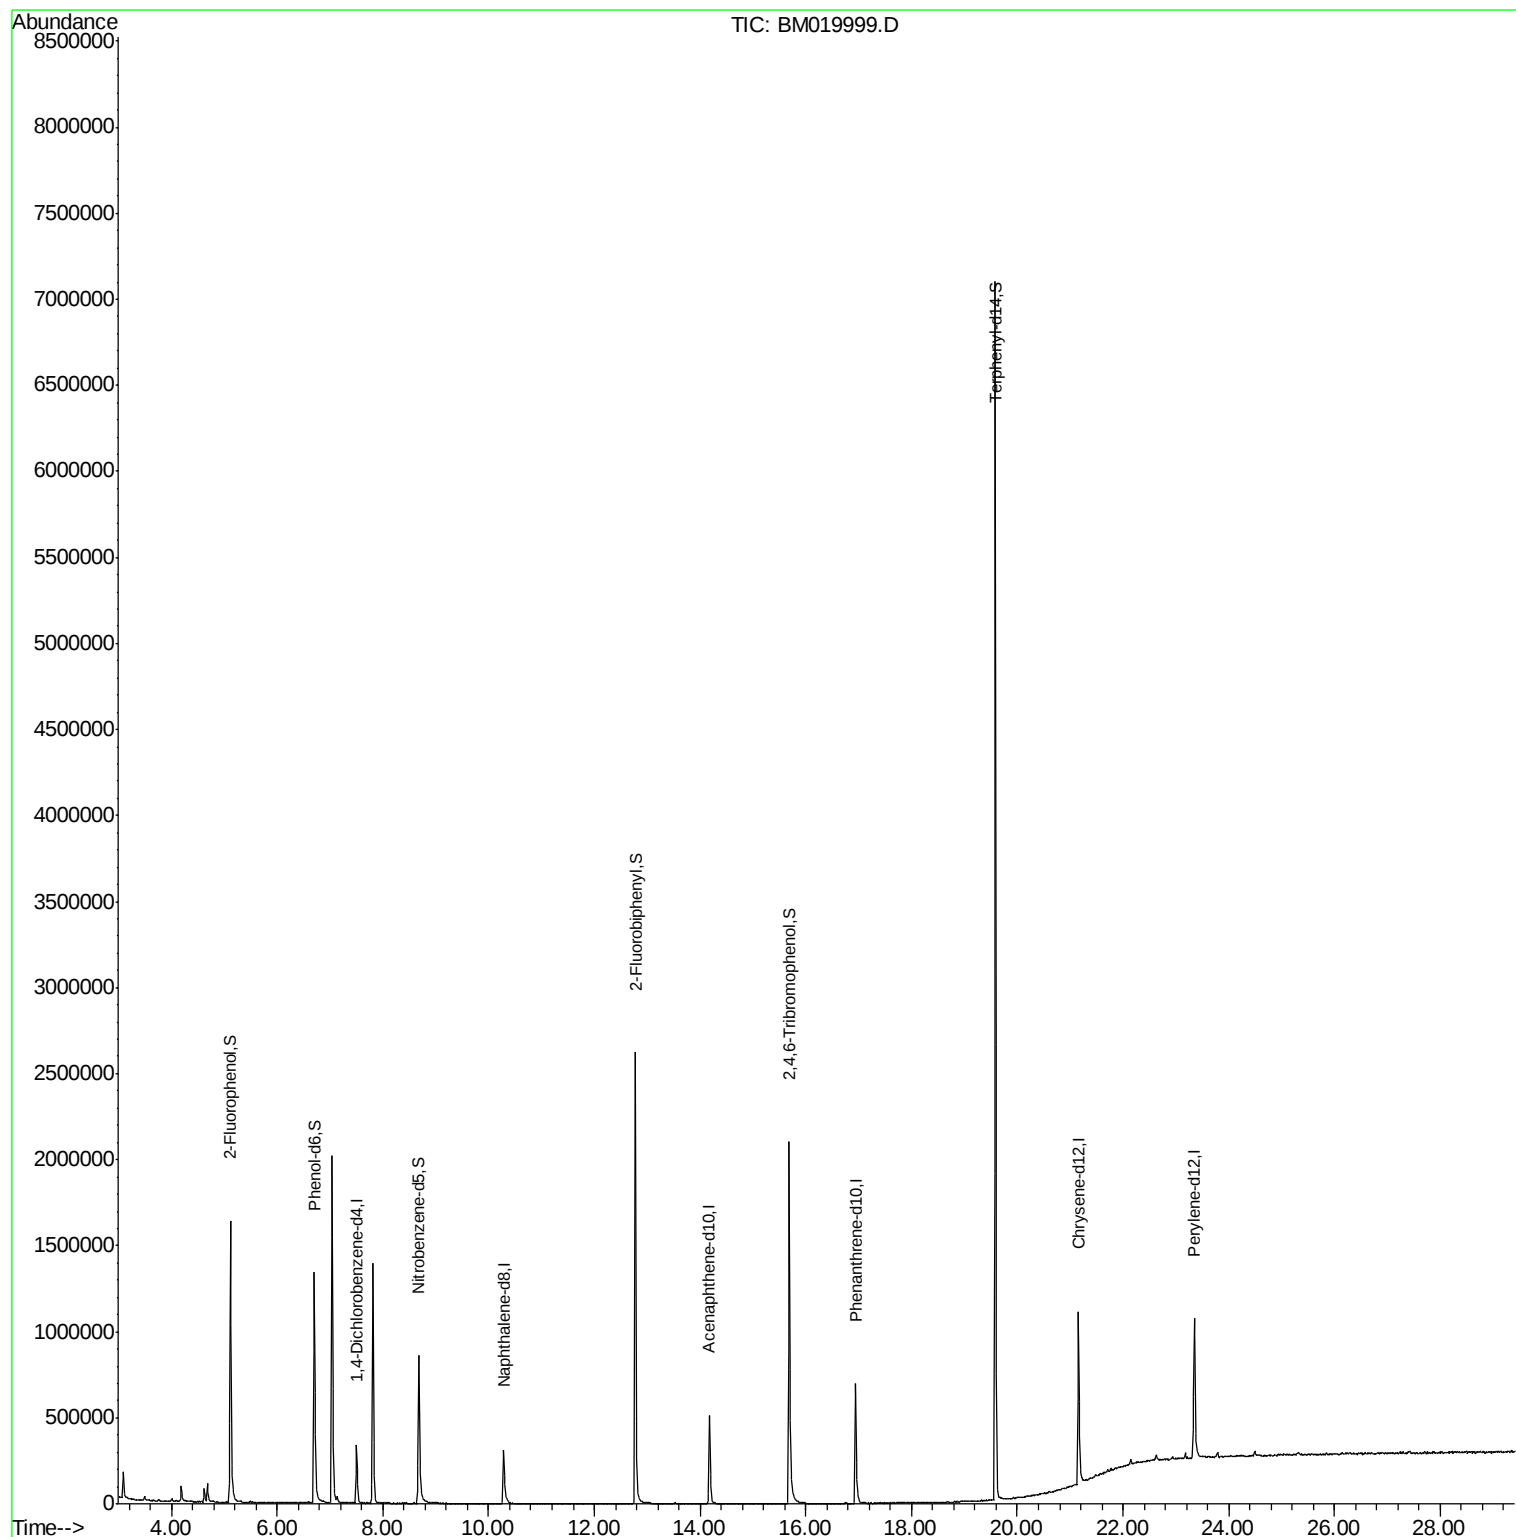

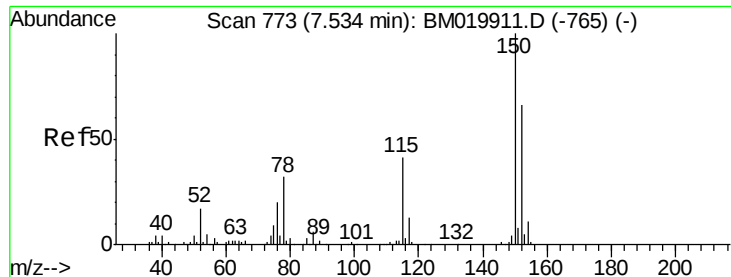


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.50 min Scan# 768
Delta R.T. -0.01 min
Lab File: BM019999.D
Acq: 20 Apr 2019 09:06

Instrument :
BNA_M
ClientSampleId :
TP-TRACK-74-75

Tgt Ion:152 Resp: 87604
Ion Ratio Lower Upper
152 100
150 155.1 122.1 183.1
115 65.9 50.0 75.0

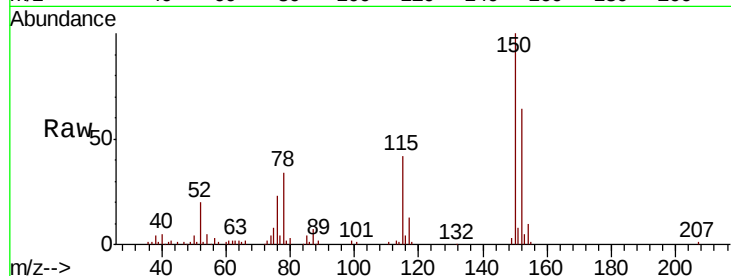


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

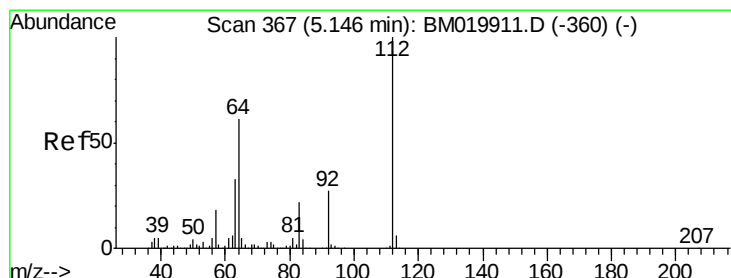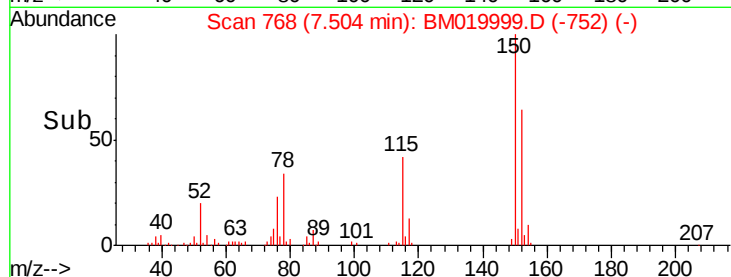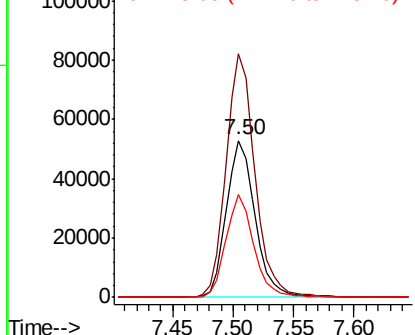



#5


2-Fluorophenol
Concen: 132.350 ng
RT: 5.12 min Scan# 362
Delta R.T. -0.01 min
Lab File: BM019999.D
Acq: 20 Apr 2019 09:06

Tgt Ion:112 Resp: 715414
Ion Ratio Lower Upper
112 100
64 65.3 49.1 73.7
63 35.8 26.5 39.7

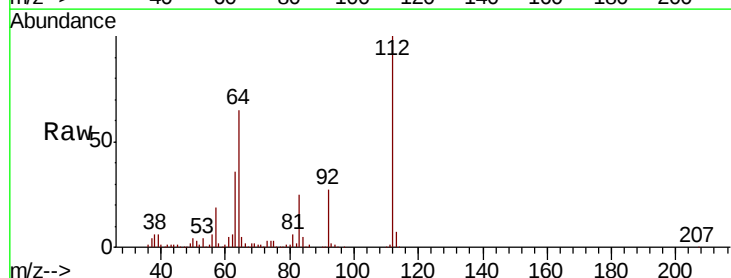

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

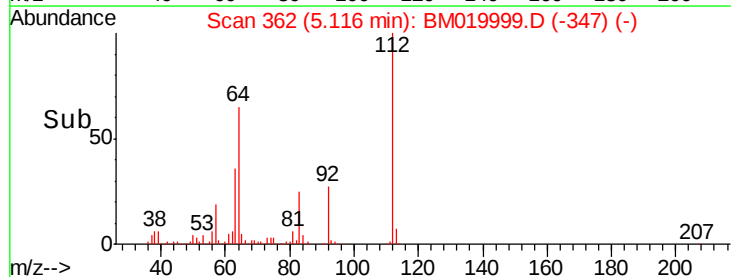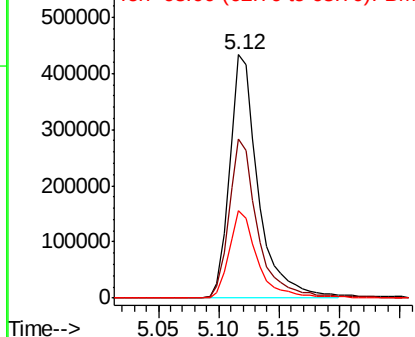

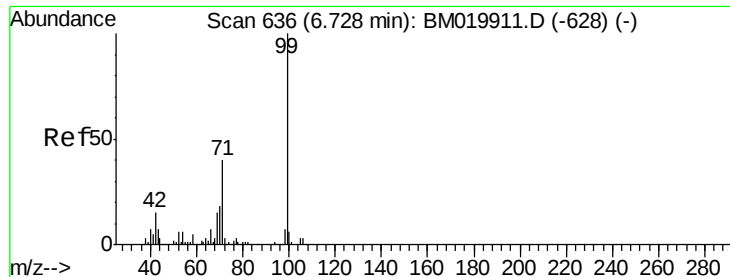

#7

Phenol-d6

Concen: 104.326 ng

RT: 6.70 min Scan# 632

Delta R.T. -0.01 min

Lab File: BM019999.D

Acq: 20 Apr 2019 09:06

Instrument :

BNA_M

ClientSampleId :

TP-TRACK-74-75


Tgt Ion: 99 Resp: 848707

Ion Ratio Lower Upper

99 100

42 15.6 11.8 17.8

71 43.1 32.0 48.0



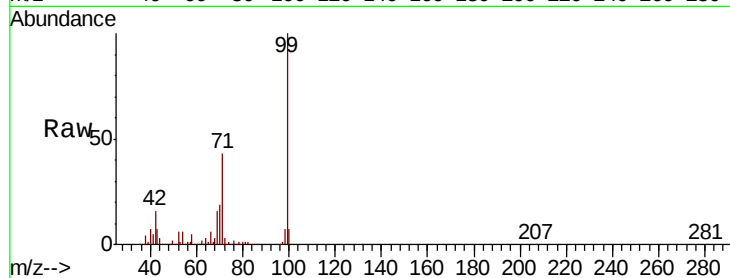


Abundance

Ion 99.00 (98.70 to 99.70): BM019911.D (-628) (-)

Ion 42.00 (41.70 to 42.70): BM019911.D (-628) (-)

Ion 71.00 (70.70 to 71.70): BM019911.D (-628) (-)

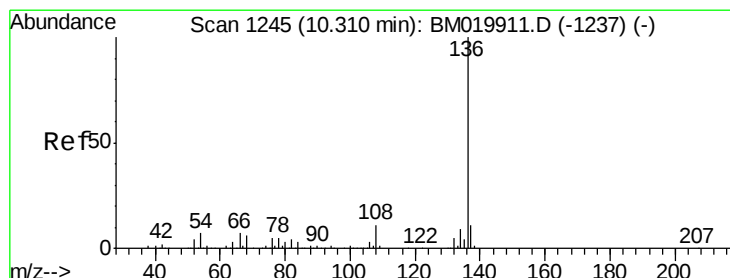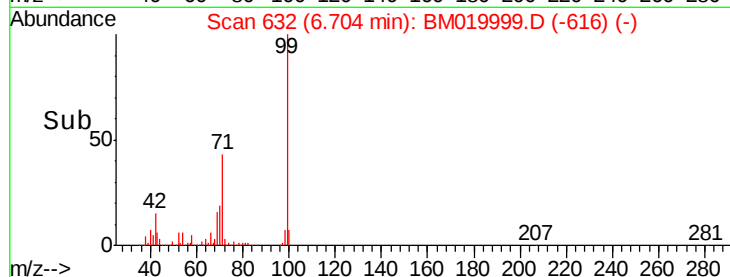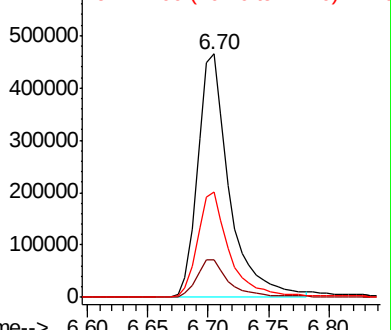

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.29 min Scan# 1241

Delta R.T. 0.00 min

Lab File: BM019999.D

Acq: 20 Apr 2019 09:06

Tgt Ion: 136 Resp: 323349


Ion Ratio Lower Upper

136 100

137 11.2 9.0 13.6

54 6.8 5.3 7.9

68 6.3 5.2 7.8

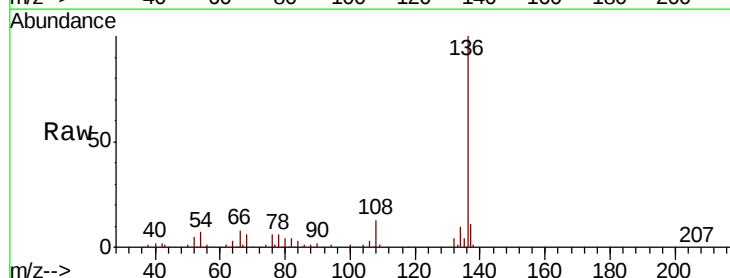



Abundance


Ion 136.00 (135.70 to 136.70): BM019911.D (-1237) (-)

Ion 137.00 (136.70 to 137.70): BM019911.D (-1237) (-)

Ion 54.00 (53.70 to 54.70): BM019911.D (-1237) (-)

Ion 68.00 (67.70 to 68.70): BM019911.D (-1237) (-)



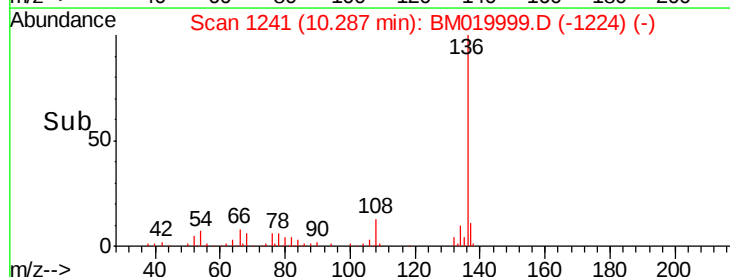
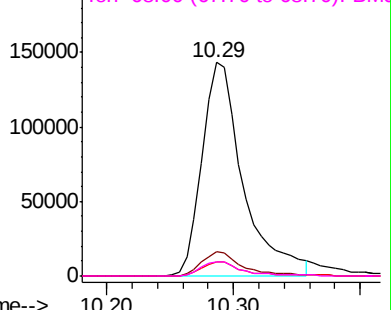


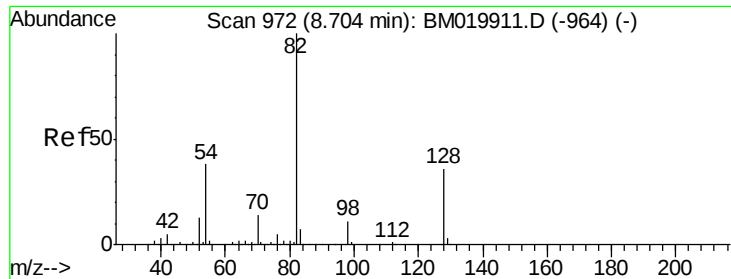

#23
 Nitrobenzene-d5
 Concen: 92.815 ng
 RT: 8.68 min Scan# 968
 Delta R.T. -0.01 min
 Lab File: BM019999.D
 Acq: 20 Apr 2019 09:06




Instrument :
 BNA_M
 ClientSampleId :
 TP-TRACK-74-75


Tgt Ion	Ratio	Lower	Upper
82	100		
128	35.6	29.0	43.4
54	39.1	30.2	45.4

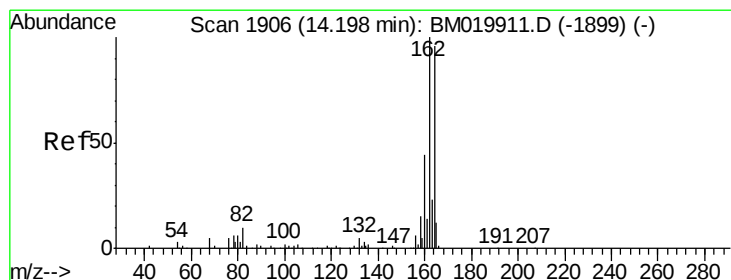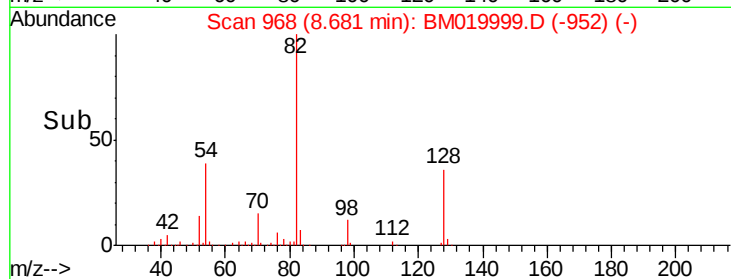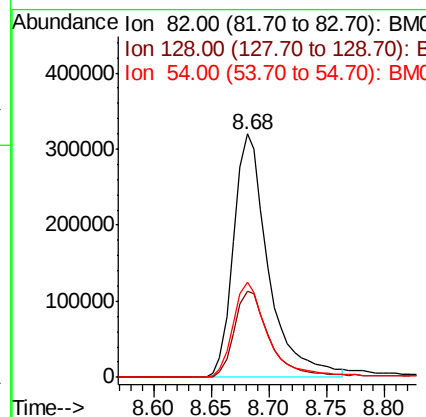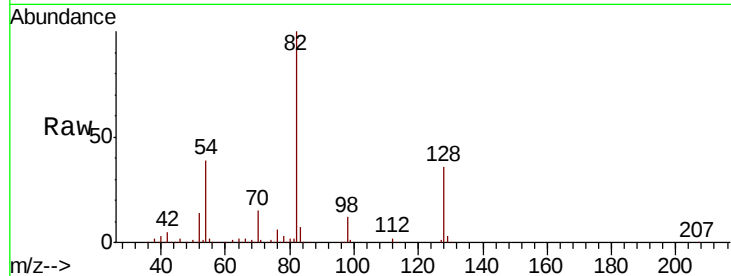

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.17 min Scan# 1902
 Delta R.T. 0.00 min
 Lab File: BM019999.D
 Acq: 20 Apr 2019 09:06

Tgt Ion	Ratio	Lower	Upper
164	100		
162	106.9	83.0	124.4
160	46.6	36.6	55.0

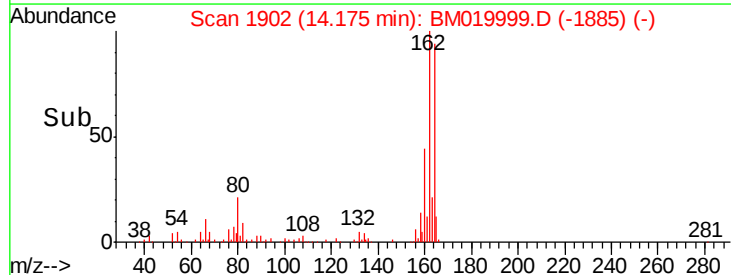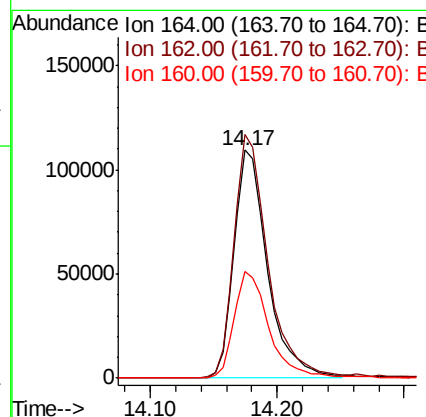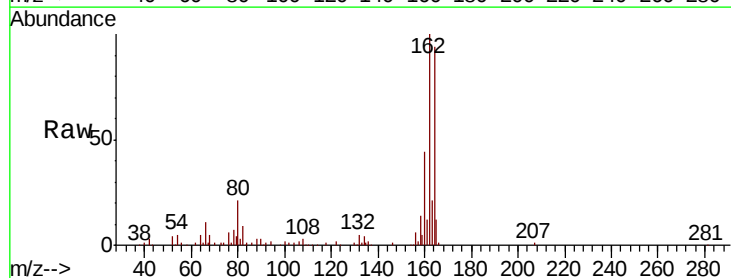


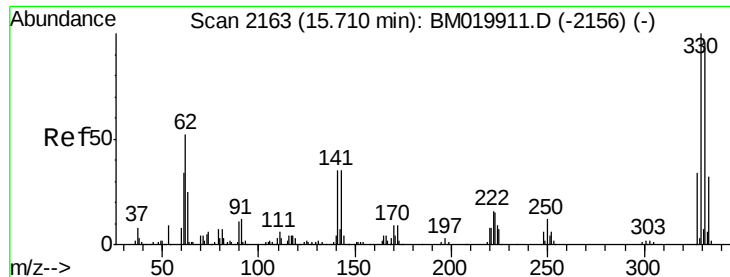




#42
 2,4,6-Tribromophenol
 Concen: 138.403 ng
 RT: 15.69 min Scan# 2159
 Delta R.T. -0.01 min
 Lab File: BM019999.D
 Acq: 20 Apr 2019 09:06

Instrument :
 BNA_M
 ClientSampleId :
 TP-TRACK-74-75

Tgt Ion: 330 Resp: 448200
 Ion Ratio Lower Upper
 330 100
 332 97.0 77.4 116.2
 141 39.2 29.0 43.4

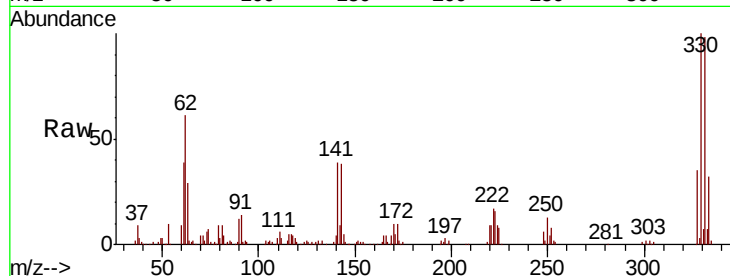


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

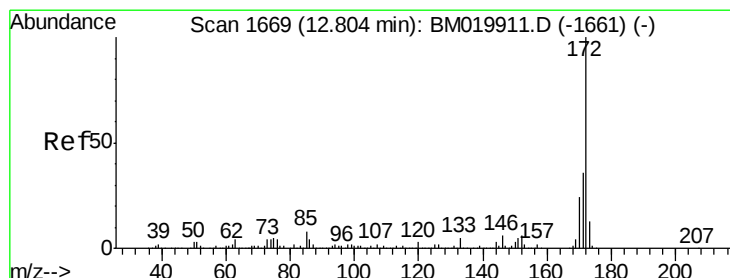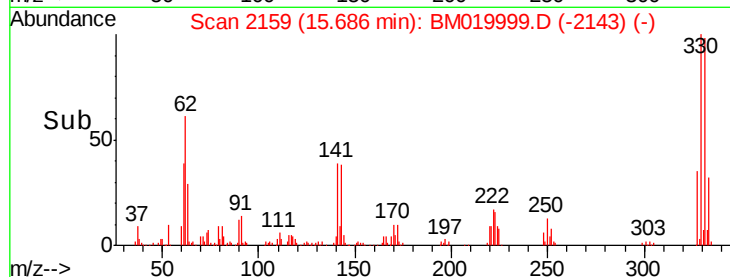
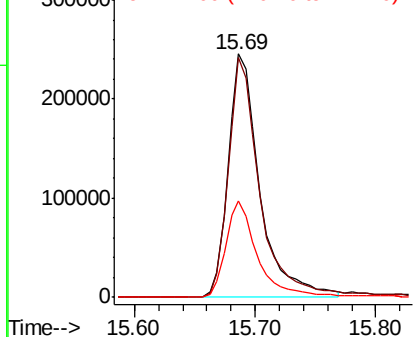


#45
 2-Fluorobiphenyl
 Concen: 88.189 ng
 RT: 12.78 min Scan# 1665
 Delta R.T. -0.01 min
 Lab File: BM019999.D
 Acq: 20 Apr 2019 09:06

Tgt Ion: 172 Resp: 1423605
 Ion Ratio Lower Upper
 172 100
 171 35.7 28.9 43.3
 170 23.1 19.0 28.4

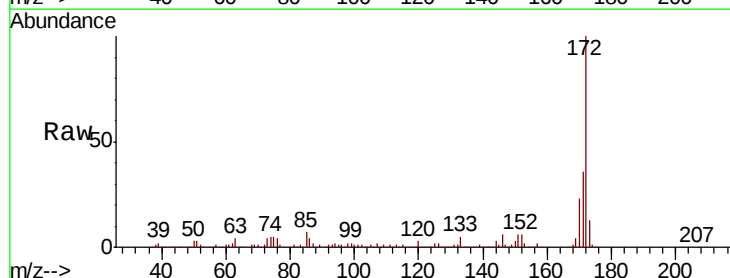

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

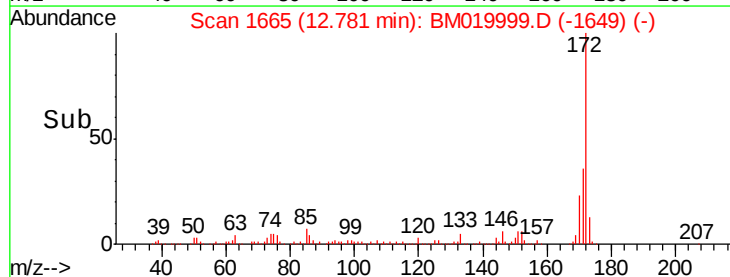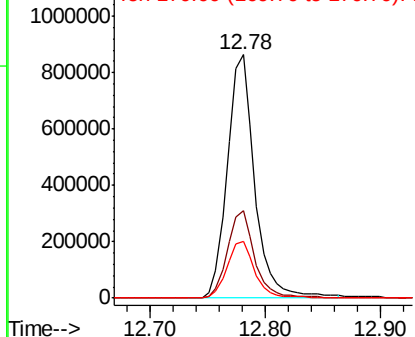



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 16.94 min Scan# 2373

Delta R.T. 0.00 min

Lab File: BM019999.D

Acq: 20 Apr 2019 09:06

Instrument :

BNA_M

ClientSampleId :

TP-TRACK-74-75


Tgt Ion:188 Resp: 475500

Ion Ratio Lower Upper

188 100

94 8.4 7.6 11.4




80 10.5 9.4 14.0

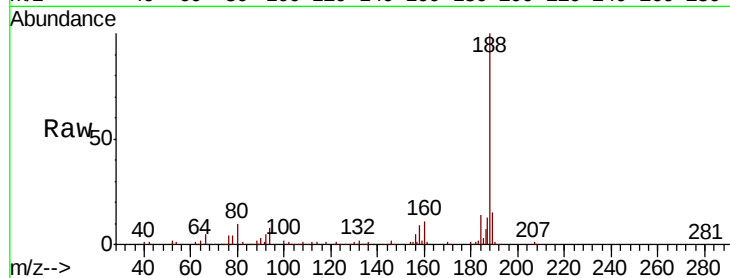

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

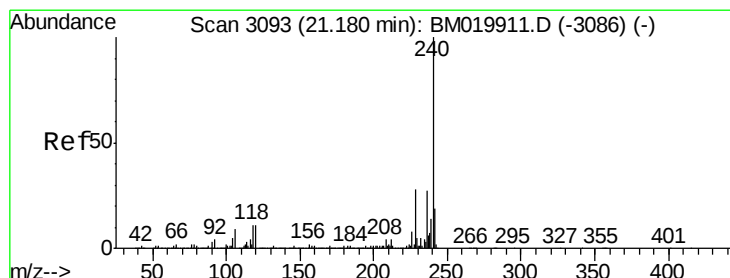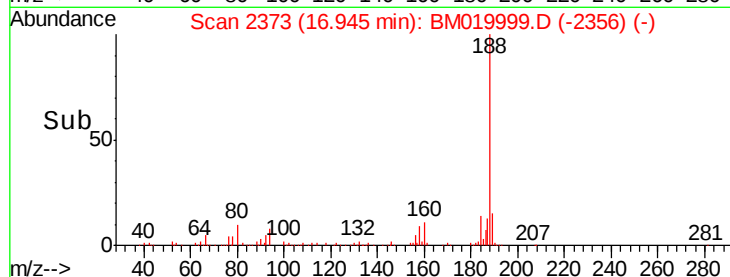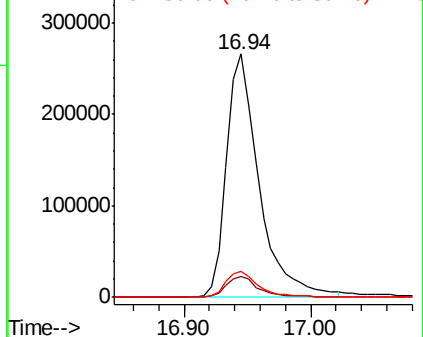

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.16 min Scan# 3090

Delta R.T. 0.00 min

Lab File: BM019999.D

Acq: 20 Apr 2019 09:06


Tgt Ion:240 Resp: 528315

Ion Ratio Lower Upper

240 100

120 10.3 8.6 13.0



236 26.8 21.4 32.2

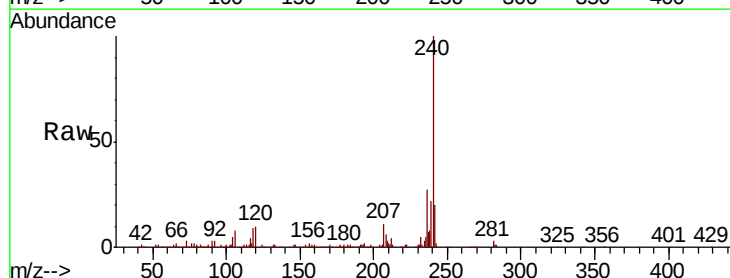


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

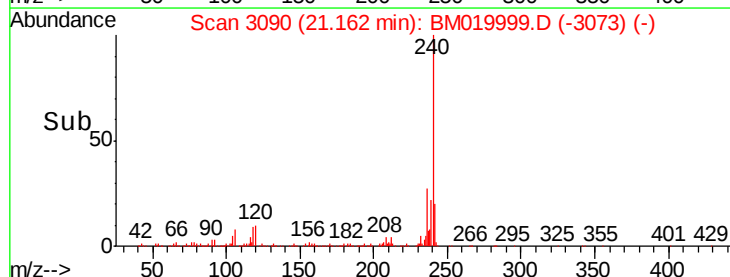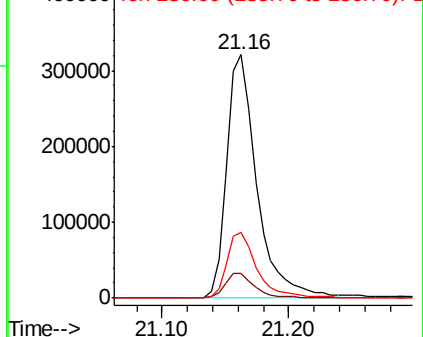

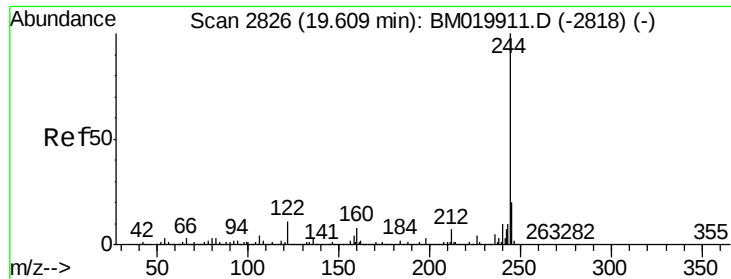

#79

Terphenyl-d14

Concen: 99.631 ng

RT: 19.59 min Scan# 2822

Delta R.T. -0.01 min

Lab File: BM019999.D

Acq: 20 Apr 2019 09:06

Instrument :

BNA_M

ClientSampleId :

TP-TRACK-74-75


Tgt Ion:244 Resp: 2984218

Ion Ratio Lower Upper

244 100

212 7.4 5.7 8.5




122 11.0 9.1 13.7

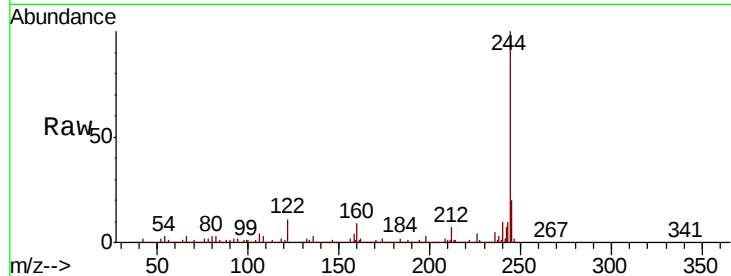

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

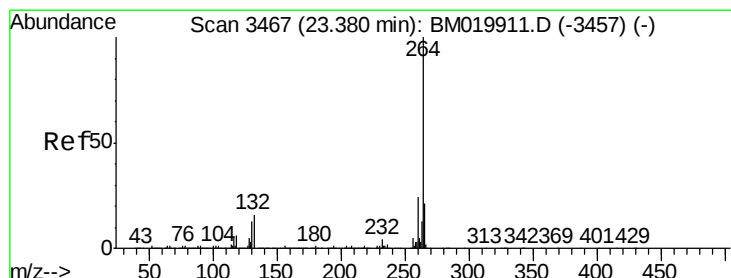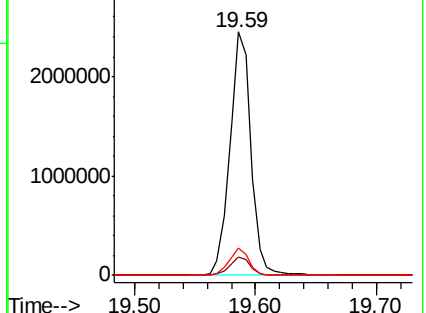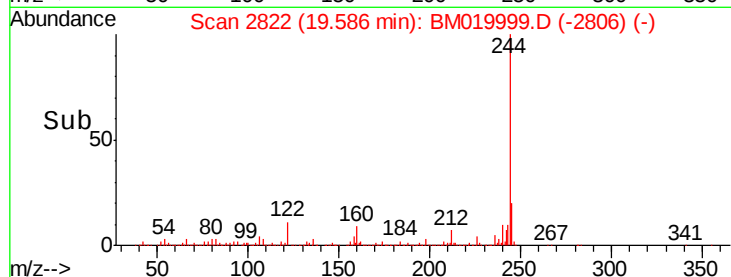

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.35 min Scan# 3462

Delta R.T. 0.00 min

Lab File: BM019999.D

Acq: 20 Apr 2019 09:06


Tgt Ion:264 Resp: 651291

Ion Ratio Lower Upper

264 100

260 24.1 19.2 28.8

265 21.8 17.2 25.8

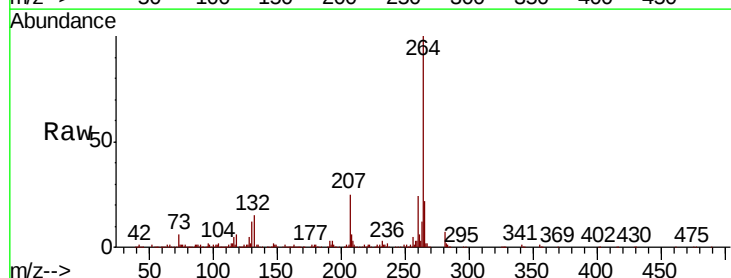

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

