

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041919\
 Data File : BM020002.D
 Acq On : 20 Apr 2019 10:55
 Operator : JU/SJ
 Sample : K2487-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 FB

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.122	357	363	386	rBV	600945	1168239	14.55%	3.784%
2	6.710	626	633	654	rBV	308565	734728	9.15%	2.380%
3	7.040	683	689	710	rBV	1381106	2457909	30.61%	7.962%
4	7.504	760	768	779	rBV	286977	486430	6.06%	1.576%
5	7.816	814	821	835	rBV	1263656	2119278	26.39%	6.865%
6	8.681	961	968	999	rBV	778831	1750416	21.80%	5.670%
7	10.292	1233	1242	1263	rBV	270696	646799	8.05%	2.095%
8	12.775	1658	1664	1682	rBV	2519512	4276409	53.26%	13.853%
9	14.180	1896	1903	1919	rBV2	458204	911063	11.35%	2.951%
10	15.686	2153	2159	2187	rBV	2098064	3776931	47.04%	12.235%
11	16.945	2367	2373	2395	rBV2	613467	1148907	14.31%	3.722%
12	19.586	2816	2822	2834	rBV	6638045	8029929	100.00%	26.012%
13	21.162	3085	3090	3103	rBV	1005552	1586400	19.76%	5.139%
14	23.350	3456	3462	3478	rVB	826633	1776075	22.12%	5.753%


Sum of corrected areas: 30869513

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041919\
Data File : BM020002.D
Acq On : 20 Apr 2019 10:55
Operator : JU/SJ
Sample : K2487-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

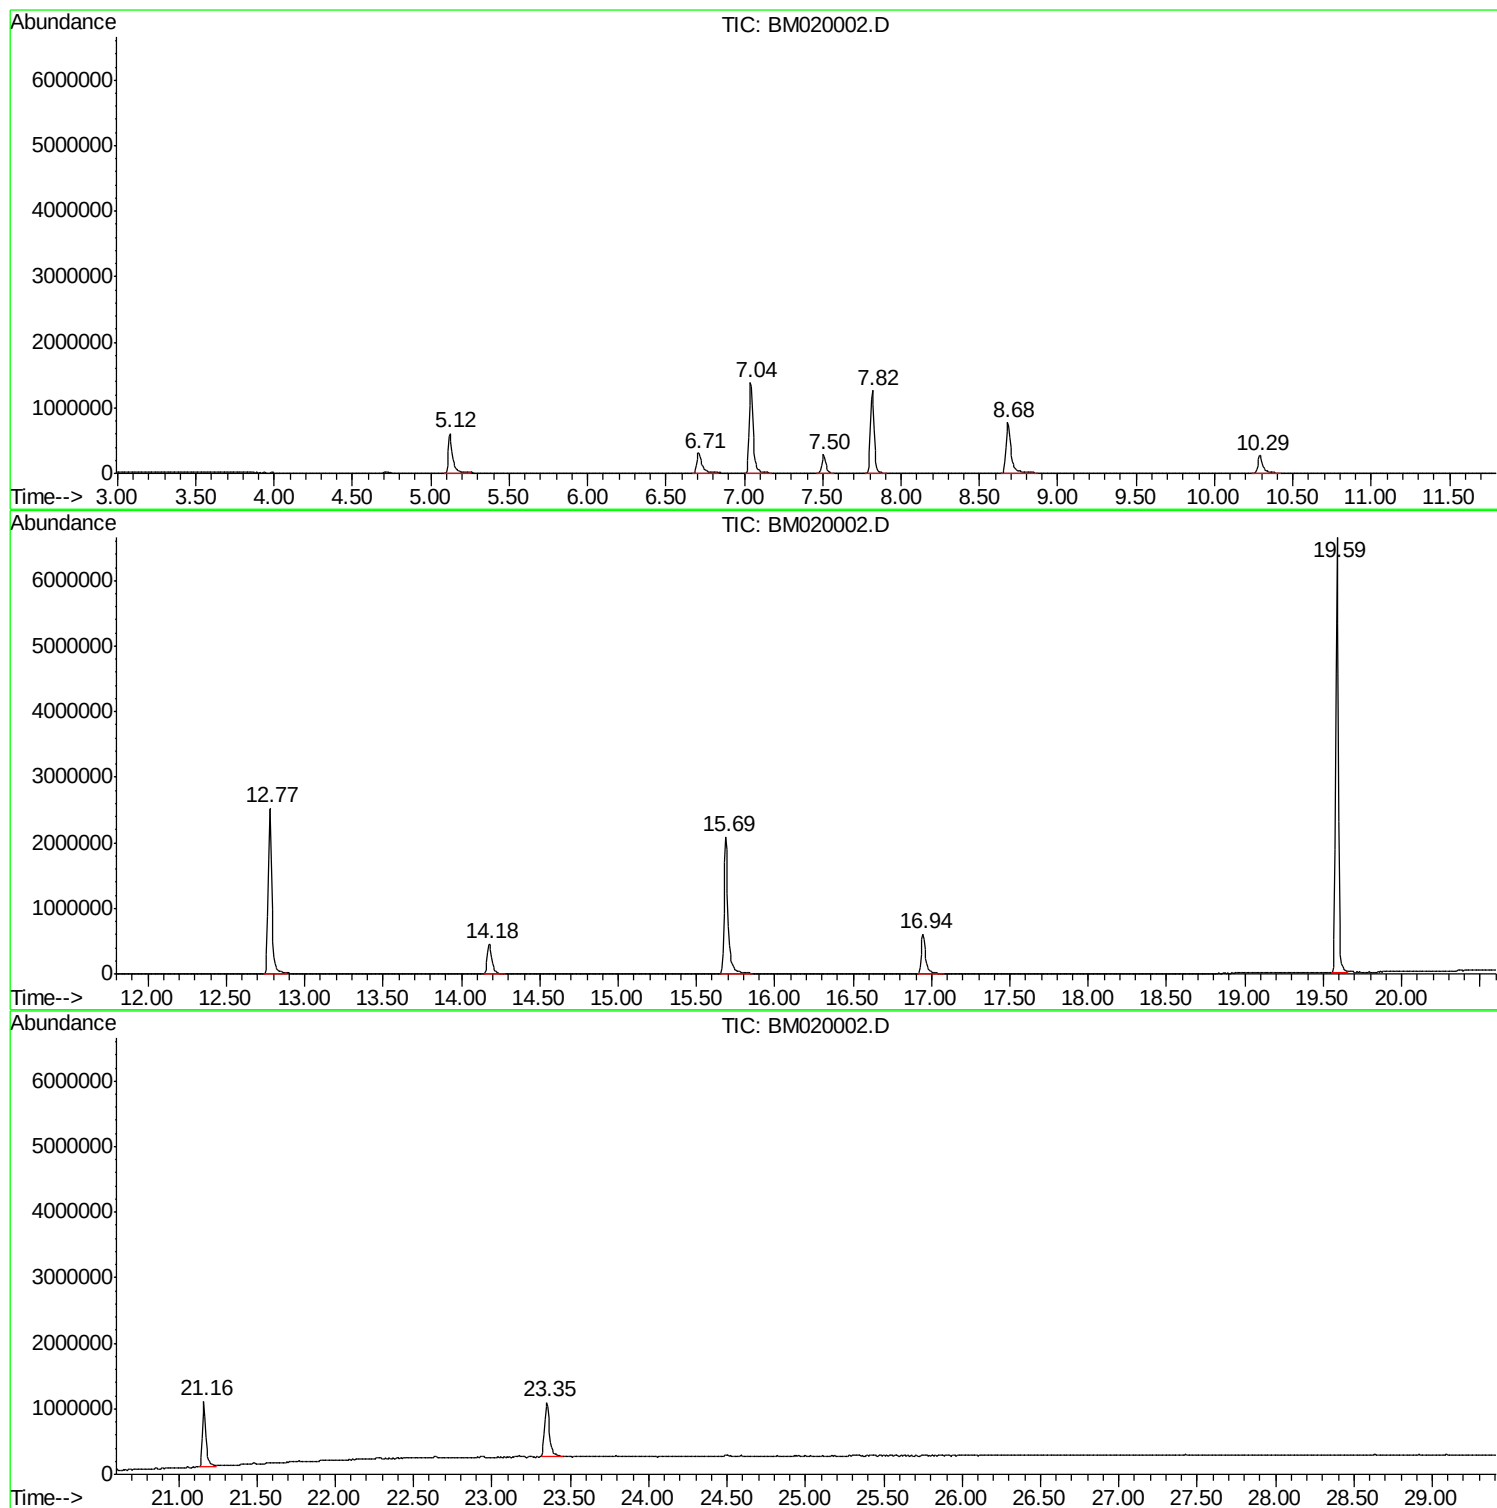

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041919\
Data File : BM020002.D
Acq On : 20 Apr 2019 10:55
Operator : JU/SJ
Sample : K2487-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.04 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.04	101.06 ng	2457910	1,4-Dichlorobenzene-d4	7.50

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
5		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	10

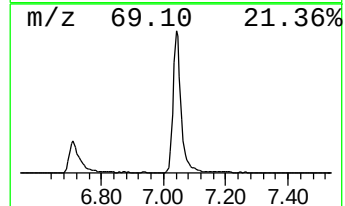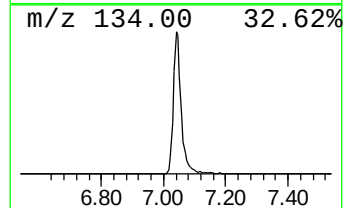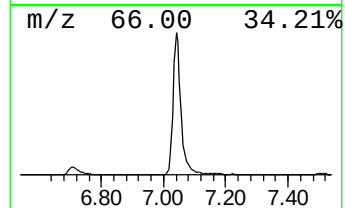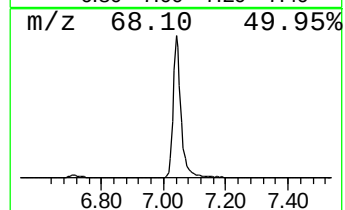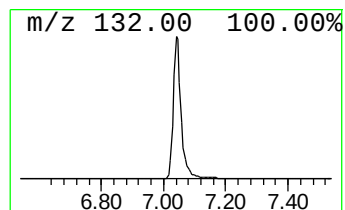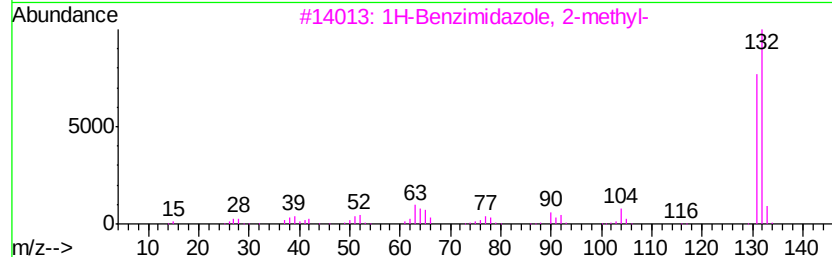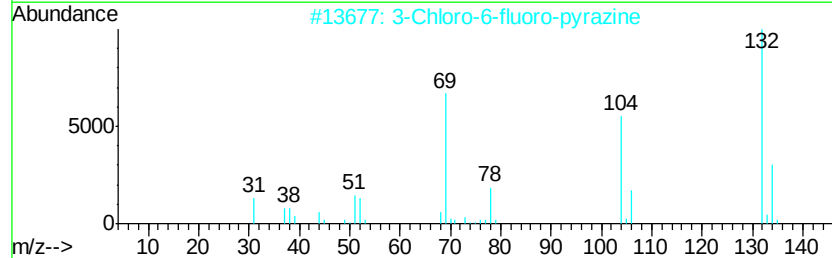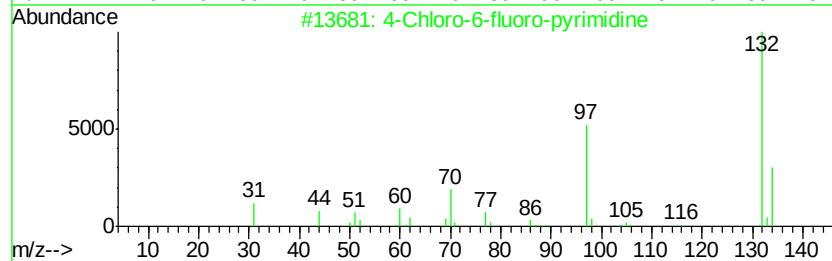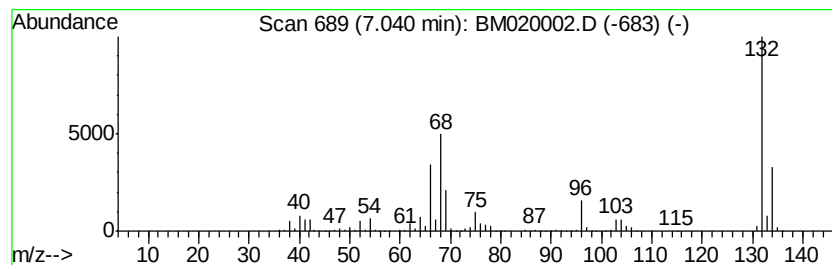

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041919\
Data File : BM020002.D
Acq On : 20 Apr 2019 10:55
Operator : JU/SJ
Sample : K2487-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.04	7.04	101.1	ng	2457910	1	7.50	486430	20.0