


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041919\
 Data File : BM019972.D
 Acq On : 19 Apr 2019 13:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 19 00:56:08 2019

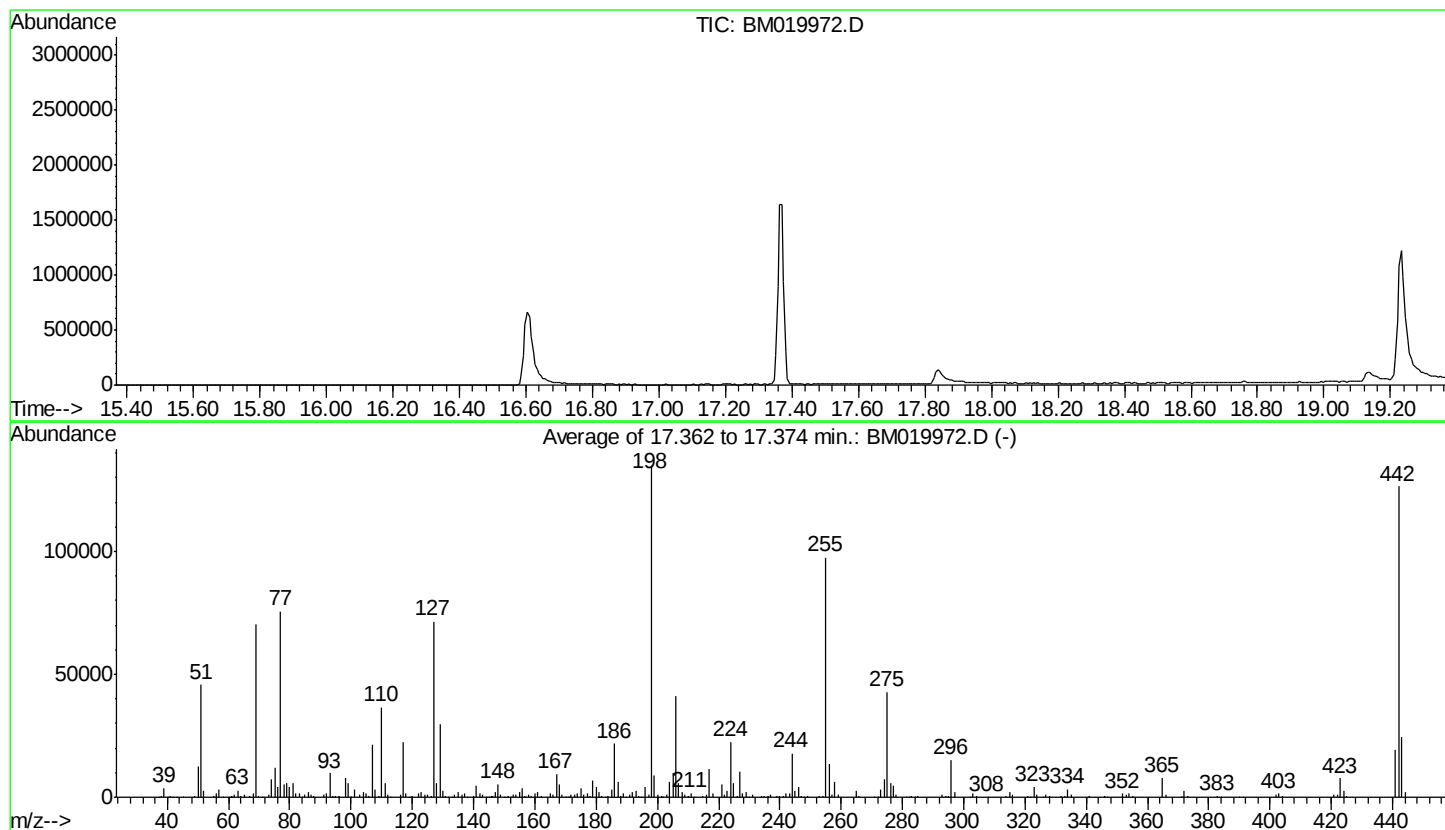

AutoFind: Scans 2444, 2445, 2446; Background Corrected with Scan 2438

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	45653	PASS
68	69	0.00	2	2.0	1439	PASS
69	198	0.00	100	52.2	70460	PASS
70	69	0.00	2	0.8	549	PASS
127	198	10	80	52.9	71445	PASS
197	198	0.00	2	0.7	927	PASS
198	198	100	100	100.0	134957	PASS
199	198	5	9	6.7	9014	PASS
275	198	10	60	31.8	42930	PASS
365	198	1	100	5.8	7878	PASS
441	198	0.01	100	14.3	19264	PASS
442	198	50	100	93.6	126357	PASS
443	442	15	24	19.2	24293	PASS