


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM041919\
 Data File : BM019989.D
 Acq On : 20 Apr 2019 03:02
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 19 00:56:08 2019

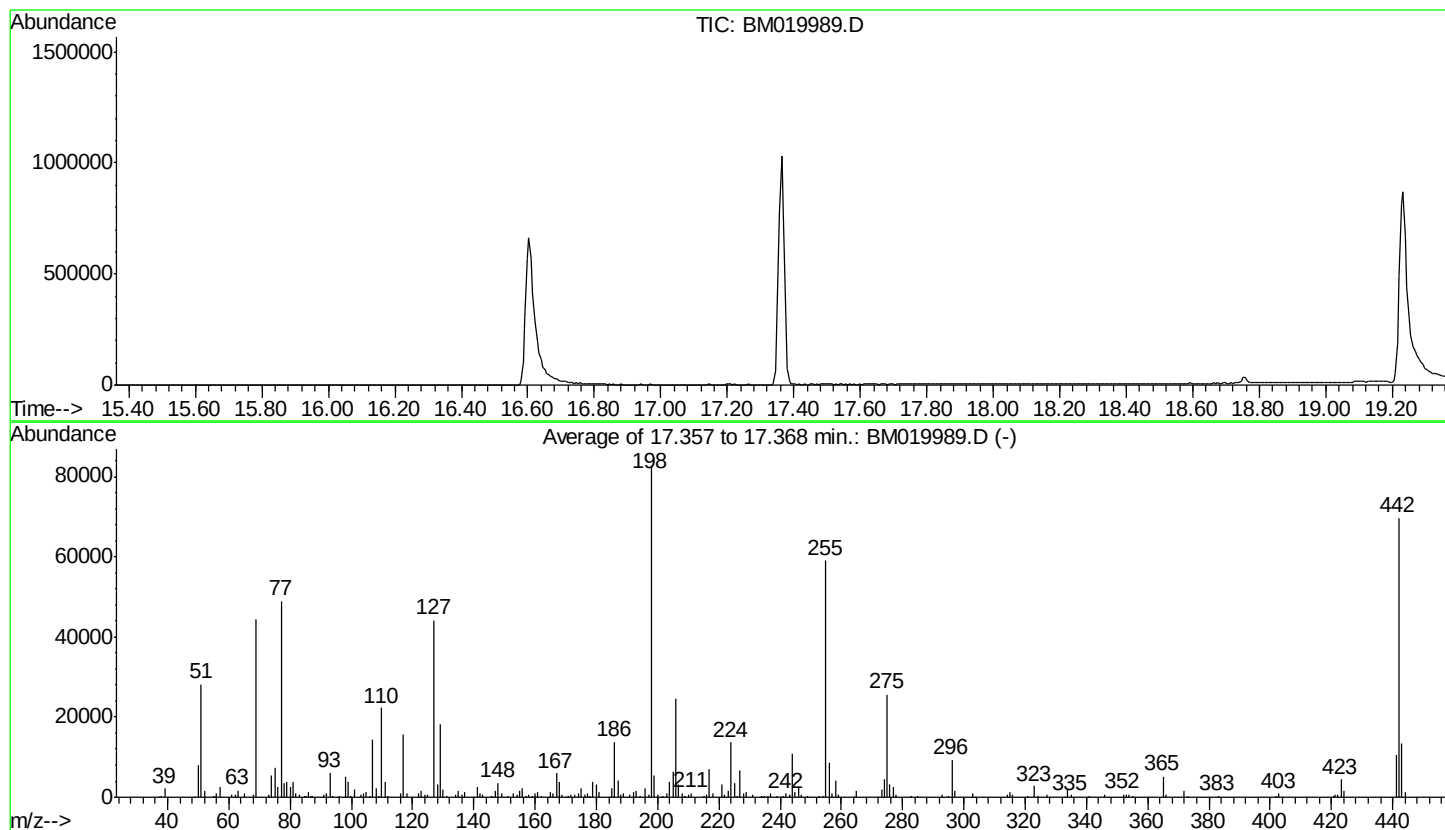

AutoFind: Scans 2443, 2444, 2445; Background Corrected with Scan 2437

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	28242	PASS
68	69	0.00	2	1.8	789	PASS
69	198	0.00	100	53.8	44504	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.5	44224	PASS
197	198	0.00	2	0.8	672	PASS
198	198	100	100	100.0	82725	PASS
199	198	5	9	6.4	5325	PASS
275	198	10	60	31.0	25626	PASS
365	198	1	100	6.2	5118	PASS
441	198	0.01	100	12.9	10696	PASS
442	198	50	100	84.2	69621	PASS
443	442	15	24	19.5	13556	PASS