




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
Data File : BM034745.D
Acq On : 21 Apr 2022 13:54
Operator : CG/JU
Sample : N2472-20
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0J37

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:16:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 05:03:15 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/22/2022
Supervised By :mohammad ahmed 04/26/2022

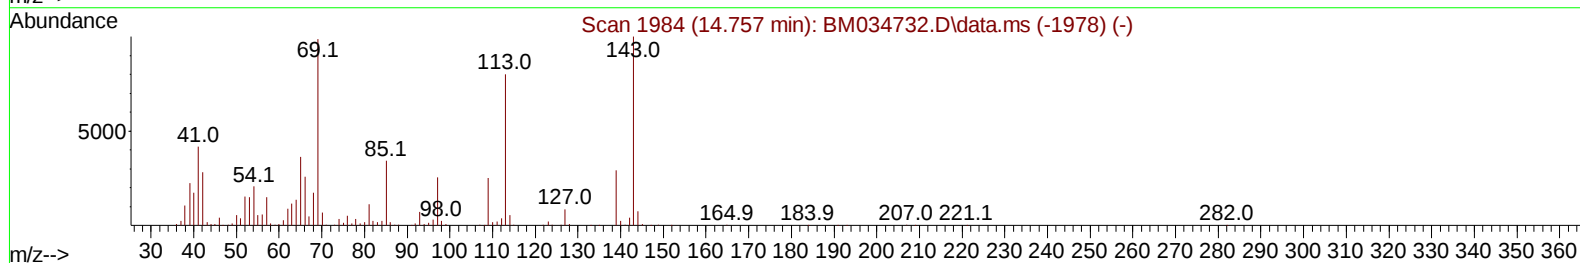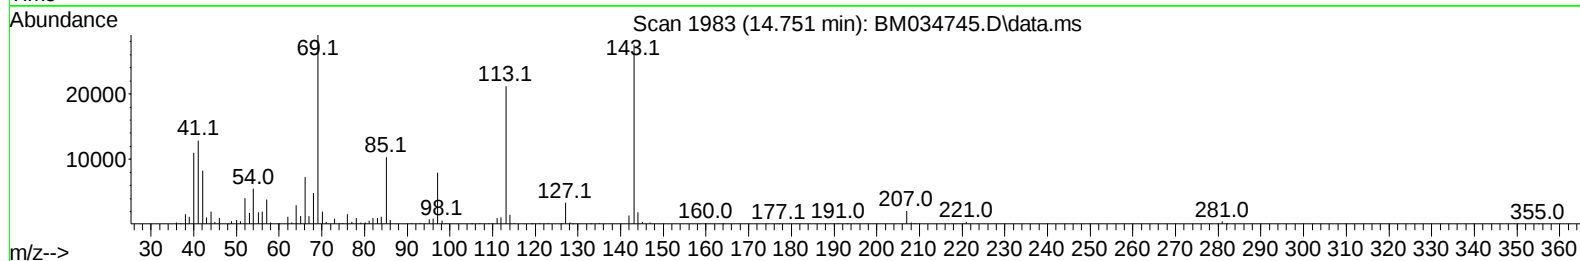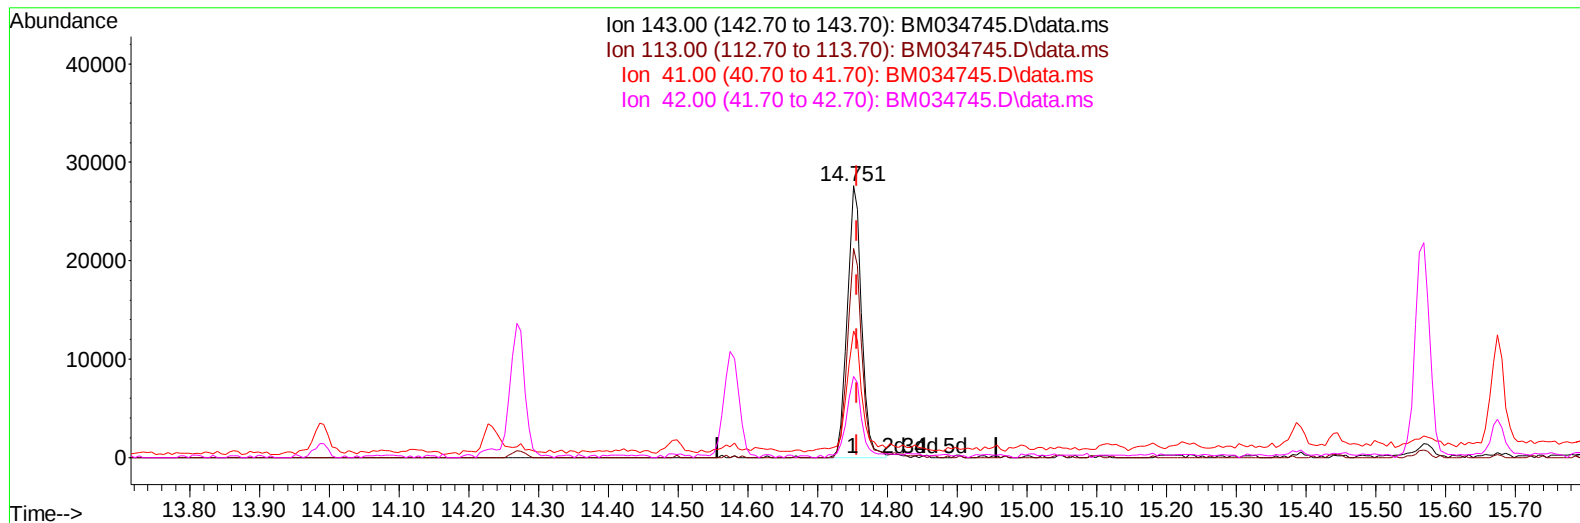

TIC: BM034745.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.751min (-0.006) 6.84 ng/u1

response 39501

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.00	76.89
41.00	42.20	46.65
42.00	28.30	29.85




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
 Data File : BM034745.D
 Acq On : 21 Apr 2022 13:54
 Operator : CG/JU
 Sample : N2472-20
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0J37

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/22/2022
 Supervised By :mohammad ahmed 04/26/2022

Quant Time: Apr 22 01:16:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 05:03:15 2022
 Response via : Initial Calibration

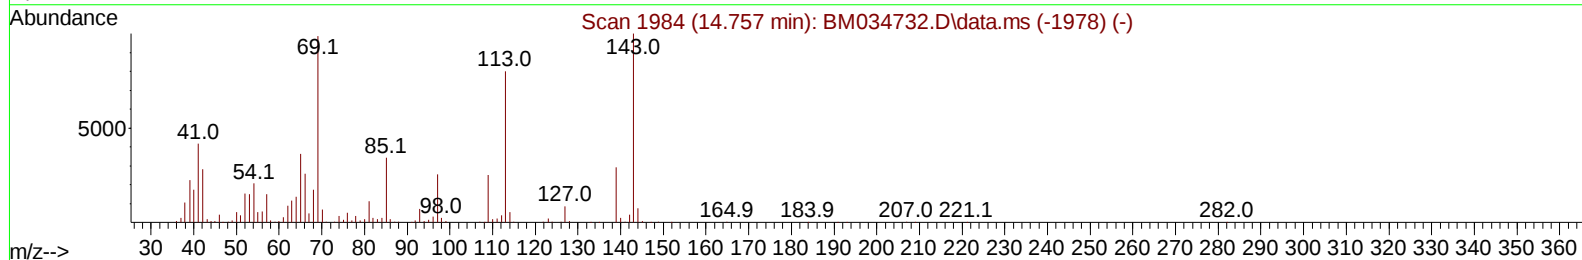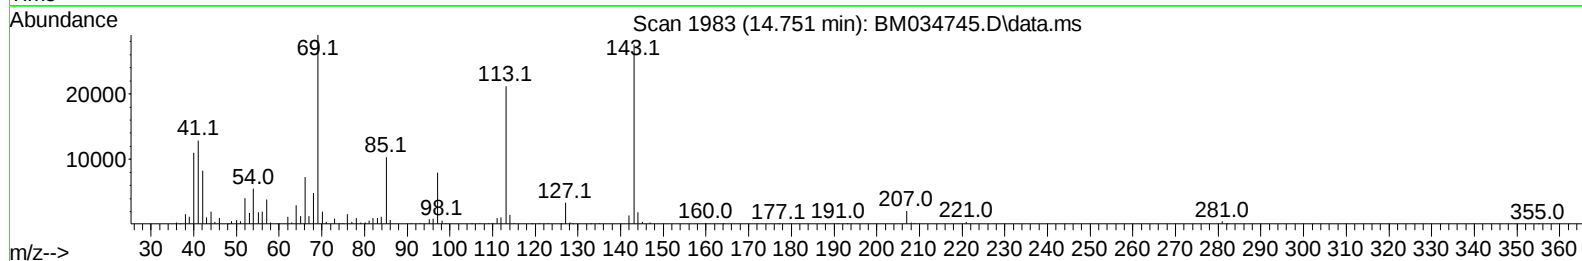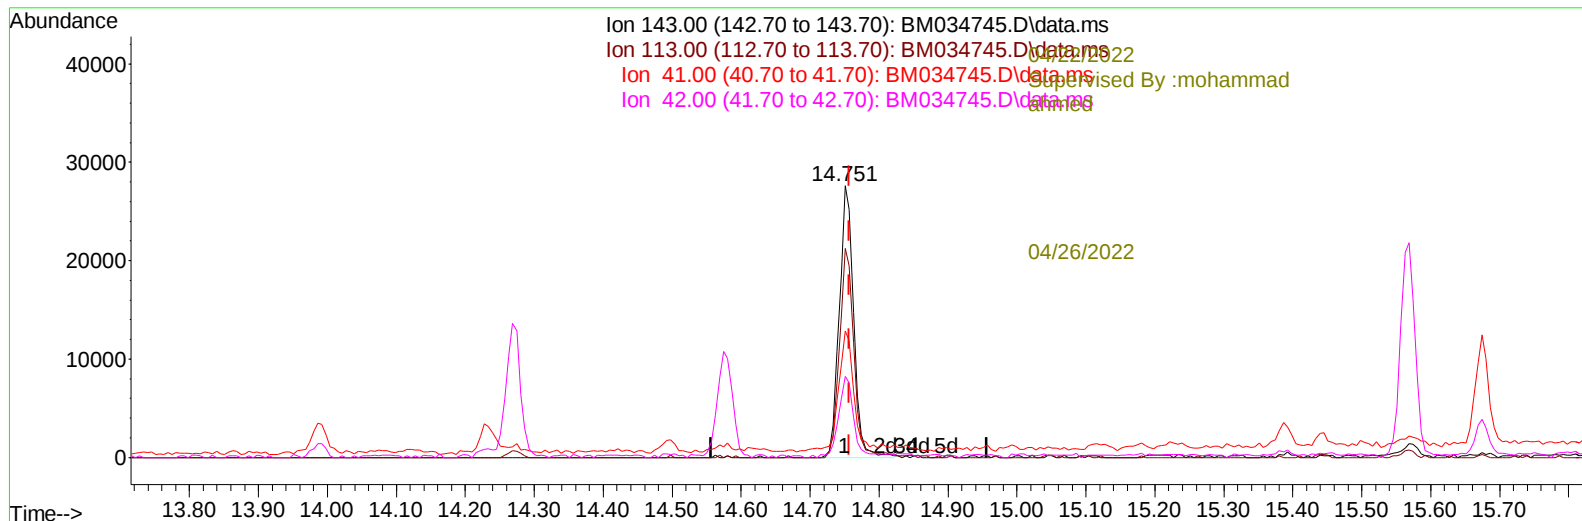

TIC: BM034745.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.751min (-0.006) 6.91 ng/ul m

response 39904

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.00	76.89
41.00	42.20	46.65
42.00	28.30	29.85

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
 Data File : BM034745.D
 Acq On : 21 Apr 2022 13:54
 Operator : CG/JU
 Sample : N2472-20
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0J37

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/22/2022
 Supervised By :mohammad ahmed 04/26/2022

Quant Time: Apr 22 01:16:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 05:03:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----04/22/2022						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	194365	20.000	ng/ul	0.00
20) Naphthalene-d8	10.751	136	765107	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	472290	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.316	188	940423	20.000	ng/ul	0.00
79) Chrysene-d12	21.492	240	901645	20.000	ng/ul	0.00
88) Perylene-d12	23.892	264	930771	20.000	ng/ul	0.00
-----04/26/2022						
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	23094	5.221	ng/uL	0.00
4) Pyridine-d5	3.799	84	107162	9.760	ng/ul	0.00
7) Phenol-d5	7.104	99	110152	7.503	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	287245	34.890	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	326819	26.304	ng/ul	0.00
15) 4-Methylphenol-d8	8.651	113	200597	17.078	ng/ul	0.00
21) Nitrobenzene-d5	9.104	128	182685	32.686	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	186804	32.191	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	334987	27.405	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131	473616	28.655	ng/ul	0.00
46) Dimethylphthalate-d6	13.986	166	1224594	35.617	ng/ul	0.00
49) Acenaphthylene-d8	14.269	160	1422987	32.181	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	39904m	6.914	ng/ul	0.00
60) Fluorene-d10	15.569	176	1080322	36.312	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.674	200	150151	27.830	ng/ul	0.00
73) Anthracene-d10	17.416	188	1711909	37.383	ng/ul	0.00
81) Pyrene-d10	19.704	212	1936691	39.466	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.739	264	1891105	40.172	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
Data File : BM034745.D
Acq On : 21 Apr 2022 13:54
Operator : CG/JU
Sample : N2472-20
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0J37

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/22/2022
Supervised By :mohammad ahmed 04/26/2022

Quant Time: Apr 22 01:16:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 05:03:15 2022
Response via : Initial Calibration

