




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
Data File : BM034747.D
Acq On : 21 Apr 2022 15:06
Operator : CG/JU
Sample : N2472-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0J17

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/22/2022
Supervised By :mohammad ahmed 04/26/2022

Quant Time: Apr 22 01:21:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 05:03:15 2022
Response via : Initial Calibration

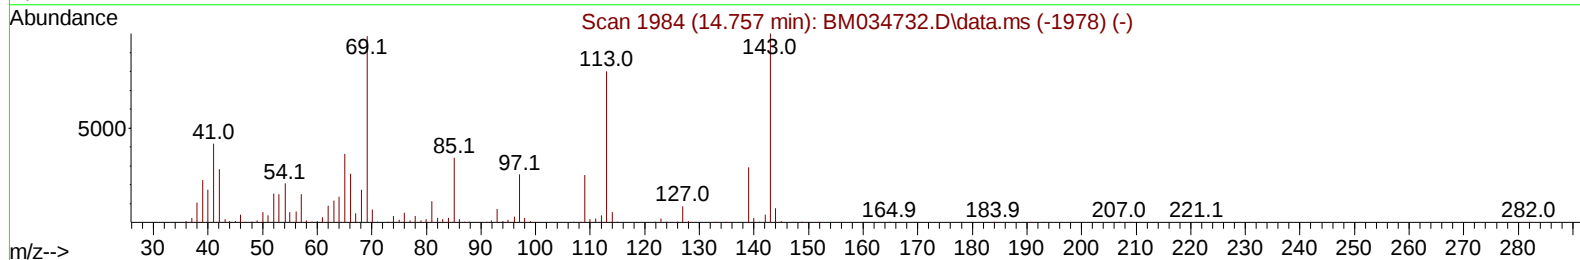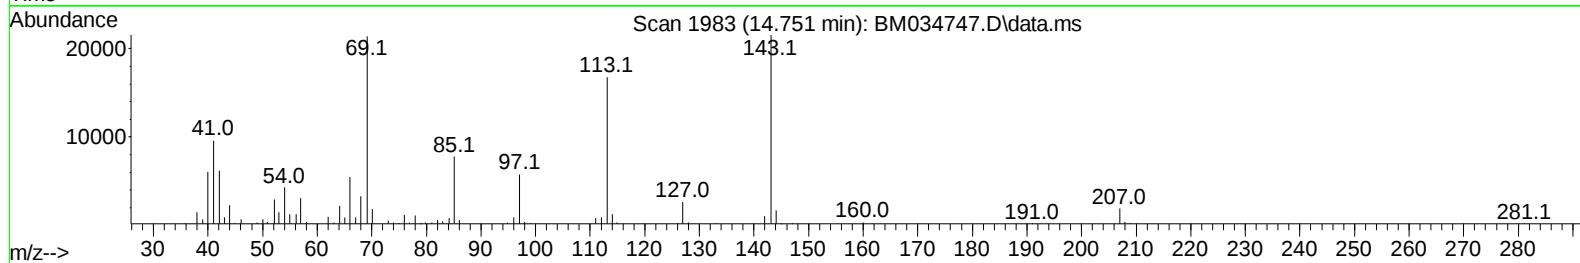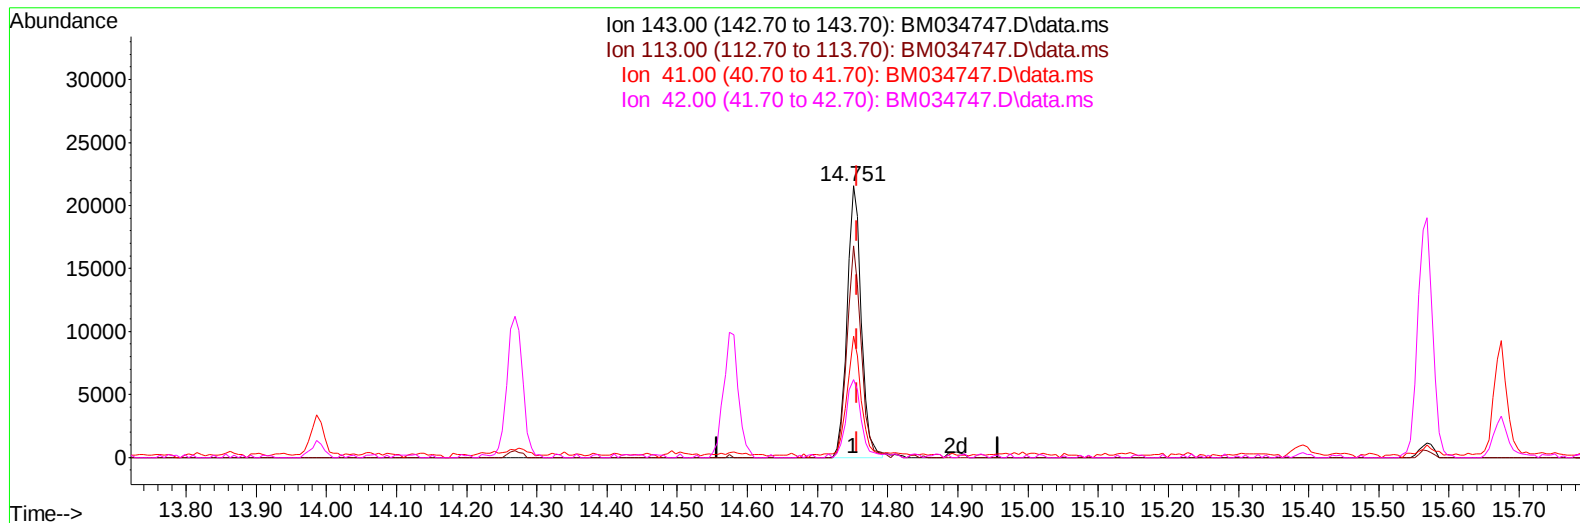

TIC: BM034747.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.751min (-0.006) 6.08 ng/u1

response 30460

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.00	77.91
41.00	42.20	44.63
42.00	28.30	28.68




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
 Data File : BM034747.D
 Acq On : 21 Apr 2022 15:06
 Operator : CG/JU
 Sample : N2472-18
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0J17

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:21:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 05:03:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/22/2022
 Supervised By :mohammad ahmed 04/26/2022

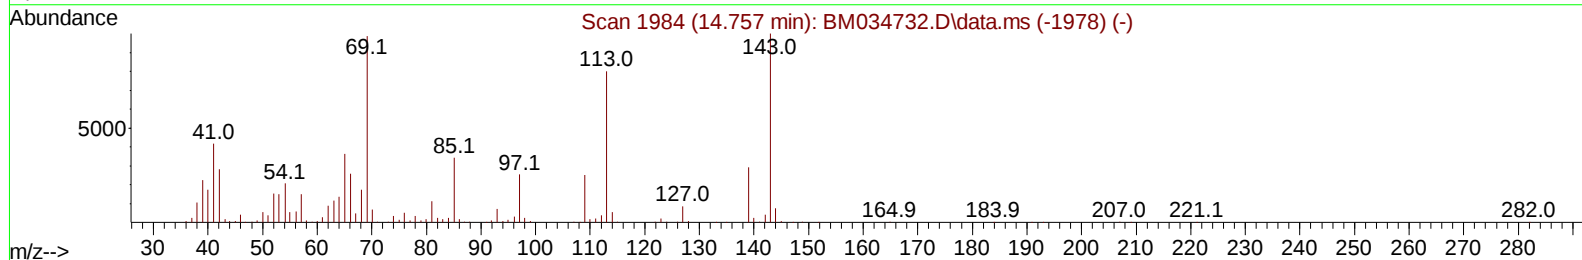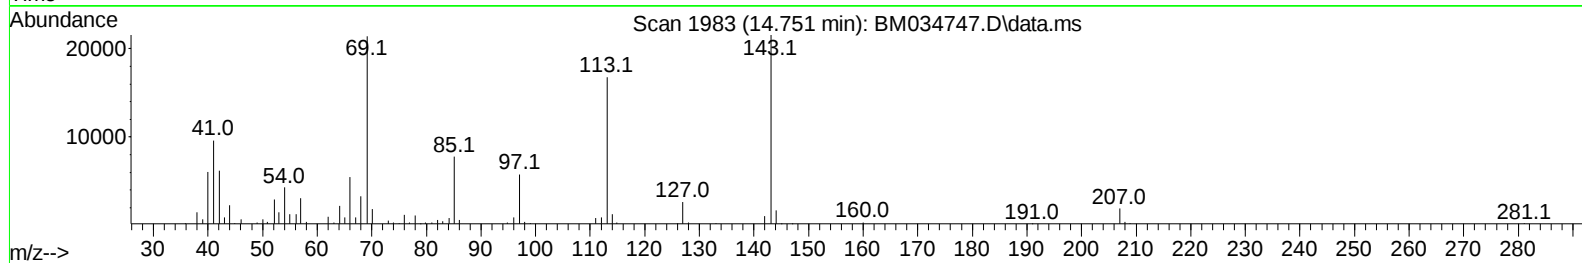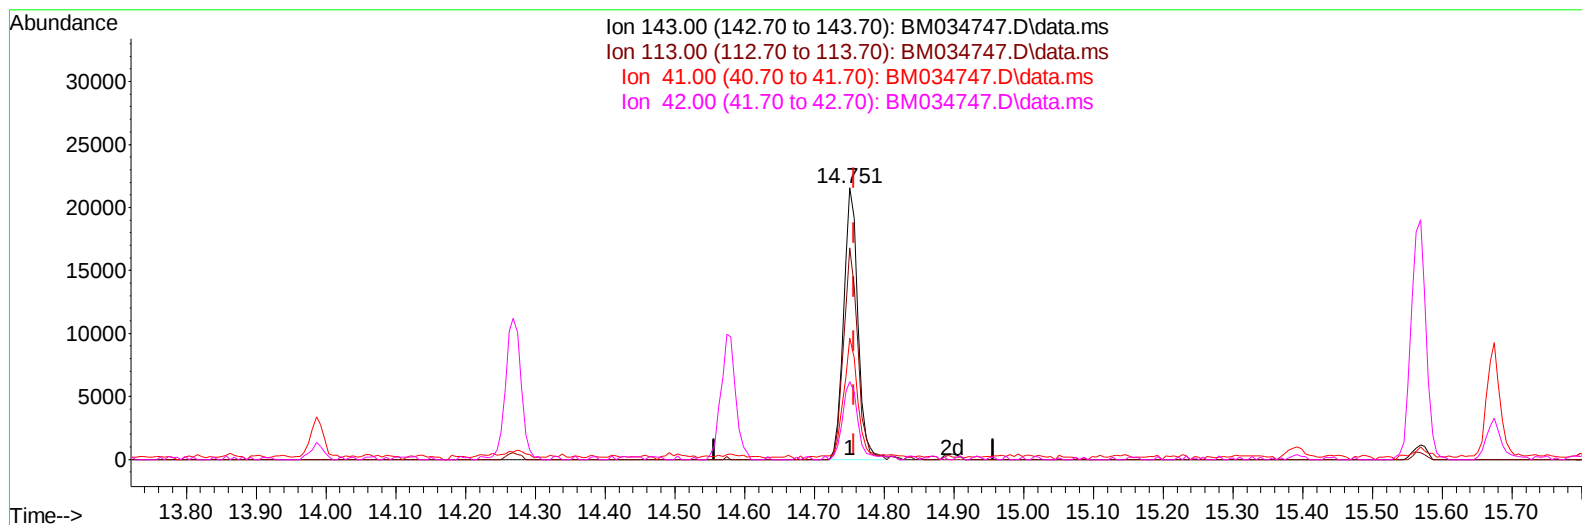

TIC: BM034747.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.751min (-0.006) 6.11 ng/ul m

response 30634

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.00	77.91
41.00	42.20	44.63
42.00	28.30	28.68

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
 Data File : BM034747.D
 Acq On : 21 Apr 2022 15:06
 Operator : CG/JU
 Sample : N2472-18
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0J17

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/22/2022
 Supervised By :mohammad ahmed 04/26/2022

Quant Time: Apr 22 01:21:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 05:03:15 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.946	152		182868	20.000	ng/ul	0.00
20) Naphthalene-d8	10.751	136		686343	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.574	164		410000	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.315	188		769376	20.000	ng/ul	0.00
79) Chrysene-d12	21.492	240		660607	20.000	ng/ul	0.00
88) Perylene-d12	23.892	264		717396	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.381	96		20068	4.822	ng/uL	0.00
4) Pyridine-d5	3.799	84		116089	11.237	ng/ul	0.00
7) Phenol-d5	7.104	99		92159	6.672	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67		276206	35.659	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132		299184	25.594	ng/ul	0.00
15) 4-Methylphenol-d8	8.651	113		176709	15.990	ng/ul	0.00
21) Nitrobenzene-d5	9.104	128		174796	34.864	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143		170950	32.840	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165		309936	28.265	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131		353494	23.842	ng/ul	0.00
46) Dimethylphthalate-d6	13.986	166		1127928	37.789	ng/ul	0.00
49) Acenaphthylene-d8	14.269	160		1270426	33.096	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143		30634m	6.114	ng/ul	0.00
60) Fluorene-d10	15.569	176		977833	37.861	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.674	200		129118	29.252	ng/ul	0.00
73) Anthracene-d10	17.415	188		1493925	39.876	ng/ul	0.00
81) Pyrene-d10	19.704	212		1587622	44.158	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.733	264		1522821	41.970	ng/ul	0.00
Target Compounds							
75) 1,2,3,4-Tetrachloroben...	13.380	216		17568	1.356	ng/uL	Qvalue 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
Data File : BM034747.D
Acq On : 21 Apr 2022 15:06
Operator : CG/JU
Sample : N2472-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0J17

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/22/2022
Supervised By :mohammad ahmed 04/26/2022

Quant Time: Apr 22 01:21:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 05:03:15 2022
Response via : Initial Calibration

