




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
 Data File : BM034750.D
 Acq On : 21 Apr 2022 16:54
 Operator : CG/JU
 Sample : N2473-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0HZ5

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:31:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 05:03:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/22/2022
 Supervised By :mohammad ahmed 04/26/2022

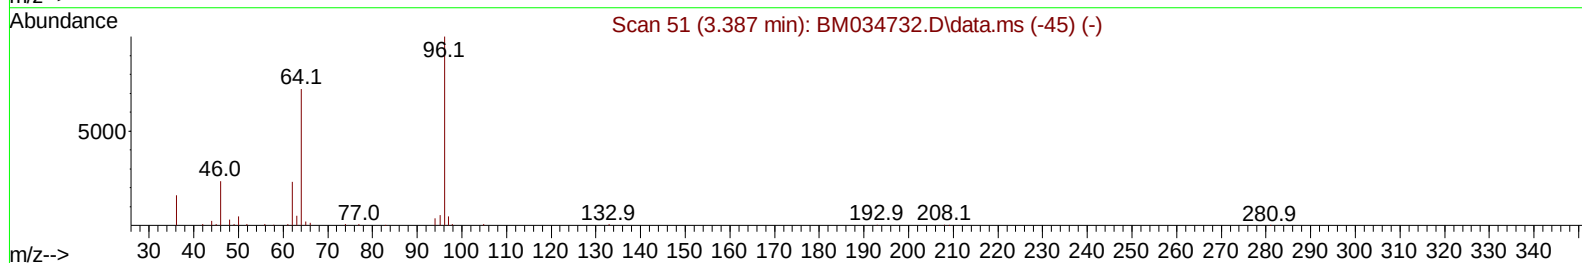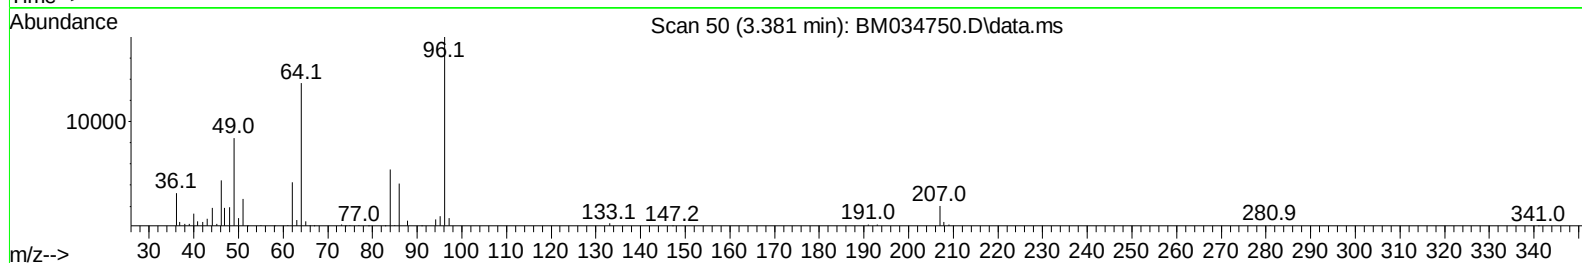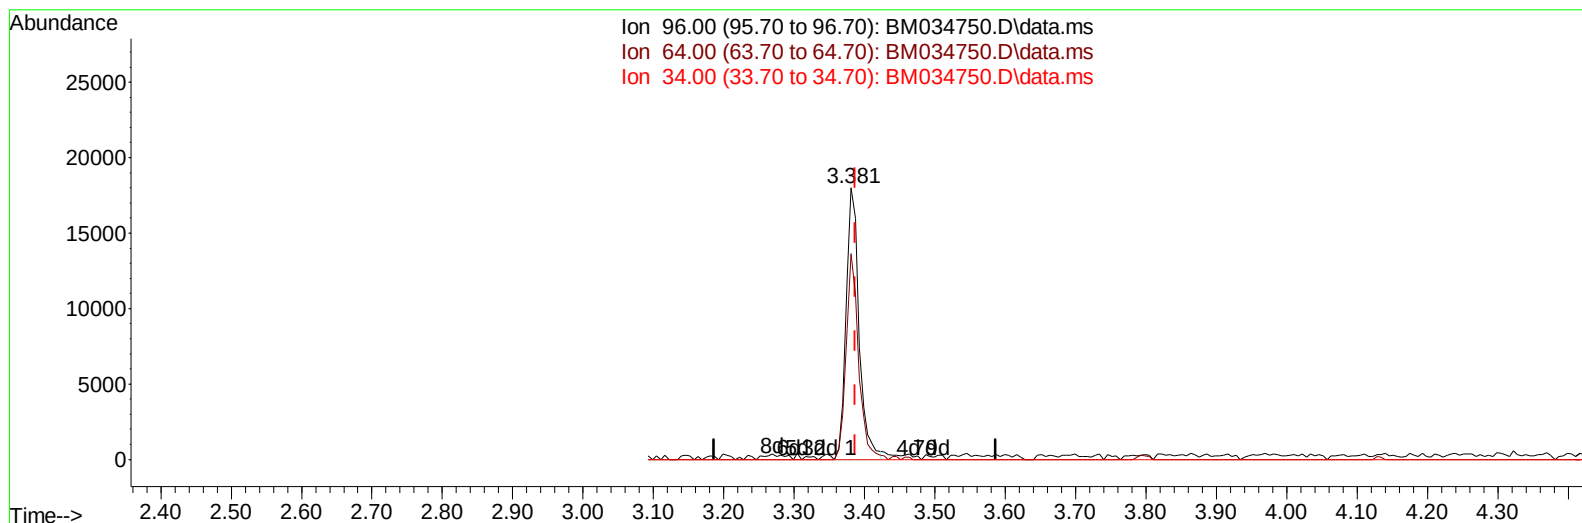

TIC: BM034750.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.381min (-0.006) 5.08 ng/uL

response 22983

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.40	75.72
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
 Data File : BM034750.D
 Acq On : 21 Apr 2022 16:54
 Operator : CG/JU
 Sample : N2473-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0HZ5

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:31:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 05:03:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/22/2022
 Supervised By :mohammad ahmed 04/26/2022

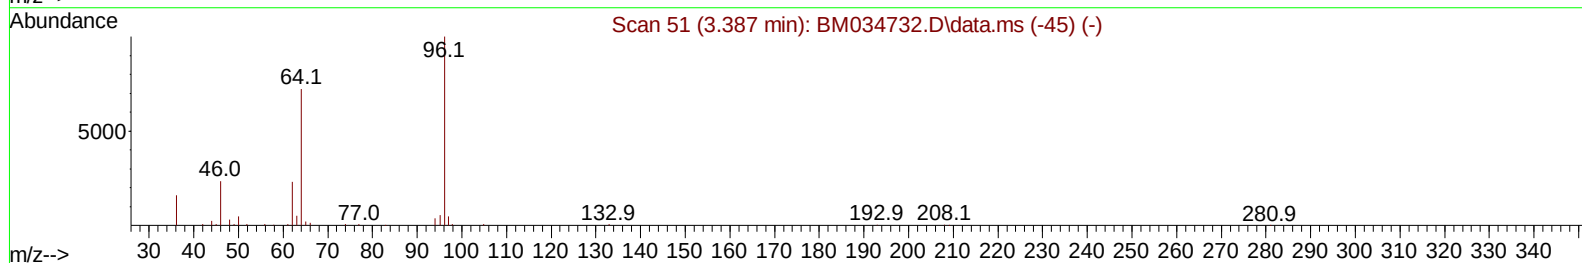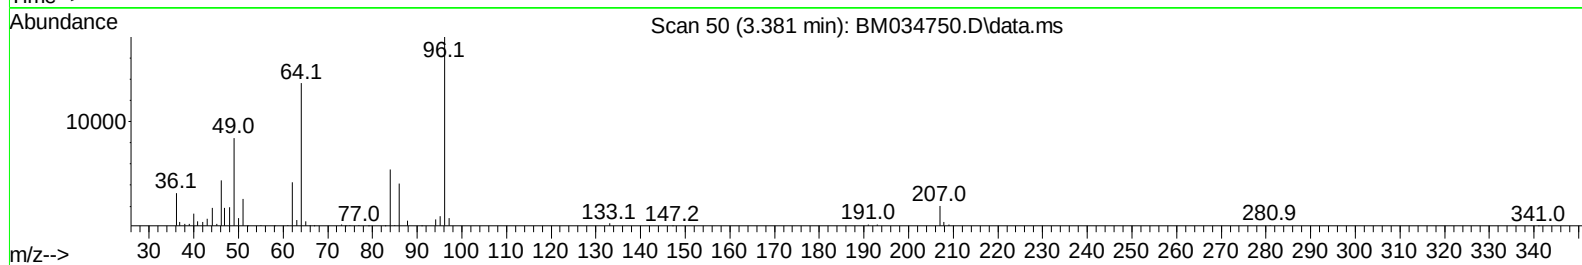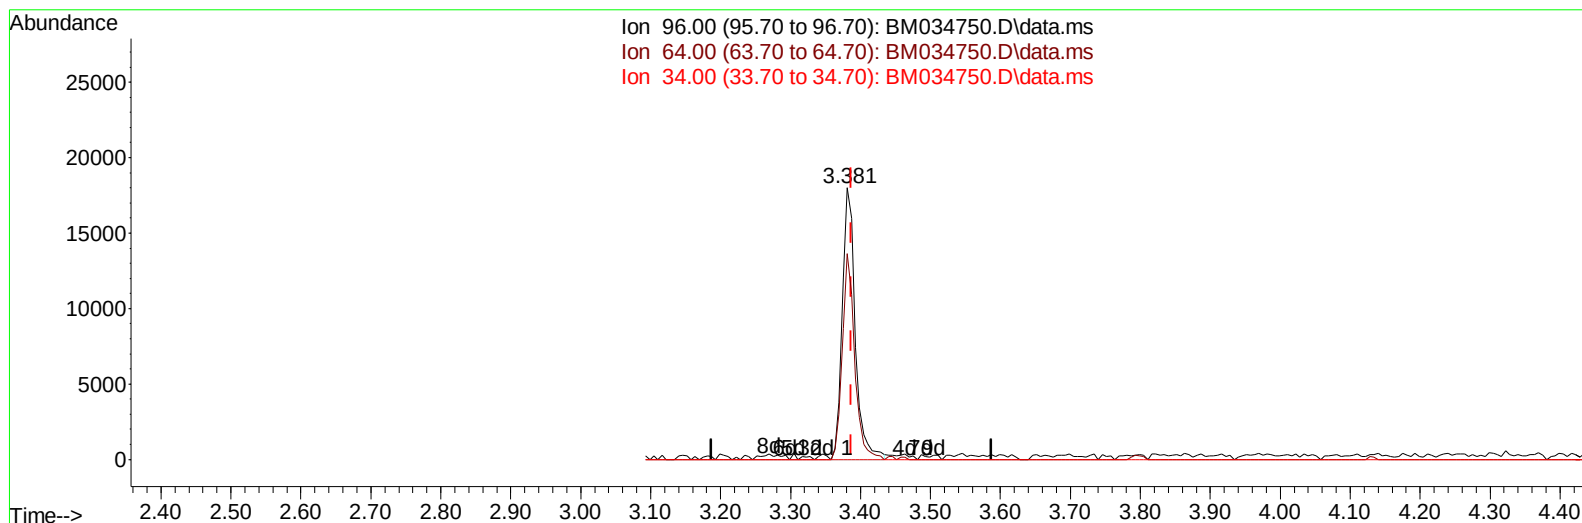

TIC: BM034750.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.381min (-0.006) 5.15 ng/uL m

response 23262

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.40	75.72
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
 Data File : BM034750.D
 Acq On : 21 Apr 2022 16:54
 Operator : CG/JU
 Sample : N2473-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0HZ5

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:31:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 05:03:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/22/2022
 Supervised By :mohammad ahmed 04/26/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	198602	20.000	ng/ul	0.00
20) Naphthalene-d8	10.751	136	785175	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.574	164	487746	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.315	188	930144	20.000	ng/ul	0.00
79) Chrysene-d12	21.492	240	821975	20.000	ng/ul	0.00
88) Perylene-d12	23.892	264	837537	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	23262m	5.147	ng/uL	0.00
4) Pyridine-d5	3.799	84	102998	9.180	ng/ul	0.00
7) Phenol-d5	7.098	99	113986	7.599	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	308398	36.661	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	351916	27.720	ng/ul	0.00
15) 4-Methylphenol-d8	8.645	113	219318	18.274	ng/ul	-0.01
21) Nitrobenzene-d5	9.104	128	203183	35.425	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	208159	34.955	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	364584	29.064	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131	372596	21.967	ng/ul	0.00
46) Dimethylphthalate-d6	13.986	166	1339537	37.725	ng/ul	0.00
49) Acenaphthylene-d8	14.269	160	1502427	32.901	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	42417	7.116	ng/ul	0.00
60) Fluorene-d10	15.569	176	1168790	38.041	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.674	200	178153	33.385	ng/ul	0.00
73) Anthracene-d10	17.415	188	1868787	41.260	ng/ul	0.00
81) Pyrene-d10	19.704	212	1981379	44.290	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.739	264	1834274	43.302	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
Data File : BM034750.D
Acq On : 21 Apr 2022 16:54
Operator : CG/JU
Sample : N2473-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HZ5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/22/2022
Supervised By :mohammad ahmed 04/26/2022

Quant Time: Apr 22 01:31:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 05:03:15 2022
Response via : Initial Calibration

