




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
Data File : BM034761.D
Acq On : 22 Apr 2022 00:05
Operator : CG/JU
Sample : N2488-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HZ0

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:52:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 05:03:15 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/22/2022
Supervised By :mohammad ahmed 04/26/2022

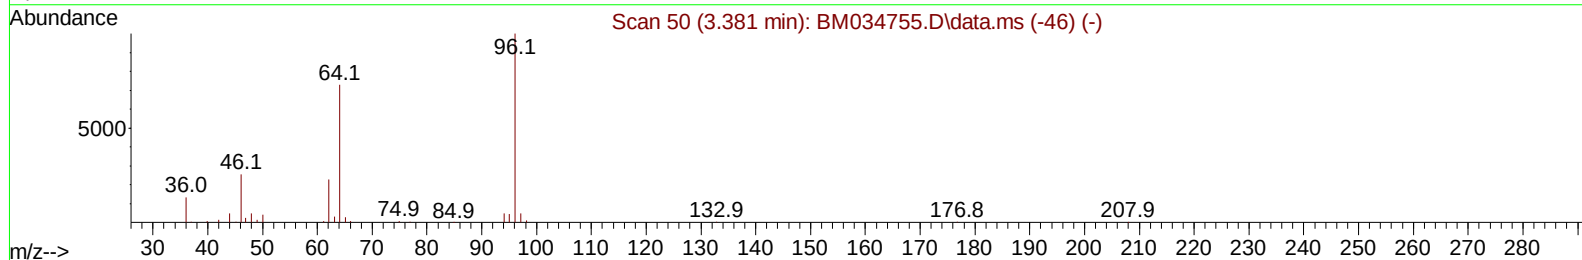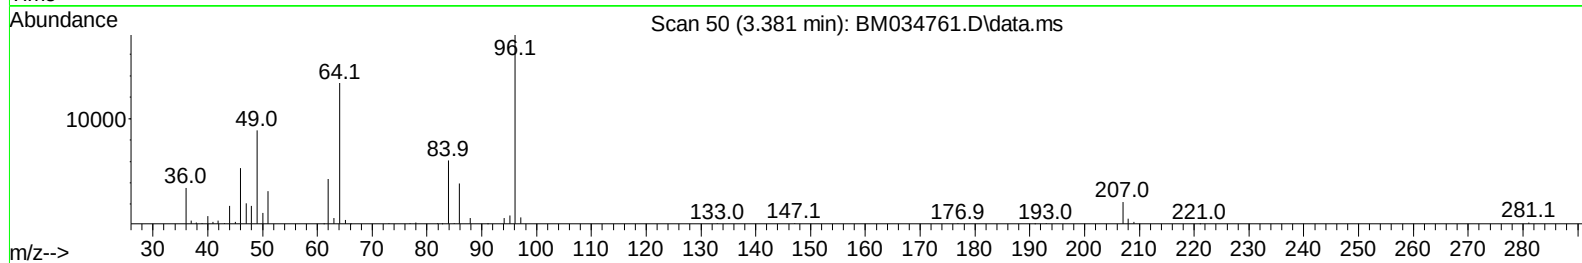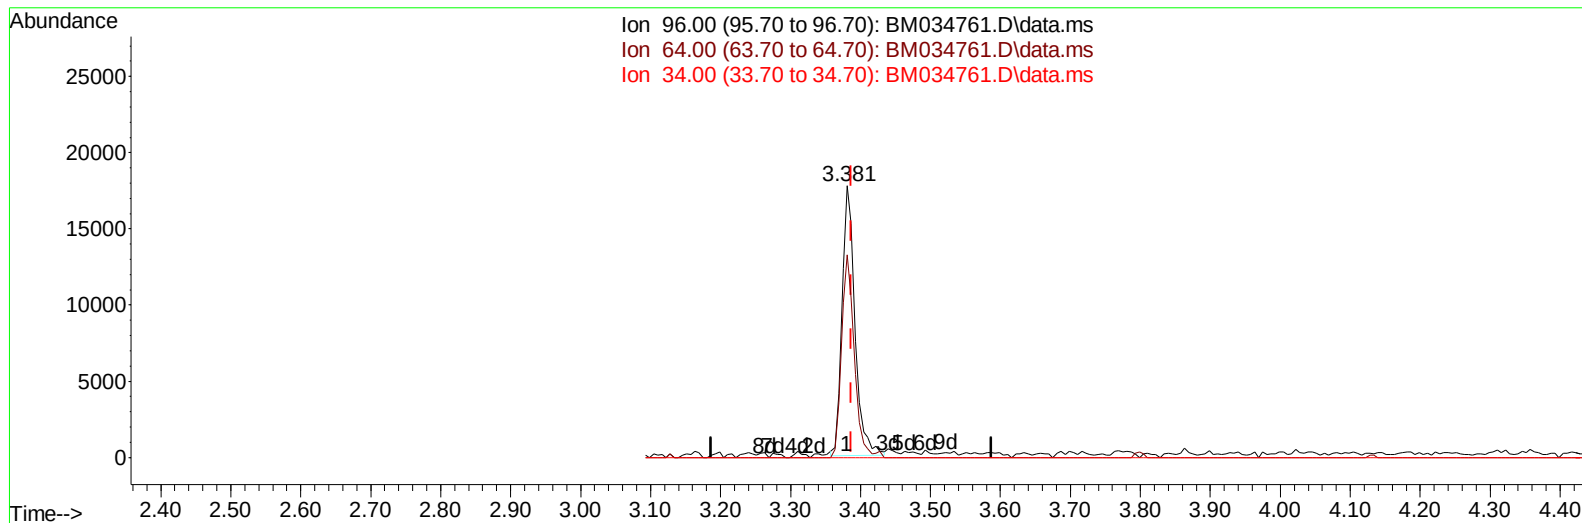

TIC: BM034761.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.381min (-0.006) 5.02 ng/uL

response 22995

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.40	74.74
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
 Data File : BM034761.D
 Acq On : 22 Apr 2022 00:05
 Operator : CG/JU
 Sample : N2488-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0HZ0

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:52:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 05:03:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/22/2022
 Supervised By :mohammad ahmed 04/26/2022

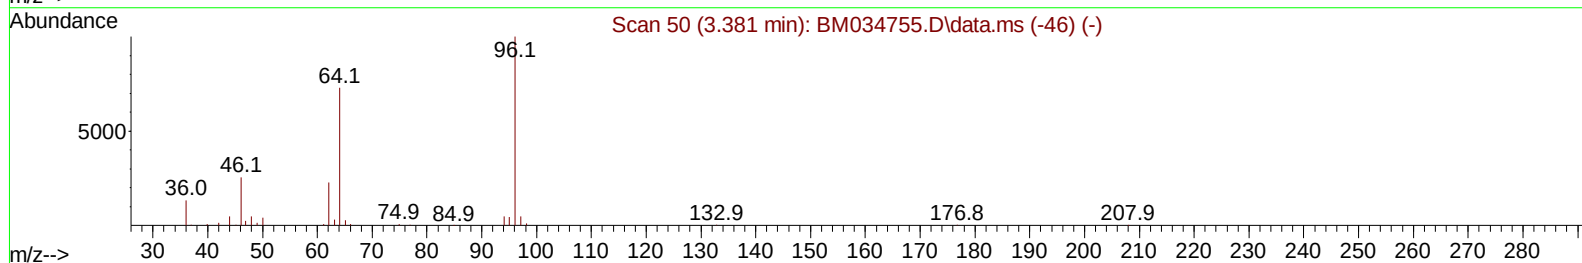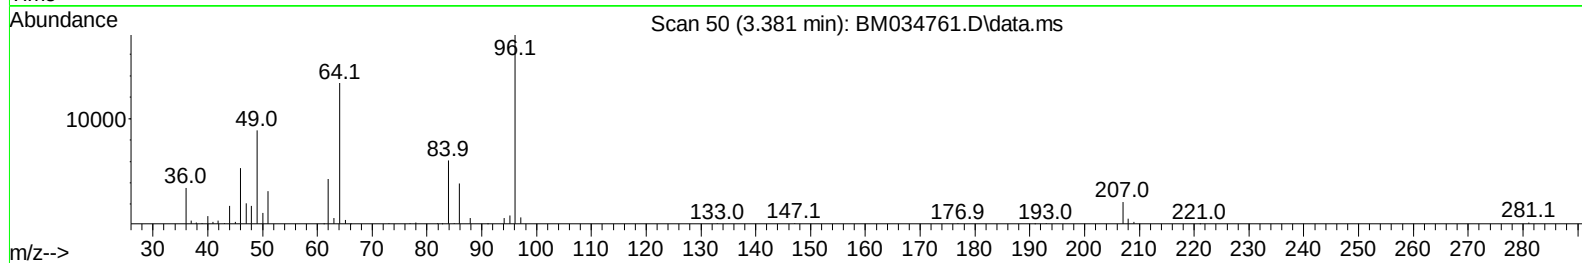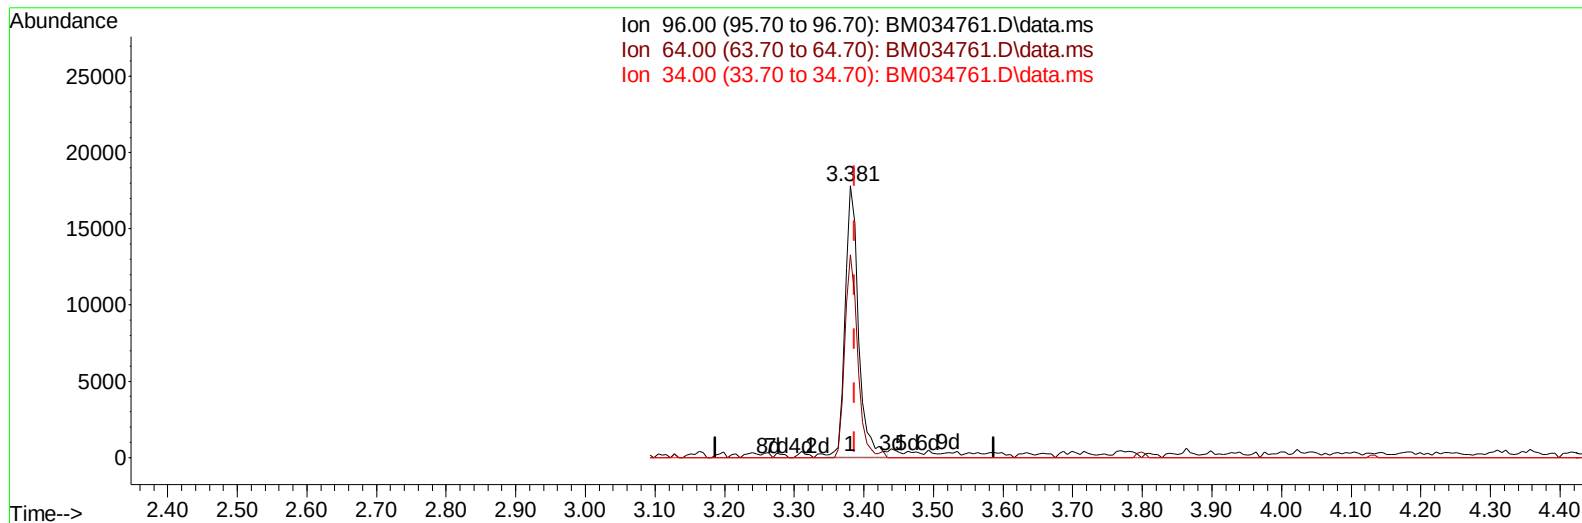

TIC: BM034761.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.381min (-0.006) 5.09 ng/uL m

response 23324

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.40	74.74
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
 Data File : BM034761.D
 Acq On : 22 Apr 2022 00:05
 Operator : CG/JU
 Sample : N2488-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COHZ0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/22/2022
 Supervised By :mohammad ahmed 04/26/2022

Quant Time: Apr 22 01:52:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 05:03:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.945	152	201279	20.000	ng/ul	0.00
20) Naphthalene-d8	10.745	136	772481	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.574	164	459551	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.315	188	899032	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	833823	20.000	ng/ul	-0.01
88) Perylene-d12	23.885	264	860178	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	23324m	5.092	ng/uL	0.00
4) Pyridine-d5	3.793	84	124000	10.905	ng/ul	0.00
7) Phenol-d5	7.098	99	65645	4.318	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	172078	20.184	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	177974	13.832	ng/ul	0.00
15) 4-Methylphenol-d8	8.645	113	67551	5.554	ng/ul	-0.01
21) Nitrobenzene-d5	9.098	128	110911	19.655	ng/ul	0.00
24) 2-Nitrophenol-d4	9.822	143	104962	17.915	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	174604	14.148	ng/ul	0.00
31) 4-Chloroaniline-d4	10.875	131	88674	5.314	ng/ul	0.00
46) Dimethylphthalate-d6	13.986	166	674847	20.172	ng/ul	0.00
49) Acenaphthylene-d8	14.268	160	755201	17.553	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	27052	4.817	ng/ul	0.00
60) Fluorene-d10	15.562	176	583950	20.172	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.668	200	75694	14.675	ng/ul	-0.01
73) Anthracene-d10	17.409	188	837346	19.127	ng/ul	0.00
81) Pyrene-d10	19.698	212	935409	20.612	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.727	264	926946	21.307	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
Data File : BM034761.D
Acq On : 22 Apr 2022 00:05
Operator : CG/JU
Sample : N2488-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HZ0

Manual IntegrationsAPPROVED

Quant Time: Apr 22 01:52:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 05:03:15 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/22/2022
Supervised By :mohammad ahmed 04/26/2022

