

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
 Data File : BM034741.D
 Acq On : 21 Apr 2022 11:31
 Operator : CG/JU
 Sample : N2472-15
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0J61

Quant Time: Apr 22 01:05:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 05:03:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.945	152	179077	20.000	ng/u1	0.00
20) Naphthalene-d8	10.751	136	703163	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.580	164	434189	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.315	188	869709	20.000	ng/u1	0.00
79) Chrysene-d12	21.491	240	817459	20.000	ng/u1	0.00
88) Perylene-d12	23.891	264	848658	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	22046	5.409	ng/uL	0.00
4) Pyridine-d5	3.798	84	115668	11.434	ng/u1	0.00
7) Phenol-d5	7.104	99	76505	5.656	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	290059	38.240	ng/u1	0.00
11) 2-Chlorophenol-d4	7.475	132	279030	24.375	ng/u1	0.00
15) 4-Methylphenol-d8	8.645	113	156632	14.474	ng/u1	-0.01
21) Nitrobenzene-d5	9.104	128	183473	35.719	ng/u1	0.00
24) 2-Nitrophenol-d4	9.828	143	167060	31.325	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	295010	26.260	ng/u1	0.00
31) 4-Chloroaniline-d4	10.880	131	476167	31.347	ng/u1	0.00
46) Dimethylphthalate-d6	13.986	166	1195400	37.819	ng/u1	0.00
49) Acenaphthylene-d8	14.268	160	1378986	33.923	ng/u1	0.00
54) 4-Nitrophenol-d4	14.751	143	26191	4.936	ng/u1	0.00
60) Fluorene-d10	15.568	176	1050039	38.391	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.674	200	137786	27.614	ng/u1	0.00
73) Anthracene-d10	17.415	188	1697019	40.071	ng/u1	0.00
81) Pyrene-d10	19.703	212	1874064	42.123	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.738	264	1841017	42.892	ng/u1	0.00
Target Compounds						
					Qvalue	
39) 1,2,4,5-Tetrachloroben...	12.774	216	49546	3.584	ng/u1	97
75) 1,2,3,4-Tetrachloroben...	13.380	216	26534	1.812	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
Data File : BM034741.D
Acq On : 21 Apr 2022 11:31
Operator : CG/JU
Sample : N2472-15
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0J61

Quant Time: Apr 22 01:05:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 05:03:15 2022
Response via : Initial Calibration




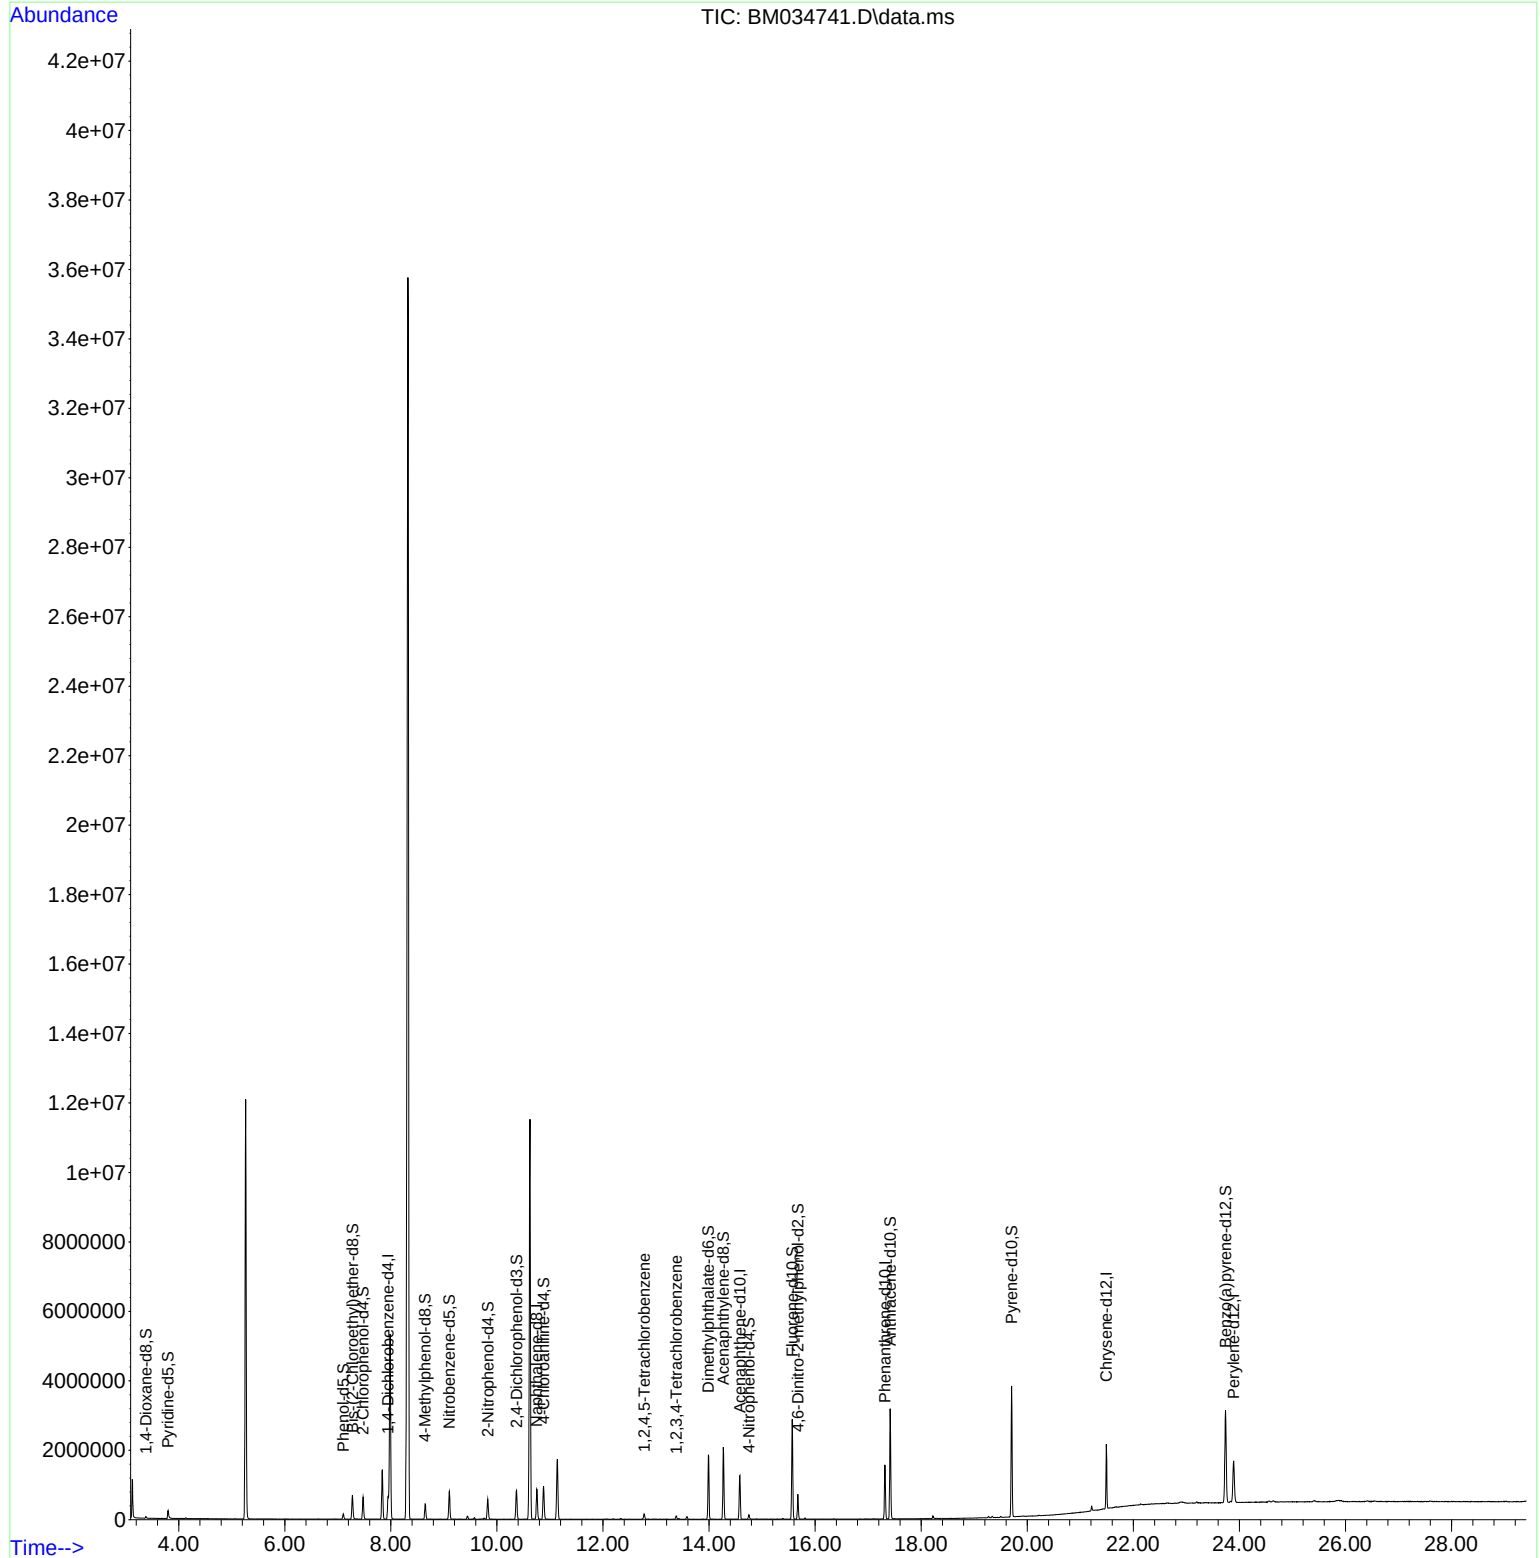


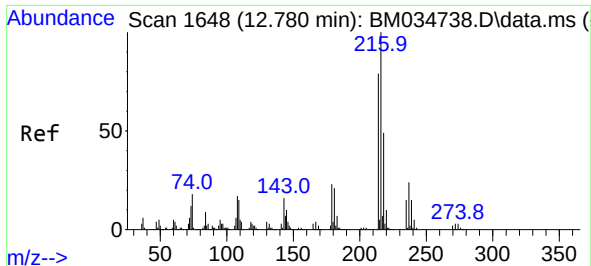

#39
1,2,4,5-Tetrachlorobenzene
Concen: 3.584 ng/ul
RT: 12.774 min Scan# 1
Delta R.T. -0.006 min
Lab File: BM034741.D
Acq: 21 Apr 2022 11:31

Instrument :
BNA_M
ClientSampleId :
C0J61

Tgt Ion:216	Resp:	49546
Ion Ratio	Lower	Upper
216	100	
214	76.8	64.5 96.7
179	22.7	17.9 26.9
108	18.0	15.0 22.4

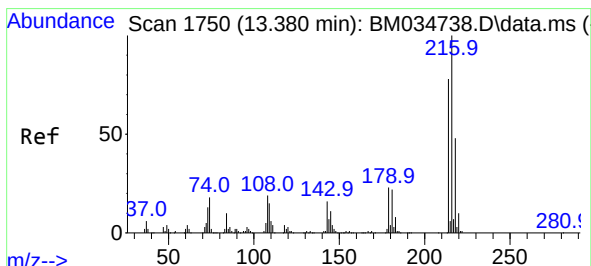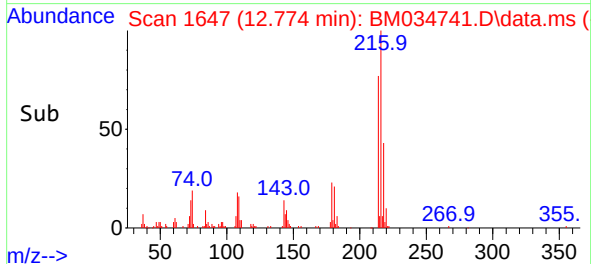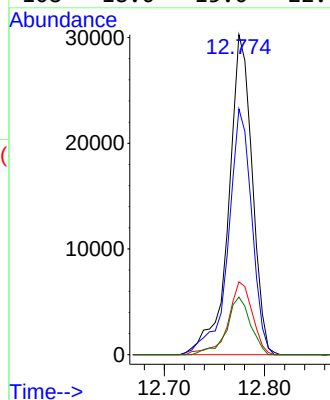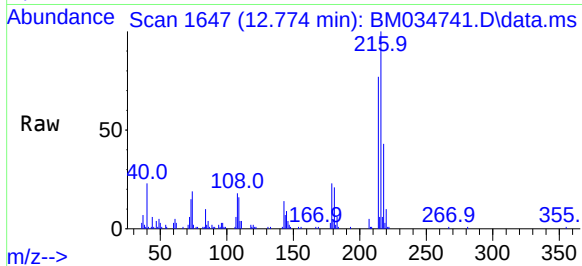

#75
1,2,3,4-Tetrachlorobenzene
Concen: 1.812 ng/ul
RT: 13.380 min Scan# 1750
Delta R.T. -0.000 min
Lab File: BM034741.D
Acq: 21 Apr 2022 11:31

Tgt Ion:216	Resp:	26534
Ion Ratio	Lower	Upper
216	100	
214	82.2	62.6 94.0
218	44.1	37.1 55.7

