

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
 Data File : BM034740.D
 Acq On : 21 Apr 2022 10:55
 Operator : CG/JU
 Sample : PB144244BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK244

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034740.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	3	6	13	rVB	46711	60359	1.46%	0.128%
2	3.381	46	50	56	rVB	62835	77072	1.86%	0.163%
3	3.793	116	120	138	rBV	683462	989209	23.90%	2.094%
4	4.134	174	178	183	rVB	16546	21604	0.52%	0.046%
5	6.081	506	509	510	rBV3	3847	4323	0.10%	0.009%
6	7.104	676	683	691	rBV	816480	1259756	30.44%	2.667%
7	7.275	705	712	725	rVB	628935	971167	23.47%	2.056%
8	7.475	739	746	758	rBV	870893	1362488	32.92%	2.885%
9	7.945	819	826	835	rVB	776034	1225068	29.60%	2.594%
10	8.651	938	946	957	rBV	975082	1581204	38.21%	3.348%
11	9.104	1015	1023	1031	rBV	753579	1226708	29.64%	2.597%
12	9.827	1138	1146	1158	rBV	606883	970185	23.44%	2.054%
13	10.363	1229	1237	1250	rBV	947430	1576555	38.09%	3.338%
14	10.751	1295	1303	1311	rBV	1010280	1672361	40.41%	3.541%
15	10.880	1316	1325	1334	rBV	995196	1640141	39.63%	3.472%
16	12.333	1567	1572	1580	rBV2	19947	30775	0.74%	0.065%
17	13.986	1847	1853	1861	rBV	1729665	2351567	56.82%	4.979%
18	14.051	1861	1864	1868	rVB5	3774	4769	0.12%	0.010%
19	14.268	1892	1901	1909	rBV	1941956	2766797	66.85%	5.858%
20	14.580	1947	1954	1963	rBV	1462590	2175127	52.56%	4.605%
21	14.757	1977	1984	1995	rBV	759228	1070776	25.87%	2.267%
22	15.568	2115	2122	2130	rBV	2556565	3501473	84.61%	7.413%
23	15.674	2134	2140	2151	rBV	660398	877844	21.21%	1.859%
24	15.809	2158	2163	2169	rVB2	28704	42091	1.02%	0.089%
25	16.127	2213	2217	2220	rBV5	4718	6653	0.16%	0.014%
26	16.351	2251	2255	2260	rVB6	7544	10483	0.25%	0.022%
27	17.098	2378	2382	2390	rVB5	8186	14442	0.35%	0.031%
28	17.315	2412	2419	2428	rBV	1776096	2459596	59.43%	5.207%
29	17.415	2430	2436	2449	rVV	2698067	3679040	88.90%	7.789%
30	17.692	2478	2483	2485	rVB4	3421	4275	0.10%	0.009%
31	19.268	2748	2751	2757	rVB3	30106	42947	1.04%	0.091%
32	19.339	2759	2763	2766	rBV2	30082	39503	0.95%	0.084%
33	19.703	2819	2825	2831	rBV	3108200	4053038	97.93%	8.581%
34	21.491	3124	3129	3136	rBV	2117931	2603466	62.91%	5.512%
35	23.738	3504	3511	3521	rVB	2082368	4138519	100.00%	8.762%
36	23.891	3530	3537	3546	rVB2	1392617	2720981	65.75%	5.761%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
Data File : BM034740.D
Acq On : 21 Apr 2022 10:55
Operator : CG/JU
Sample : PB144244BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK244

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
Title : SVOA CALIBRATION


Sum of corrected areas: 47232362

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
Data File : BM034740.D
Acq On : 21 Apr 2022 10:55
Operator : CG/JU
Sample : PB144244BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK244

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

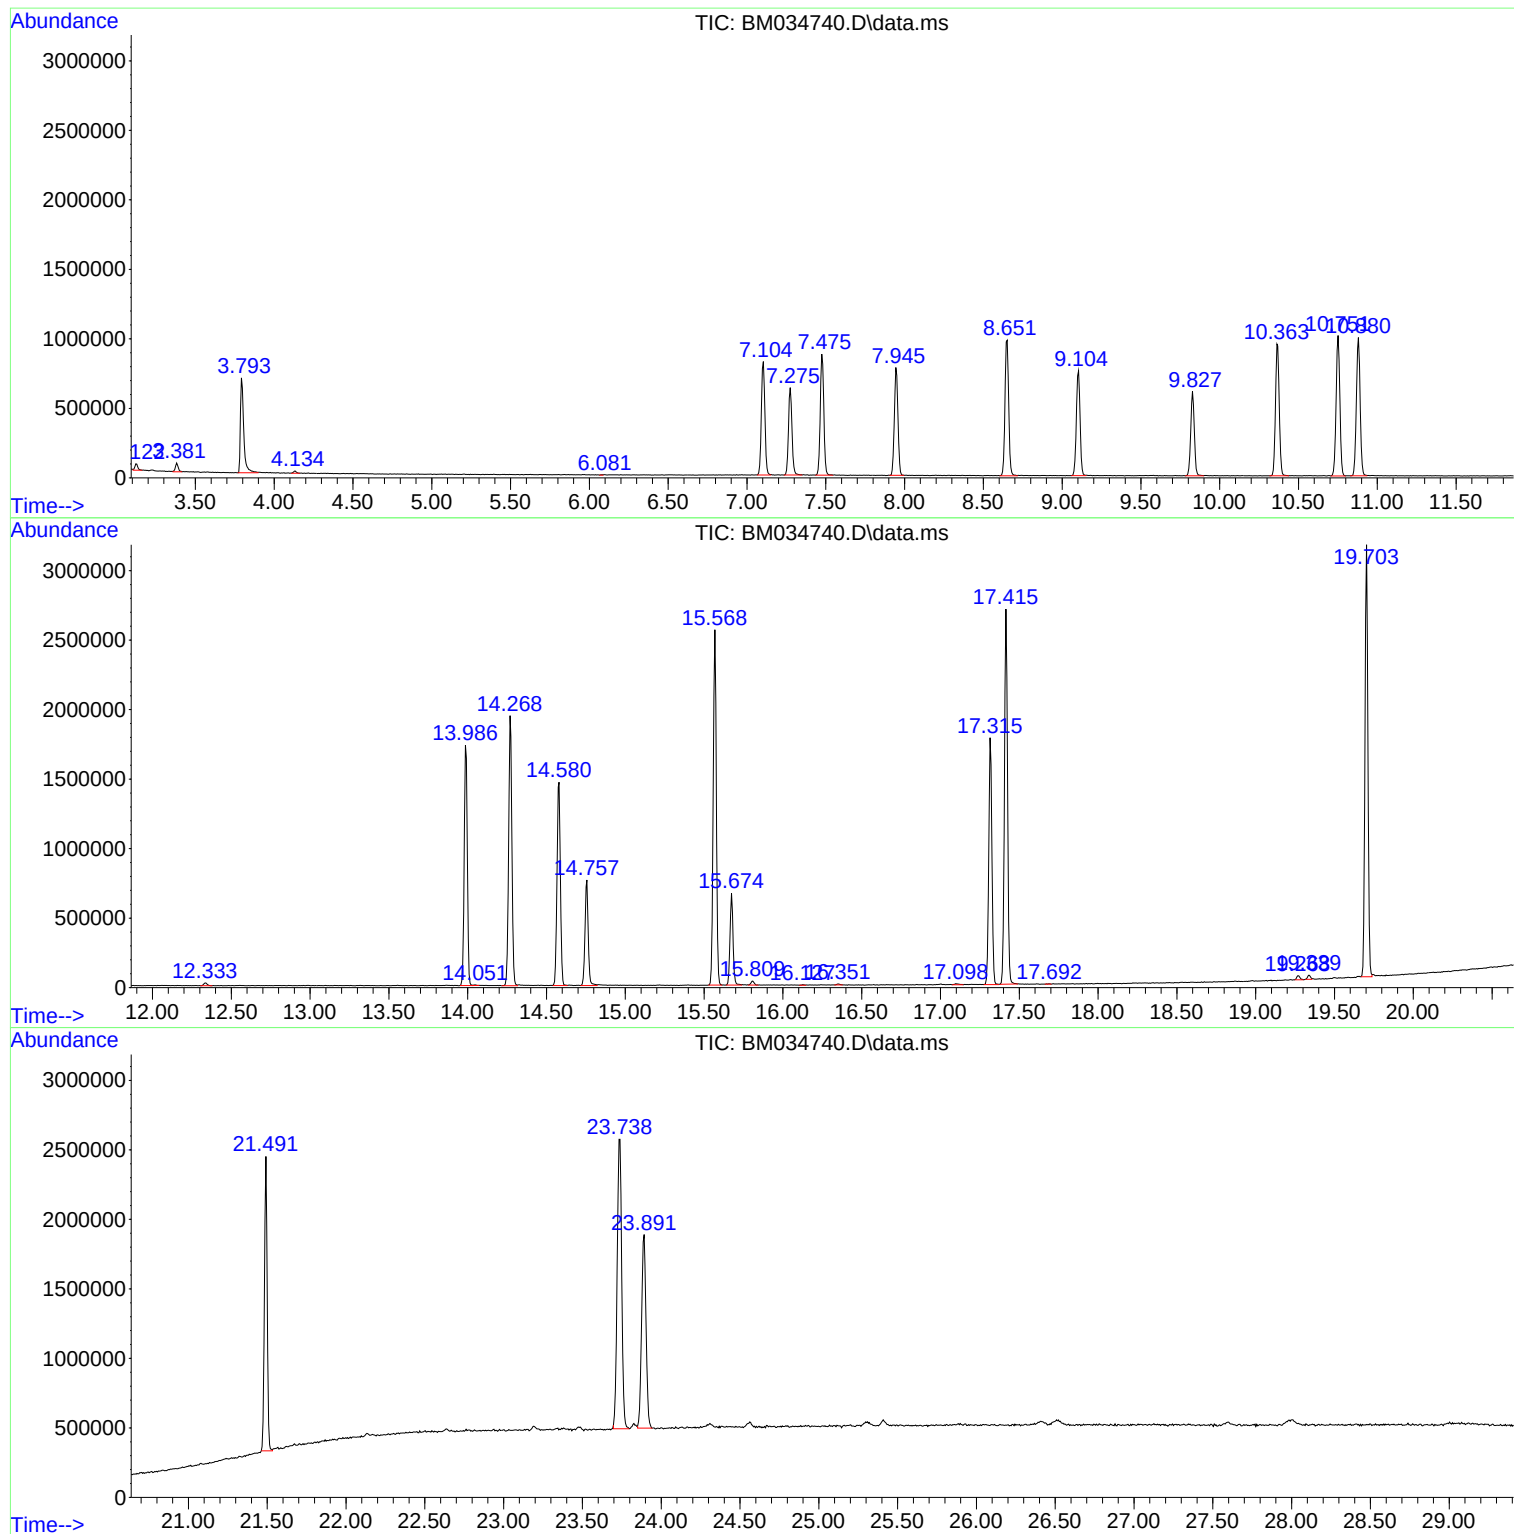

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
Data File : BM034740.D
Acq On : 21 Apr 2022 10:55
Operator : CG/JU
Sample : PB144244BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK244

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042122\
Data File : BM034740.D
Acq On : 21 Apr 2022 10:55
Operator : CG/JU
Sample : PB144244BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK244

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------