


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM042219\
 Data File : BM020004.D
 Acq On : 22 Apr 2019 10:34
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 19 00:56:08 2019

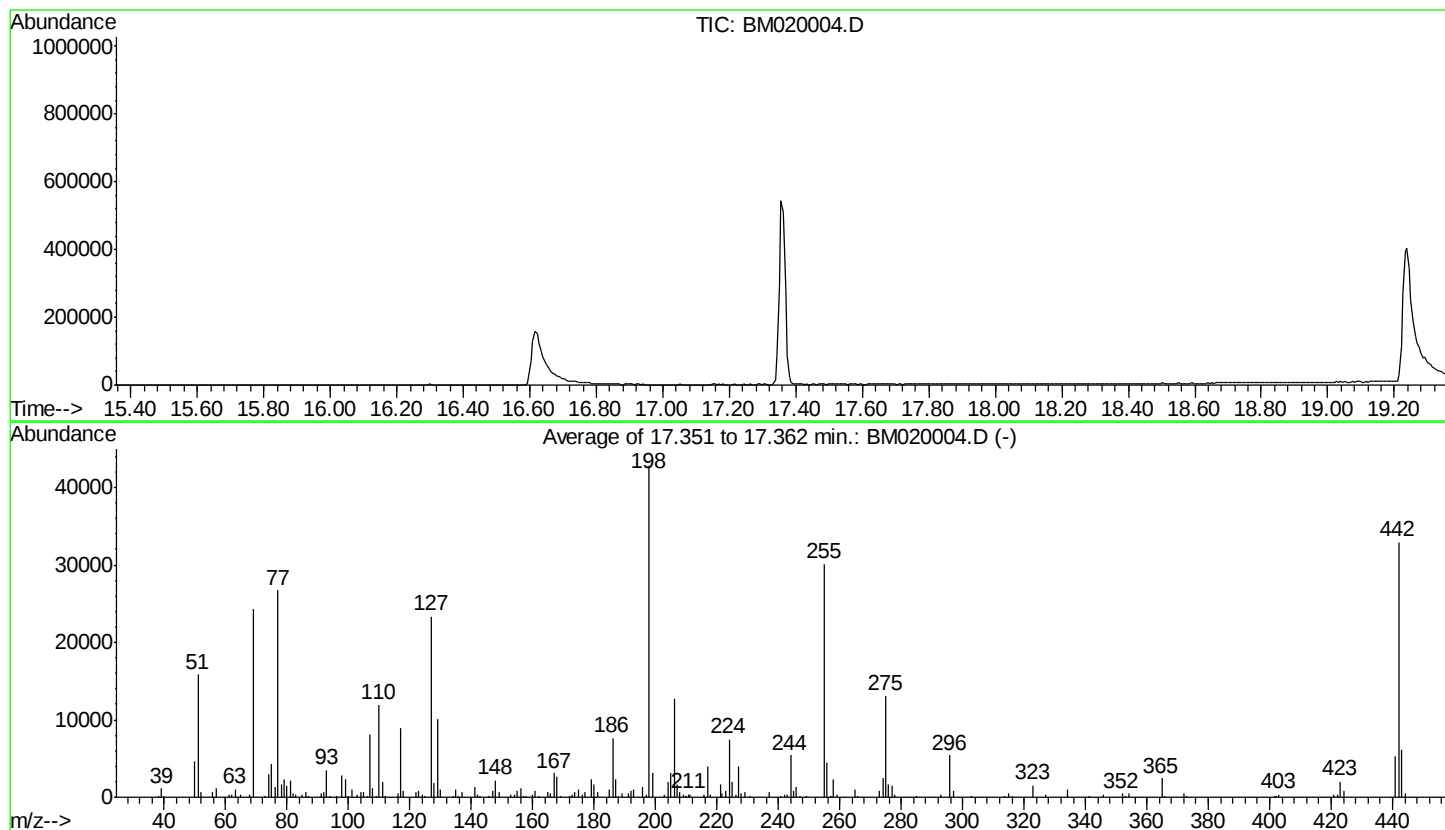

AutoFind: Scans 2442, 2443, 2444; Background Corrected with Scan 2437

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	15830	PASS
68	69	0.00	2	1.2	295	PASS
69	198	0.00	100	56.8	24309	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.5	23346	PASS
197	198	0.00	2	0.7	280	PASS
198	198	100	100	100.0	42824	PASS
199	198	5	9	7.3	3146	PASS
275	198	10	60	30.6	13110	PASS
365	198	1	100	5.7	2450	PASS
441	198	0.01	100	12.2	5218	PASS
442	198	50	100	76.9	32945	PASS
443	442	15	24	18.8	6195	PASS