


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM042219\
Data File : BM020023.D
Acq On : 23 Apr 2019 02:43
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 19 00:56:08 2019

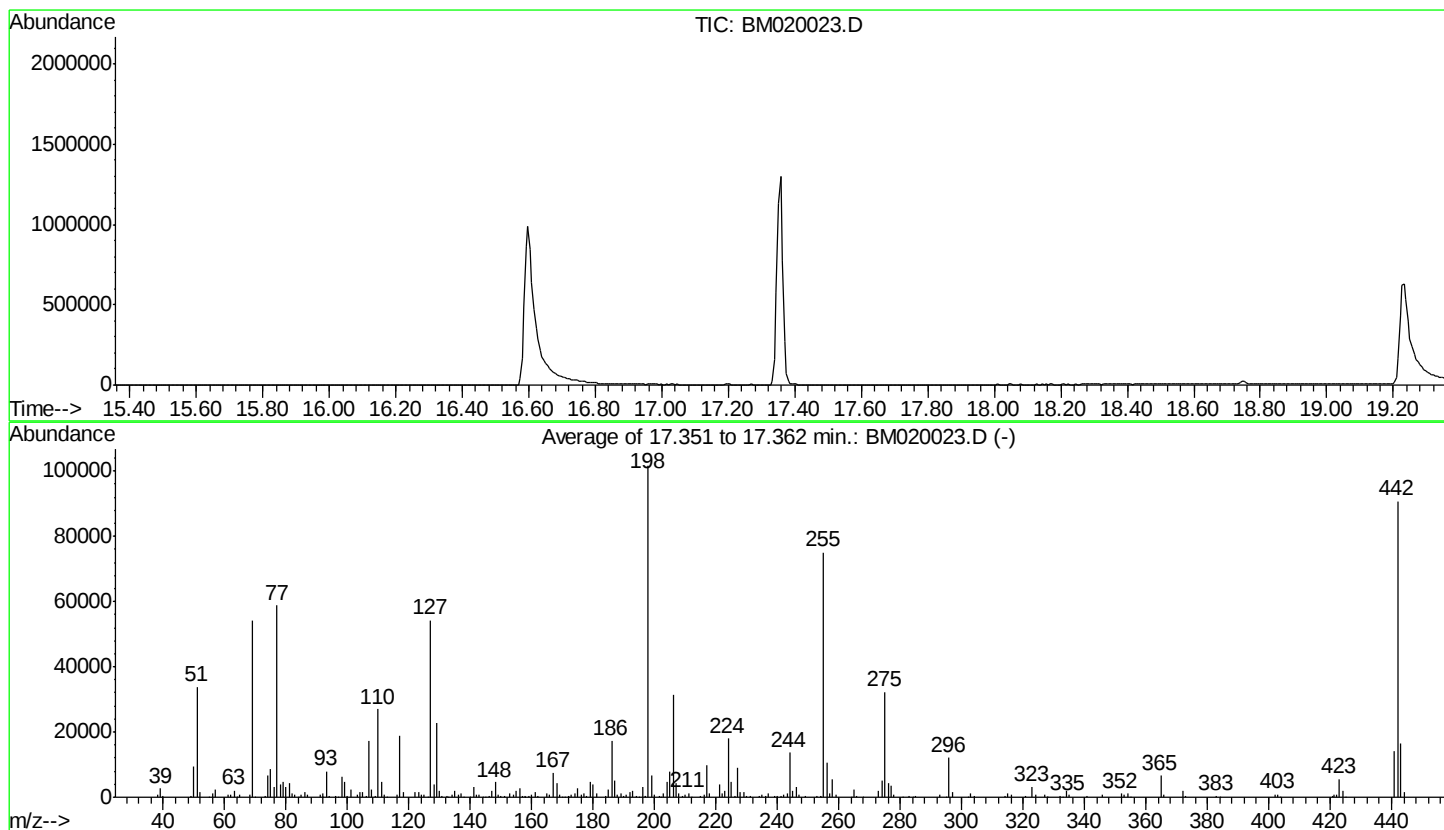

AutoFind: Scans 2442, 2443, 2444; Background Corrected with Scan 2436

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	33933	PASS
68	69	0.00	2	1.7	945	PASS
69	198	0.00	100	53.5	54328	PASS
70	69	0.00	2	0.2	118	PASS
127	198	10	80	53.4	54272	PASS
197	198	0.00	2	0.4	379	PASS
198	198	100	100	100.0	101642	PASS
199	198	5	9	6.7	6829	PASS
275	198	10	60	31.8	32370	PASS
365	198	1	100	6.5	6616	PASS
441	198	0.01	100	13.8	14051	PASS
442	198	50	100	89.2	90682	PASS
443	442	15	24	18.0	16342	PASS