




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039577.D
Acq On : 22 Apr 2023 15:40
Operator : CG/JU
Sample : 02440-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMP7

Manual IntegrationsAPPROVED

Quant Time: Apr 22 23:34:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 19 08:18:41 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/24/2023
Supervised By :Jagrut Upadhyay 04/24/2023

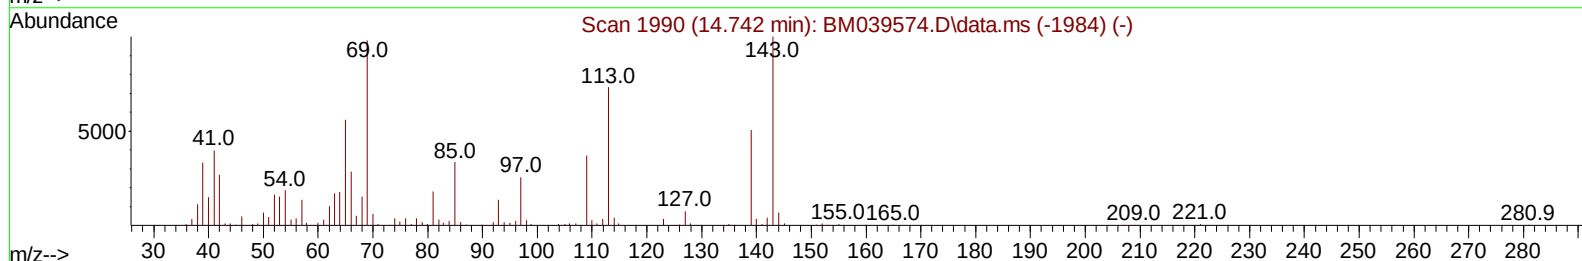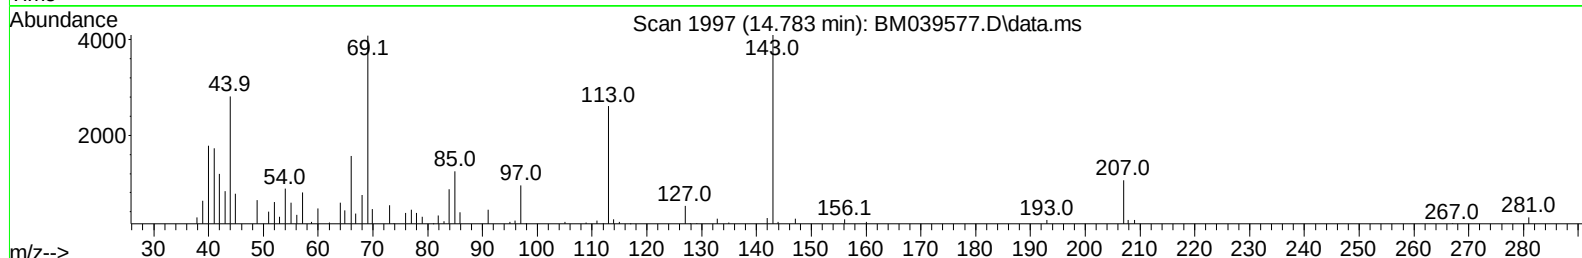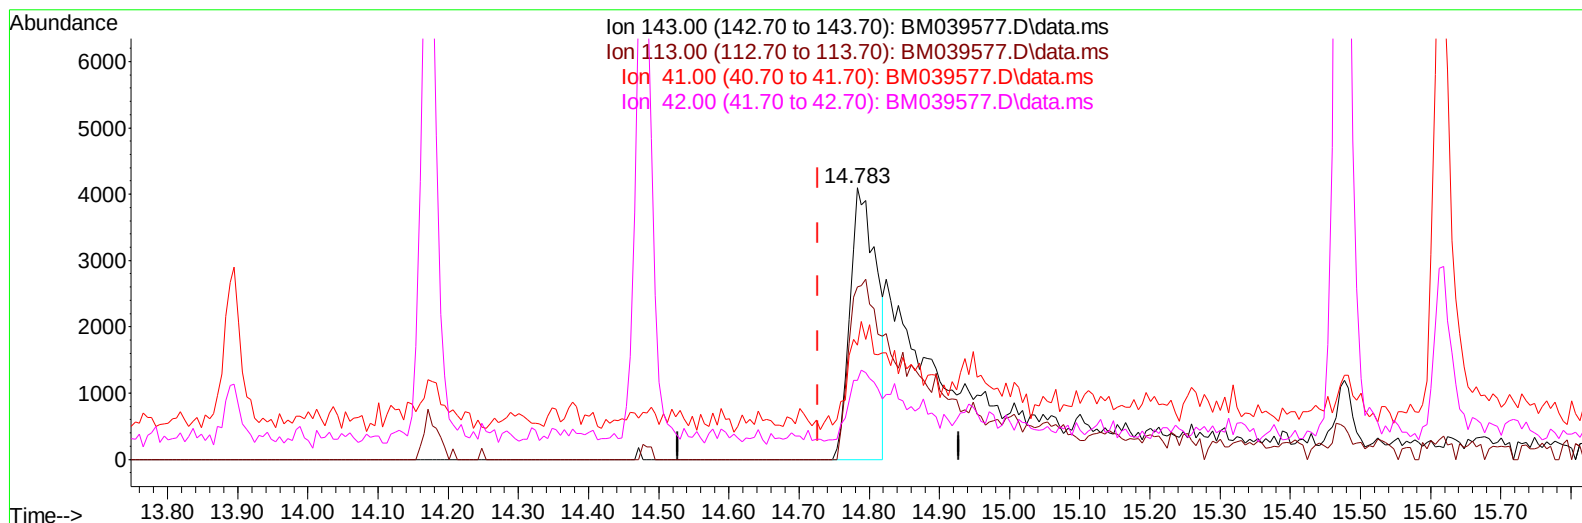

TIC: BM039577.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.783min (+ 0.056) 2.07 ng/u1

response 10785

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.20	63.61
41.00	39.90	42.12
42.00	26.60	29.13




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039577.D
Acq On : 22 Apr 2023 15:40
Operator : CG/JU
Sample : 02440-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMP7

Manual IntegrationsAPPROVED

Quant Time: Apr 22 23:34:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 19 08:18:41 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/24/2023
Supervised By :Jagrut Upadhyay 04/24/2023

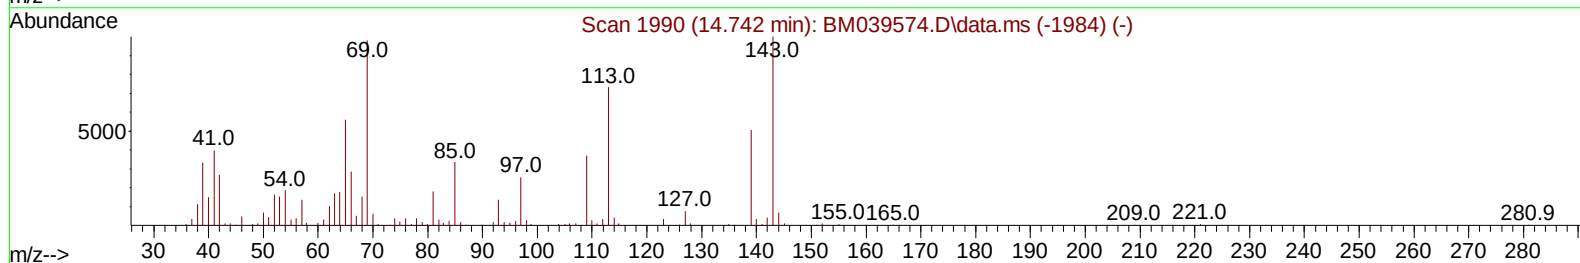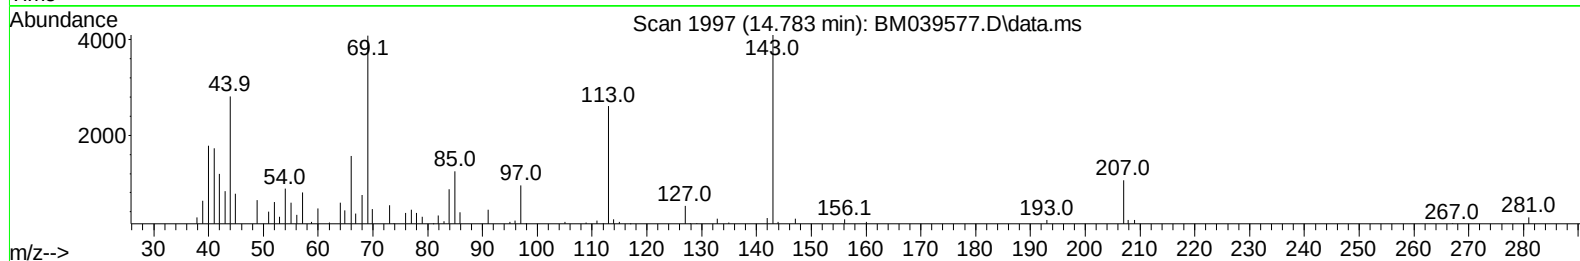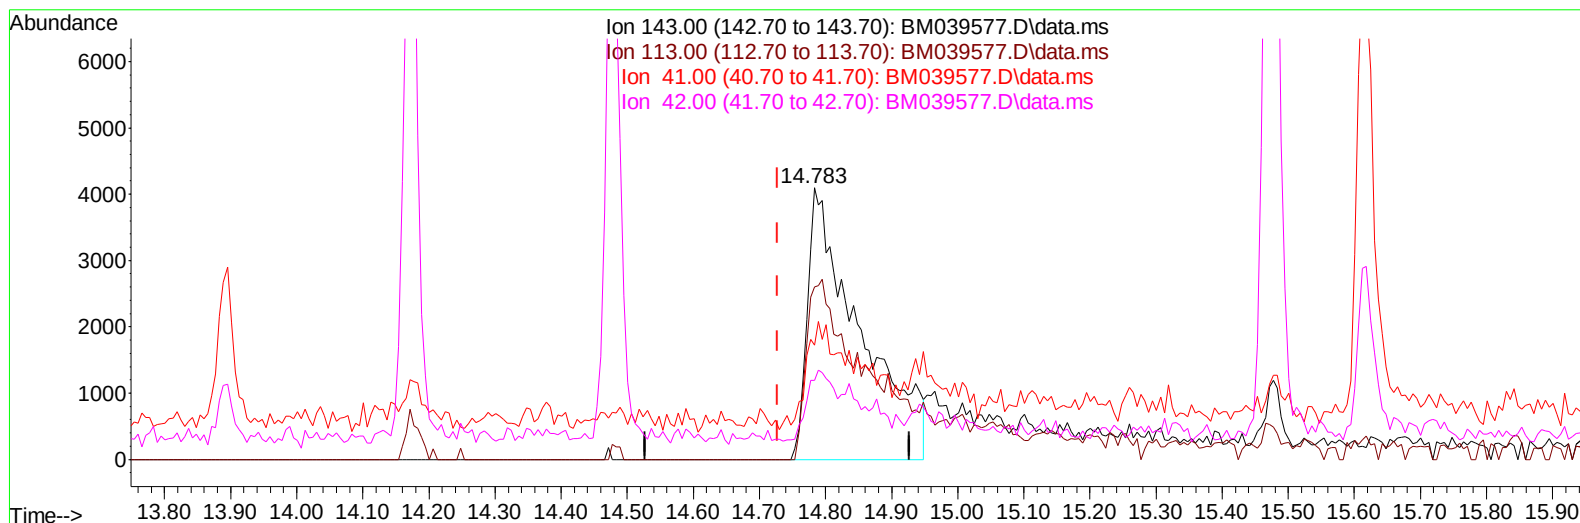

TIC: BM039577.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.783min (+ 0.056) 4.34 ng/ul m

response 22613

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.20	63.61
41.00	39.90	42.12
42.00	26.60	29.13

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
 Data File : BM039577.D
 Acq On : 22 Apr 2023 15:40
 Operator : CG/JU
 Sample : 02440-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COMP7

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/24/2023
 Supervised By :Jagrut Upadhyay 04/24/2023

Quant Time: Apr 22 23:48:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 19 08:18:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.819	152	186330	20.000	ng/ul	0.00
20) Naphthalene-d8	10.630	136	740666	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.477	164	426682	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.230	188	864942	20.000	ng/ul	0.00
79) Chrysene-d12	21.430	240	759459	20.000	ng/ul	0.00
88) Perylene-d12	23.794	264	822898	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.213	96	20892	4.304	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.013	99	95900	5.623	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.154	67	277997	24.663	ng/ul	0.00
11) 2-Chlorophenol-d4	7.354	132	287323	21.478	ng/ul	0.00
15) 4-Methylphenol-d8	8.554	113	178139	12.967	ng/ul	0.00
21) Nitrobenzene-d5	8.995	128	170844	28.671	ng/ul	0.00
24) 2-Nitrophenol-d4	9.719	143	187373	28.003	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.272	165	284396	24.702	ng/ul	0.00
31) 4-Chloroaniline-d4	10.789	131	97155	5.650	ng/ul	0.00
46) Dimethylphthalate-d6	13.895	166	1062518	30.877	ng/ul	0.00
49) Acenaphthylene-d8	14.171	160	1181794	30.570	ng/ul	0.00
54) 4-Nitrophenol-d4	14.783	143	22613m	4.342	ng/ul	0.06
60) Fluorene-d10	15.477	176	921442	32.683	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.618	200	148669	25.865	ng/ul	0.00
73) Anthracene-d10	17.330	188	1579211	37.965	ng/ul	0.00
81) Pyrene-d10	19.630	212	1827579	36.214	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.647	264	1699963	38.264	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039577.D
Acq On : 22 Apr 2023 15:40
Operator : CG/JU
Sample : 02440-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMP7

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/24/2023
Supervised By :Jagrut Upadhyay 04/24/2023

Quant Time: Apr 22 23:48:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 19 08:18:41 2023
Response via : Initial Calibration

