




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039598.D
Acq On : 23 Apr 2023 04:57
Operator : CG/JU
Sample : 02392-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE30

Manual IntegrationsAPPROVED

Quant Time: Apr 23 05:29:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 00:18:16 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/24/2023
Supervised By :Jagrut Upadhyay 04/24/2023

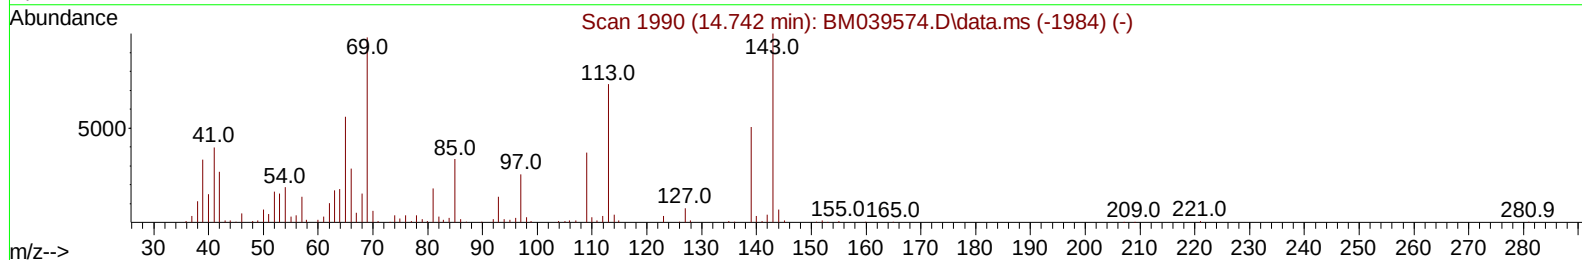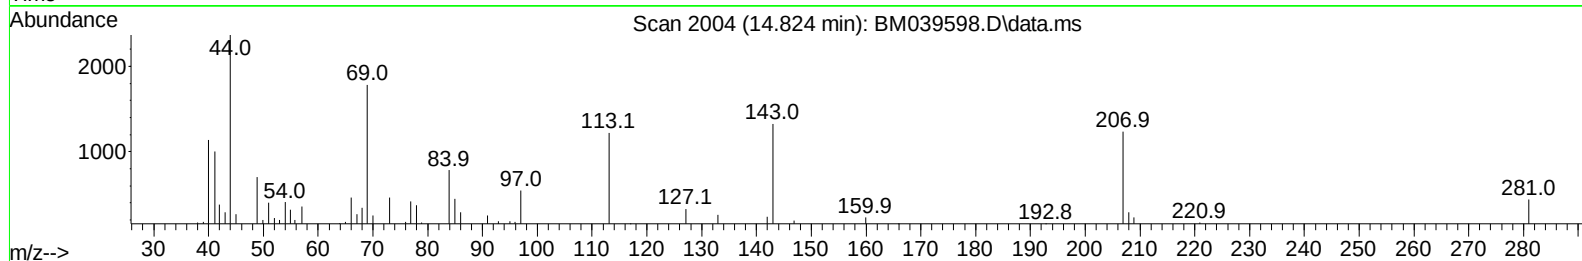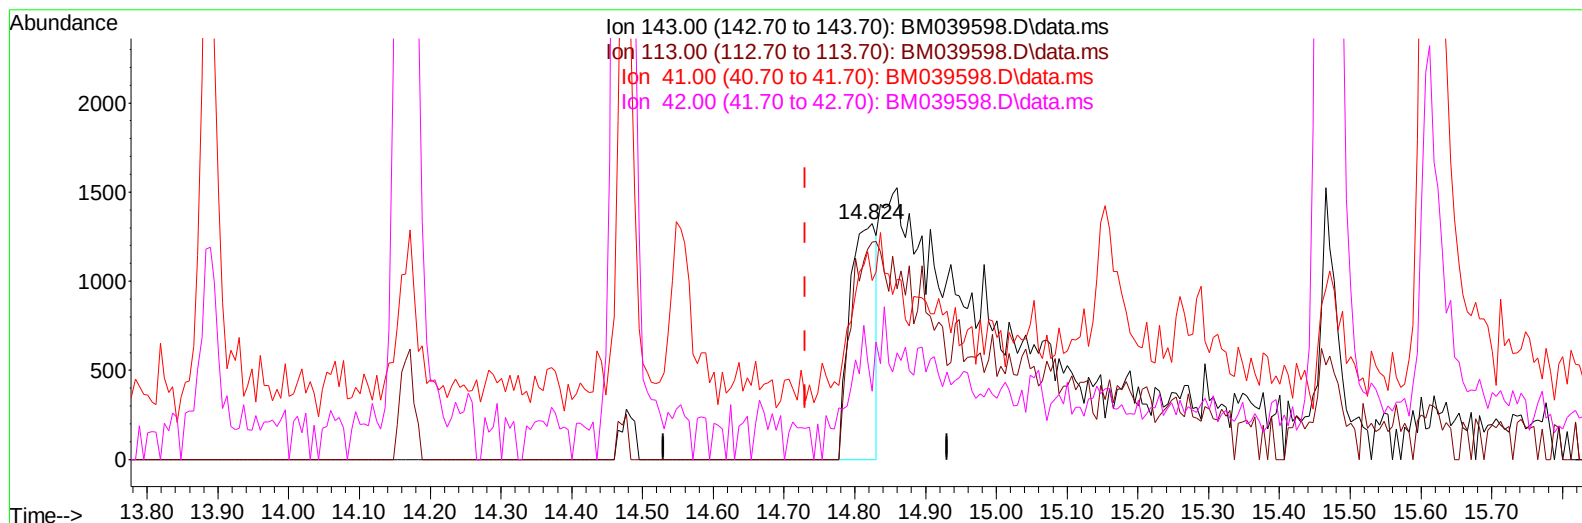

TIC: BM039598.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.824min (+ 0.094) 0.55 ng/ul

response 3421

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.20	92.29#
41.00	39.90	75.81#
42.00	26.60	28.95




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039598.D
Acq On : 23 Apr 2023 04:57
Operator : CG/JU
Sample : 02392-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE30

Manual IntegrationsAPPROVED

Quant Time: Apr 23 05:29:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 00:18:16 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/24/2023
Supervised By :Jagrut Upadhyay 04/24/2023

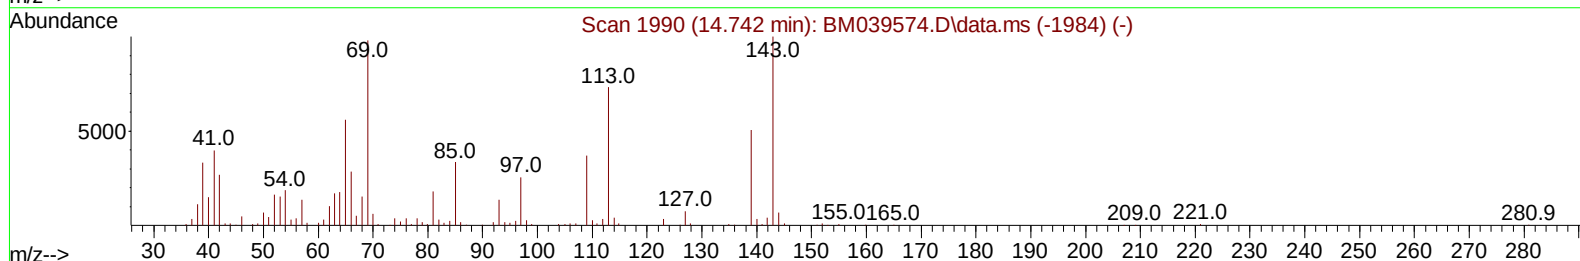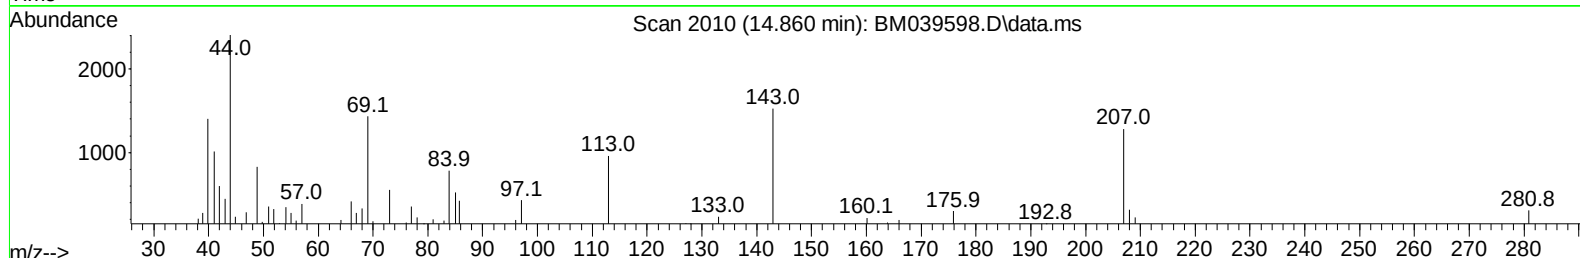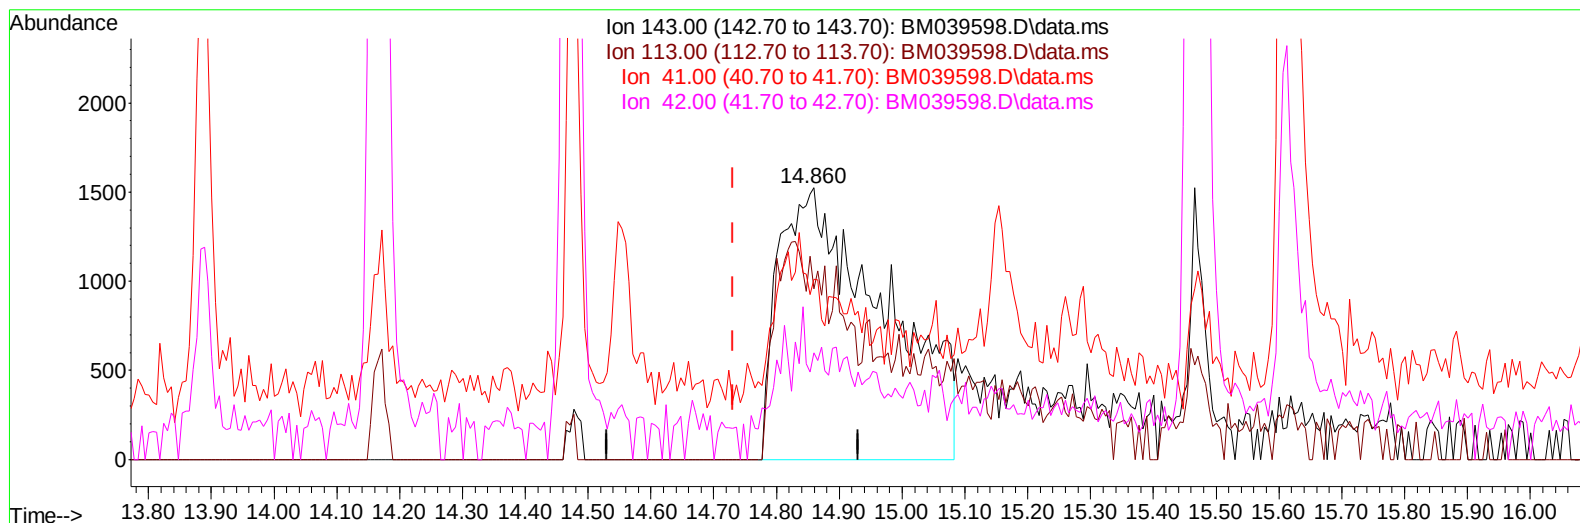

TIC: BM039598.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.860min (+ 0.129) 2.84 ng/ul m

response 17636

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.20	62.97
41.00	39.90	66.38#
42.00	26.60	39.33#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
 Data File : BM039598.D
 Acq On : 23 Apr 2023 04:57
 Operator : CG/JU
 Sample : 02392-10
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE30

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/24/2023
 Supervised By :Jagrut Upadhyay 04/24/2023

Quant Time: Apr 23 05:30:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 23 00:18:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	192578	20.000	ng/ul	0.00
20) Naphthalene-d8	10.625	136	823599	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.471	164	509624	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.224	188	1000100	20.000	ng/ul	0.00
79) Chrysene-d12	21.424	240	768097	20.000	ng/ul	0.00
88) Perylene-d12	23.782	264	803621	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	23285	4.641	ng/uL	0.00
4) Pyridine-d5	3.643	84	90674	6.432	ng/ul	0.01
7) Phenol-d5	7.007	99	88268	5.008	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.148	67	319130	27.393	ng/ul	0.00
11) 2-Chlorophenol-d4	7.348	132	294028	21.266	ng/ul	0.00
15) 4-Methylphenol-d8	8.548	113	174514	12.291	ng/ul	0.00
21) Nitrobenzene-d5	8.989	128	194507	29.355	ng/ul	0.00
24) 2-Nitrophenol-d4	9.713	143	210316	28.267	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.260	165	304096	23.753	ng/ul	0.00
31) 4-Chloroaniline-d4	10.777	131	439094	22.964	ng/ul	0.00
46) Dimethylphthalate-d6	13.889	166	1266151	30.806	ng/ul	0.00
49) Acenaphthylene-d8	14.165	160	1397446	30.265	ng/ul	0.00
54) 4-Nitrophenol-d4	14.860	143	17636m	2.835	ng/ul	0.13
60) Fluorene-d10	15.471	176	1076444	31.967	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.612	200	121464	18.276	ng/ul	0.00
73) Anthracene-d10	17.324	188	1691062	35.160	ng/ul	0.00
81) Pyrene-d10	19.624	212	1802787	35.321	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.630	264	1497482	34.515	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039598.D
Acq On : 23 Apr 2023 04:57
Operator : CG/JU
Sample : 02392-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE30

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/24/2023
Supervised By :Jagrut Upadhyay 04/24/2023

Quant Time: Apr 23 05:30:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 00:18:16 2023
Response via : Initial Calibration

