

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
 Data File : BM039575.D
 Acq On : 22 Apr 2023 14:12
 Operator : CG/JU
 Sample : PB152287BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK287

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039575.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.213	26	30	36	rVB	63067	84933	2.33%	0.205%
2	3.637	99	102	121	rBV	604433	930493	25.51%	2.243%
3	3.966	155	158	165	rVB2	15963	24945	0.68%	0.060%
4	5.107	350	352	356	rVB3	8223	9019	0.25%	0.022%
5	6.707	621	624	630	rBV7	2131	5053	0.14%	0.012%
6	7.007	668	675	694	rBV	604638	1181157	32.39%	2.847%
7	7.154	694	700	714	rVV	590056	971779	26.65%	2.343%
8	7.354	728	734	754	rBV	759313	1295058	35.51%	3.122%
9	7.819	806	813	827	rBV	638310	1067760	29.28%	2.574%
10	8.166	870	872	874	rBV3	3367	3832	0.11%	0.009%
11	8.554	931	938	955	rBV	730067	1454142	39.87%	3.505%
12	8.989	1005	1012	1034	rBV	635756	1188360	32.59%	2.865%
13	9.713	1128	1135	1152	rBV	544559	1038891	28.49%	2.504%
14	10.148	1207	1209	1212	rVB4	4238	4197	0.12%	0.010%
15	10.183	1212	1215	1216	rBV3	3751	4427	0.12%	0.011%
16	10.266	1220	1229	1253	rBV	589984	1425314	39.08%	3.436%
17	10.631	1284	1291	1306	rVB	819681	1442159	39.54%	3.477%
18	10.778	1309	1316	1334	rBV	610243	1326626	36.38%	3.198%
19	12.236	1557	1564	1567	rBV4	8848	17096	0.47%	0.041%
20	13.372	1752	1757	1763	rBV8	6524	11988	0.33%	0.029%
21	13.454	1768	1771	1774	rBV5	3354	4740	0.13%	0.011%
22	13.889	1839	1845	1862	rBV	1393092	2126492	58.31%	5.126%
23	14.171	1886	1893	1910	rBV	1714343	2648617	72.63%	6.385%
24	14.477	1938	1945	1959	rBV	1198177	1832072	50.24%	4.416%
25	14.766	1986	1994	2013	rBV3	110298	554649	15.21%	1.337%
26	15.477	2108	2115	2133	rBV	1917208	3058259	83.86%	7.372%
27	15.618	2133	2139	2153	rVV	414257	763463	20.93%	1.840%
28	15.718	2153	2156	2162	rVB6	13537	24268	0.67%	0.059%
29	16.230	2241	2243	2246	rBV4	2504	3969	0.11%	0.010%
30	17.230	2406	2413	2424	rBV	1393252	2061325	56.52%	4.969%
31	17.330	2424	2430	2442	rVV	2187831	3190896	87.50%	7.692%
32	17.901	2525	2527	2530	rBV4	4649	4380	0.12%	0.011%
33	18.159	2565	2571	2586	rBV7	45075	197185	5.41%	0.475%
34	19.195	2744	2747	2751	rBV3	27151	34379	0.94%	0.083%
35	19.436	2784	2788	2796	rBV9	41750	134058	3.68%	0.323%
36	19.630	2815	2821	2830	rBV	2647709	3646890	100.00%	8.791%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039575.D
Acq On : 22 Apr 2023 14:12
Operator : CG/JU
Sample : PB152287BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK287

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION

37	21.424	3122	3126	3134	rBV	1450235	2025671	55.55%	4.883%
38	23.641	3497	3503	3520	rVB	1735669	3555980	97.51%	8.572%
39	23.794	3523	3529	3542	rVB2	1002951	2128053	58.35%	5.130%




Sum of corrected areas: 41482575

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039575.D
Acq On : 22 Apr 2023 14:12
Operator : CG/JU
Sample : PB152287BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK287

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

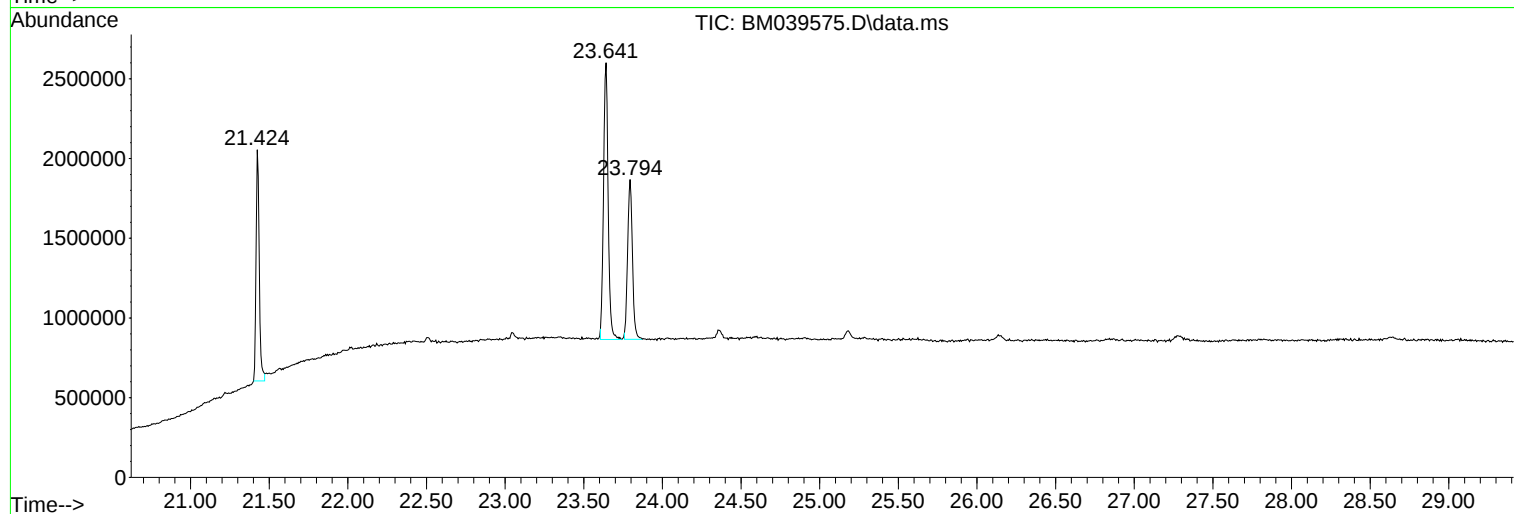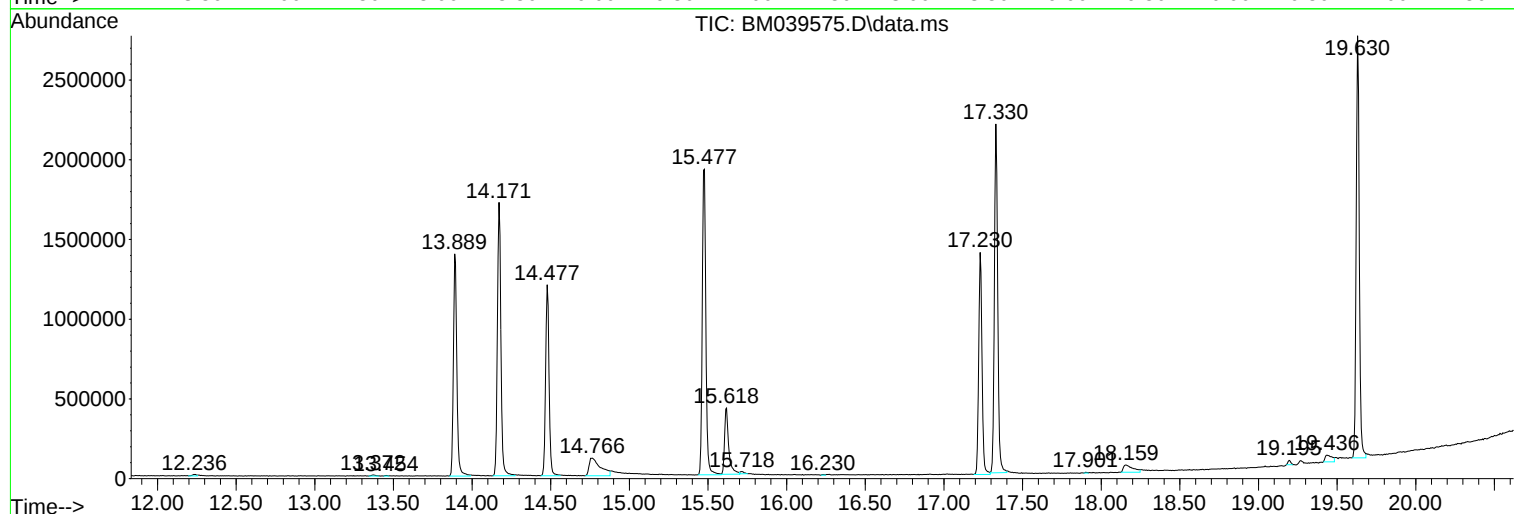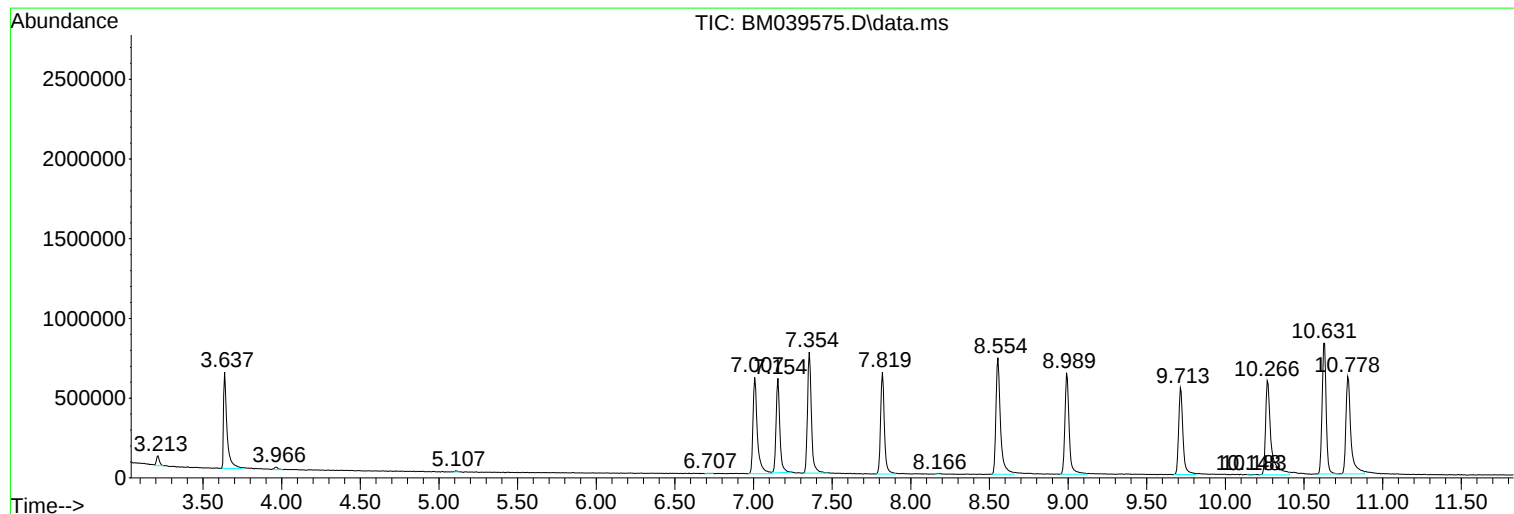

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039575.D
Acq On : 22 Apr 2023 14:12
Operator : CG/JU
Sample : PB152287BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK287

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039575.D
Acq On : 22 Apr 2023 14:12
Operator : CG/JU
Sample : PB152287BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK287

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
