

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
 Data File : BM039576.D
 Acq On : 22 Apr 2023 14:49
 Operator : CG/JU
 Sample : 02440-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COMP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039576.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.207	26	29	33	rVB	35484	43954	0.95%	0.109%
2	3.672	105	108	116	rBV2	15480	37595	0.81%	0.093%
3	3.866	138	141	147	rVB	16697	22018	0.47%	0.055%
4	3.960	154	157	162	rVB	14393	19617	0.42%	0.049%
5	5.501	417	419	425	rVB	10406	12429	0.27%	0.031%
6	7.013	670	676	693	rBV	141925	336921	7.26%	0.834%
7	7.154	694	700	719	rVB	621173	1052314	22.68%	2.605%
8	7.354	728	734	750	rBV	579694	1034930	22.30%	2.562%
9	7.819	806	813	832	rBV	632016	1073124	23.13%	2.657%
10	8.554	932	938	953	rBV	375525	800957	17.26%	1.983%
11	8.931	998	1002	1005	rBV6	3115	4935	0.11%	0.012%
12	8.989	1005	1012	1030	rBV	681583	1276581	27.51%	3.160%
13	9.719	1129	1136	1149	rBV	193117	401815	8.66%	0.995%
14	10.272	1222	1230	1255	rBV	476021	1246965	26.87%	3.087%
15	10.625	1283	1290	1310	rBV	817950	1473375	31.75%	3.648%
16	10.783	1310	1317	1344	rVV	156796	425311	9.17%	1.053%
17	11.995	1518	1523	1524	rBV4	5802	8093	0.17%	0.020%
18	12.236	1558	1564	1566	rBV5	7853	12456	0.27%	0.031%
19	12.766	1650	1654	1658	rBV7	5127	7422	0.16%	0.018%
20	13.366	1755	1756	1761	rVB4	4708	5487	0.12%	0.014%
21	13.448	1766	1770	1775	rBV7	5409	9520	0.21%	0.024%
22	13.807	1827	1831	1839	rBV2	22529	37620	0.81%	0.093%
23	13.889	1839	1845	1859	rBV	1592241	2378601	51.26%	5.889%
24	14.171	1885	1893	1912	rBV	1878527	2886137	62.20%	7.145%
25	14.477	1939	1945	1955	rBV	1298651	1984016	42.76%	4.912%
26	14.554	1955	1958	1965	rVB6	17185	30958	0.67%	0.077%
27	15.471	2106	2114	2140	rBV	2222726	3525218	75.97%	8.728%
28	15.654	2141	2145	2149	rVV7	8614	17166	0.37%	0.042%
29	15.718	2153	2156	2163	rVB5	12136	17803	0.38%	0.044%
30	15.883	2182	2184	2188	rVB5	3742	5071	0.11%	0.013%
31	16.818	2340	2343	2348	rBV6	6597	10525	0.23%	0.026%
32	17.177	2402	2404	2407	rVV4	5173	5758	0.12%	0.014%
33	17.230	2407	2413	2424	rVV	1390178	2033338	43.82%	5.034%
34	17.330	2424	2430	2453	rVB2	2669072	4055275	87.40%	10.040%
35	17.895	2521	2526	2532	rBV	150128	201787	4.35%	0.500%
36	18.148	2565	2569	2576	rBV4	39500	108466	2.34%	0.269%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039576.D
Acq On : 22 Apr 2023 14:49
Operator : CG/JU
Sample : 02440-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMP9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION

37	19.195	2743	2747	2753	rBV2	33697	53493	1.15%	0.132%
38	19.271	2756	2760	2765	rBV	29998	56617	1.22%	0.140%
39	19.436	2782	2788	2797	rBV10	48383	172596	3.72%	0.427%
40	19.630	2815	2821	2832	rBV	3313575	4640159	100.00%	11.488%
41	21.424	3122	3126	3135	rBV	1494968	2102799	45.32%	5.206%
42	23.641	3497	3503	3519	rVB2	2224472	4560412	98.28%	11.290%
43	23.794	3523	3529	3540	rVB2	1035052	2202385	47.46%	5.453%




Sum of corrected areas: 40392019

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039576.D
Acq On : 22 Apr 2023 14:49
Operator : CG/JU
Sample : 02440-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMP9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

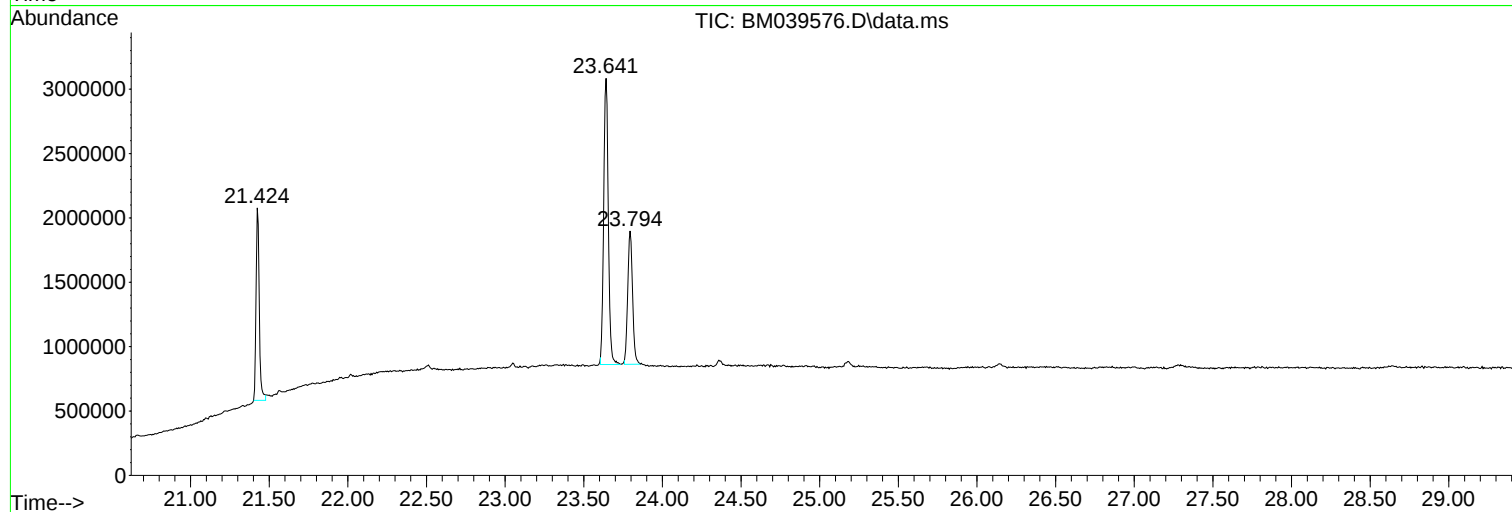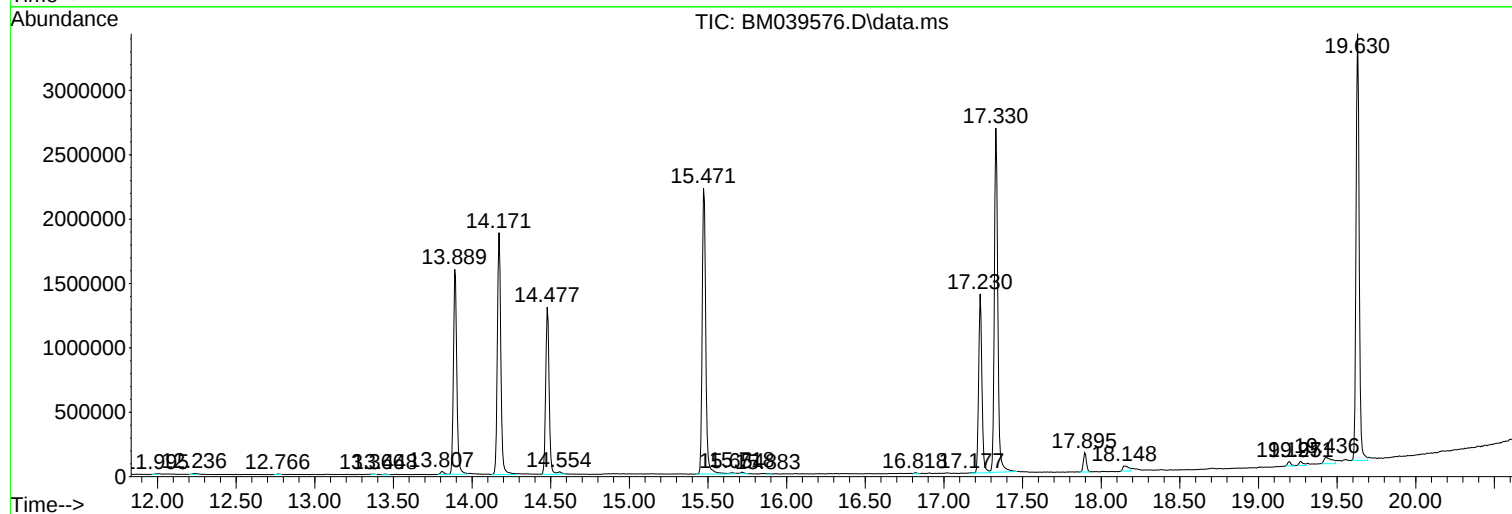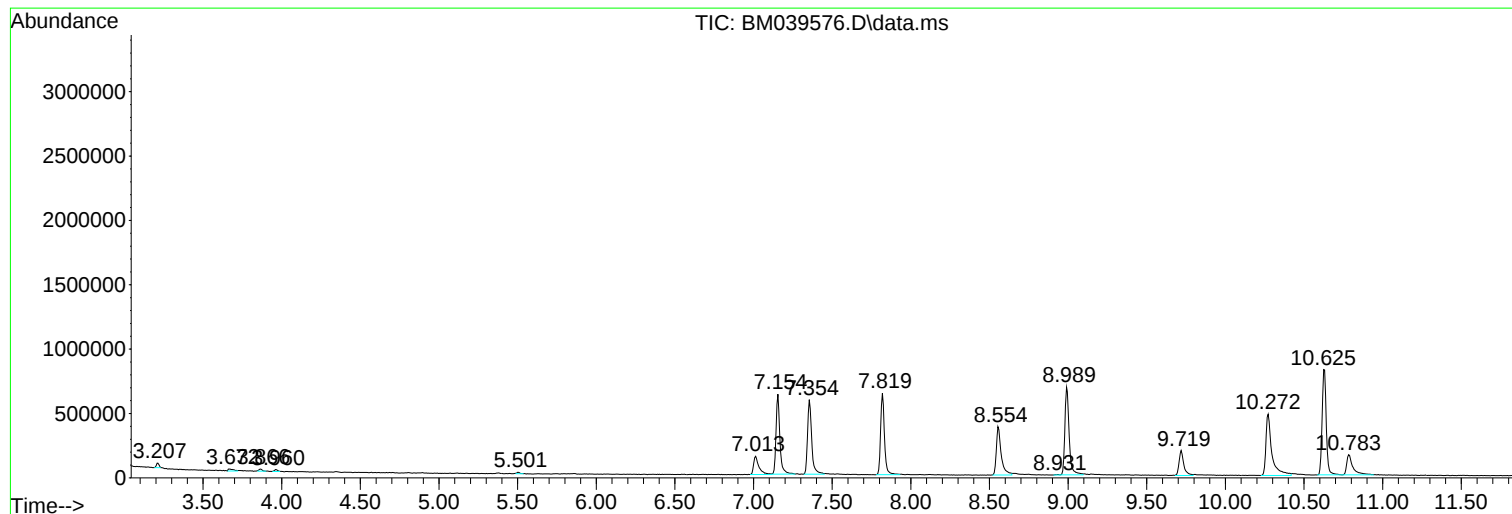

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039576.D
Acq On : 22 Apr 2023 14:49
Operator : CG/JU
Sample : 02440-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMP9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039576.D
Acq On : 22 Apr 2023 14:49
Operator : CG/JU
Sample : 02440-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMP9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc