

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
 Data File : BM039586.D
 Acq On : 22 Apr 2023 21:06
 Operator : CG/JU
 Sample : 02440-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COMQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039586.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.207	26	29	36	rVB	48216	65309	1.43%	0.154%
2	3.860	136	140	147	rVB2	21664	36144	0.79%	0.085%
3	3.960	154	157	163	rVB2	16194	24403	0.53%	0.058%
4	5.378	395	398	402	rVB	7906	11146	0.24%	0.026%
5	5.501	415	419	425	rVB	13031	17540	0.38%	0.041%
6	7.007	669	675	689	rBV	104144	265164	5.81%	0.626%
7	7.148	693	699	719	rVV	628328	1116334	24.46%	2.636%
8	7.348	727	733	750	rBV	583255	1091265	23.91%	2.577%
9	7.813	805	812	825	rBV	627071	1096422	24.03%	2.589%
10	8.548	929	937	952	rBV	330161	737818	16.17%	1.742%
11	8.989	1005	1012	1032	rBV	723988	1370810	30.04%	3.237%
12	9.372	1075	1077	1081	rVB4	5730	7649	0.17%	0.018%
13	9.713	1127	1135	1154	rBV	599434	1159212	25.40%	2.738%
14	10.266	1221	1229	1251	rBV	522980	1400283	30.68%	3.307%
15	10.625	1280	1290	1306	rBV	873383	1523192	33.38%	3.597%
16	10.772	1313	1315	1317	rBV2	5345	6308	0.14%	0.015%
17	11.183	1379	1385	1389	rVB7	3322	4953	0.11%	0.012%
18	11.383	1416	1419	1426	rVB8	3376	8750	0.19%	0.021%
19	11.448	1428	1430	1434	rVB5	3514	4592	0.10%	0.011%
20	11.636	1458	1462	1472	rBV3	14591	28934	0.63%	0.068%
21	12.042	1526	1531	1539	rBV	27123	47385	1.04%	0.112%
22	12.230	1559	1563	1566	rBV4	10102	16690	0.37%	0.039%
23	12.677	1633	1639	1642	rBV7	5847	10507	0.23%	0.025%
24	12.736	1642	1649	1655	rVV10	6098	16445	0.36%	0.039%
25	12.854	1667	1669	1673	rVB5	4386	6644	0.15%	0.016%
26	12.942	1682	1684	1689	rBV4	5632	9303	0.20%	0.022%
27	13.001	1689	1694	1699	rVB	18440	27423	0.60%	0.065%
28	13.289	1734	1743	1753	rBV	47931	85421	1.87%	0.202%
29	13.372	1753	1757	1763	rVB7	10429	17571	0.39%	0.041%
30	13.807	1828	1831	1832	rBV3	4209	5195	0.11%	0.012%
31	13.889	1838	1845	1853	rBV	1815501	2562832	56.16%	6.053%
32	13.989	1860	1862	1872	rVB9	10696	19594	0.43%	0.046%
33	14.060	1872	1874	1881	rVB6	4891	6776	0.15%	0.016%
34	14.166	1885	1892	1911	rBV	1954462	3055792	66.96%	7.217%
35	14.301	1913	1915	1920	rVB6	4832	6913	0.15%	0.016%
36	14.366	1920	1926	1930	rBV2	28948	41687	0.91%	0.098%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
 Data File : BM039586.D
 Acq On : 22 Apr 2023 21:06
 Operator : CG/JU
 Sample : 02440-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COMQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

37	14.477	1936	1945	1962	rBV	1214011	1926925	42.22%	4.551%
38	14.789	1992	1998	1999	rBV4	15991	20402	0.45%	0.048%
39	15.307	2083	2086	2090	rVB5	4560	7245	0.16%	0.017%
40	15.471	2106	2114	2132	rBV	2532593	3754384	82.27%	8.867%
41	15.613	2132	2138	2151	rBV	586660	1069022	23.42%	2.525%
42	15.842	2172	2177	2188	rVB	116475	191984	4.21%	0.453%
43	16.254	2244	2247	2250	rVB4	4904	5003	0.11%	0.012%
44	16.901	2354	2357	2361	rBV6	3471	4752	0.10%	0.011%
45	17.018	2375	2377	2382	rVB6	4126	4666	0.10%	0.011%
46	17.142	2393	2398	2399	rBV5	3839	5037	0.11%	0.012%
47	17.230	2406	2413	2423	rBV	1360051	2066890	45.29%	4.881%
48	17.330	2423	2430	2446	rVV	2624143	4016472	88.01%	9.486%
49	17.642	2480	2483	2486	rBV5	3542	5719	0.13%	0.014%
50	17.907	2523	2528	2531	rBV7	6327	11336	0.25%	0.027%
51	18.136	2563	2567	2575	rBV5	31211	75156	1.65%	0.177%
52	18.412	2612	2614	2618	rBV5	3403	4861	0.11%	0.011%
53	19.195	2742	2747	2754	rBV2	37677	64952	1.42%	0.153%
54	19.265	2755	2759	2762	rBV2	29790	42190	0.92%	0.100%
55	19.418	2781	2785	2792	rBV6	30340	73931	1.62%	0.175%
56	19.624	2815	2820	2830	rBV	3163436	4563647	100.00%	10.778%
57	21.424	3121	3126	3138	rBV	1402824	2044083	44.79%	4.827%
58	23.636	3495	3502	3516	rVB2	2184255	4432922	97.14%	10.469%
59	23.788	3522	3528	3544	rVB2	956140	2038605	44.67%	4.815%




Sum of corrected areas: 42342590

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039586.D
Acq On : 22 Apr 2023 21:06
Operator : CG/JU
Sample : 02440-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMQ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

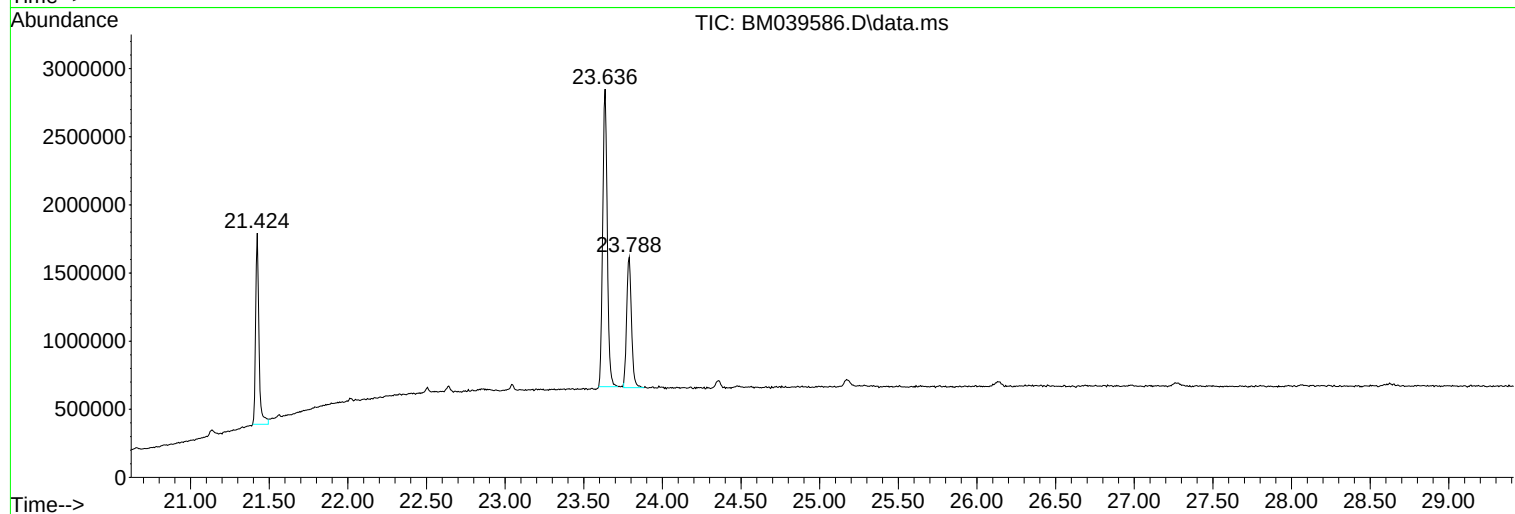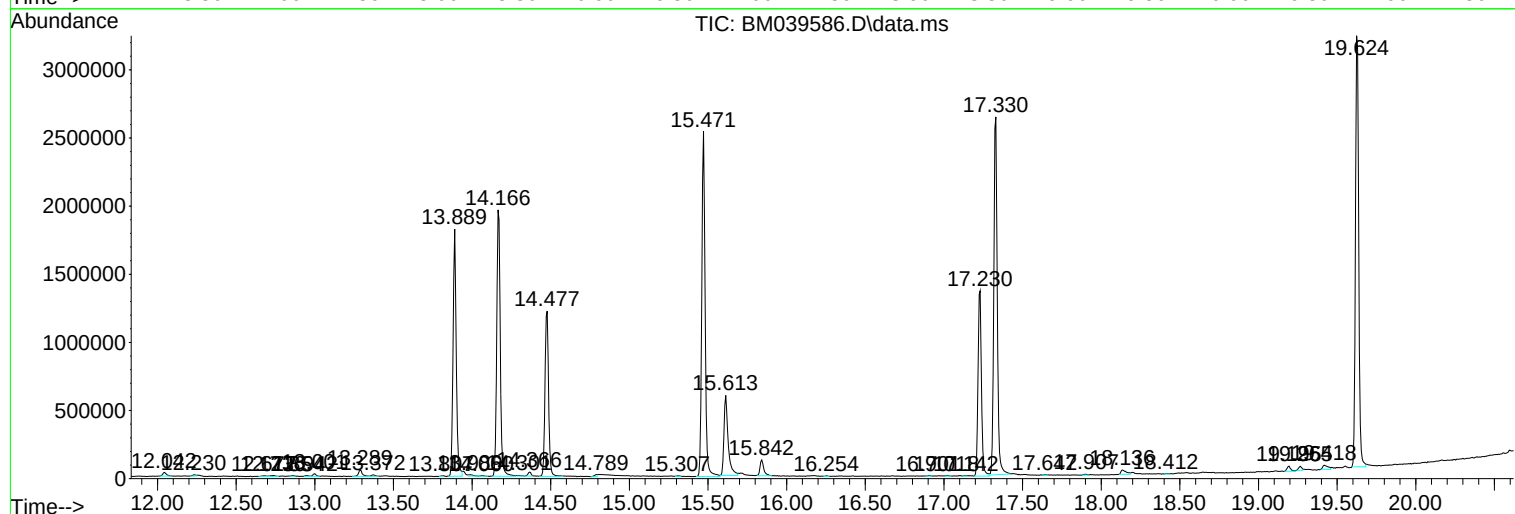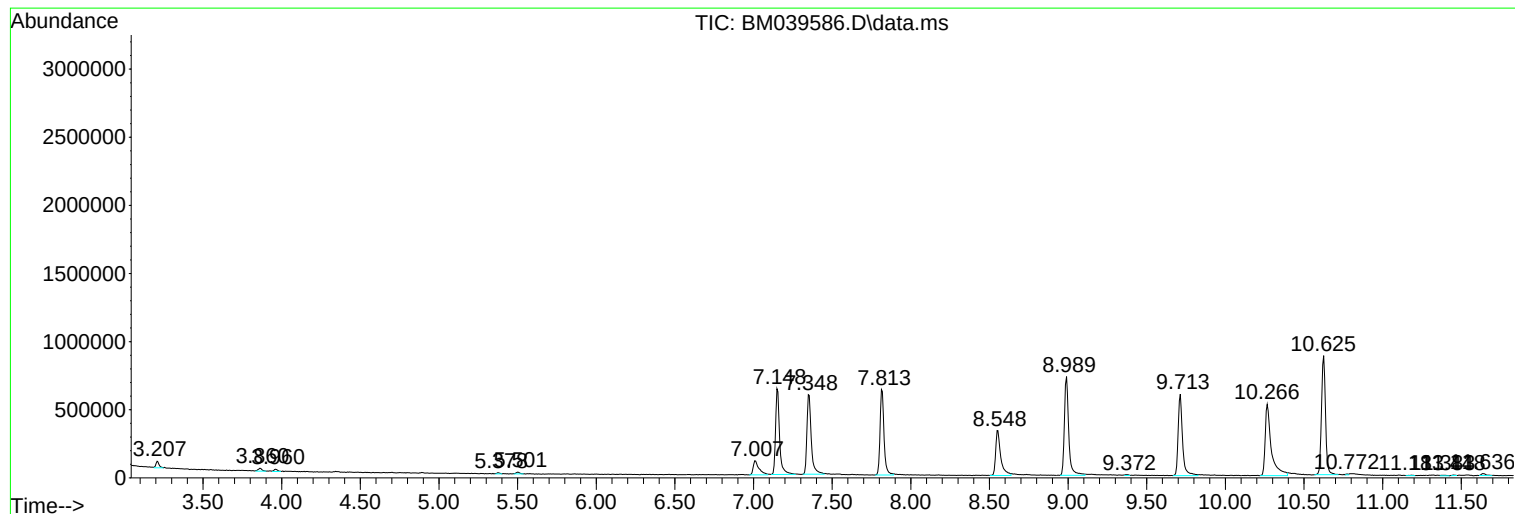

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039586.D
Acq On : 22 Apr 2023 21:06
Operator : CG/JU
Sample : 02440-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0MQ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039586.D
Acq On : 22 Apr 2023 21:06
Operator : CG/JU
Sample : 02440-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0MQ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc