

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
 Data File : BM039589.D
 Acq On : 22 Apr 2023 23:30
 Operator : CG/JU
 Sample : PB152288BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK288

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039589.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.208	26	29	40	rVB	72631	103432	2.45%	0.210%
2	3.631	99	101	122	rBV	669776	1131190	26.82%	2.297%
3	3.960	154	157	162	rVB2	16343	22581	0.54%	0.046%
4	7.001	668	674	694	rBV	710760	1391606	32.99%	2.826%
5	7.148	694	699	723	rVV	685681	1223823	29.01%	2.485%
6	7.348	727	733	754	rVV	870754	1512789	35.86%	3.072%
7	7.813	806	812	827	rBV	712323	1229224	29.14%	2.496%
8	8.548	930	937	960	rBV	914414	1808748	42.88%	3.673%
9	8.989	1005	1012	1028	rBV	798987	1457210	34.55%	2.959%
10	9.713	1128	1135	1159	rBV	678846	1293504	30.67%	2.626%
11	10.260	1222	1228	1254	rBV	715457	1707211	40.47%	3.466%
12	10.625	1283	1290	1305	rVB	1029375	1772421	42.02%	3.599%
13	10.778	1308	1316	1340	rBV	747748	1707268	40.48%	3.467%
14	12.236	1559	1564	1575	rBV6	8735	25689	0.61%	0.052%
15	13.366	1749	1756	1762	rBV7	4160	9469	0.22%	0.019%
16	13.889	1837	1845	1865	rBV	1794147	2715825	64.39%	5.514%
17	14.166	1886	1892	1913	rBV2	2135924	3370536	79.91%	6.844%
18	14.471	1938	1944	1958	rBV	1499274	2333935	55.33%	4.739%
19	14.748	1983	1991	2010	rBV2	133557	654717	15.52%	1.329%
20	15.471	2106	2114	2132	rBV	2587926	3909296	92.68%	7.938%
21	15.613	2132	2138	2152	rBV	577731	1045731	24.79%	2.123%
22	15.848	2176	2178	2185	rVB7	3777	4594	0.11%	0.009%
23	16.907	2354	2358	2362	rVB7	4097	5053	0.12%	0.010%
24	17.018	2373	2377	2381	rVB6	3340	6176	0.15%	0.013%
25	17.230	2406	2413	2423	rBV	1679550	2523994	59.84%	5.125%
26	17.324	2423	2429	2448	rVB	2576534	3934970	93.29%	7.990%
27	17.642	2481	2483	2486	rBV3	3071	4236	0.10%	0.009%
28	18.201	2570	2578	2579	rBV7	5433	11199	0.27%	0.023%
29	18.236	2582	2584	2589	rVV6	3368	4731	0.11%	0.010%
30	19.189	2743	2746	2755	rBV	28317	42470	1.01%	0.086%
31	19.265	2755	2759	2764	rBV	26473	37943	0.90%	0.077%
32	19.624	2814	2820	2833	rBV	2845160	4218027	100.00%	8.565%
33	21.424	3121	3126	3140	rBV	1471440	2299163	54.51%	4.668%
34	23.636	3495	3502	3516	rVB2	1715310	3572182	84.69%	7.253%
35	23.789	3522	3528	3542	rVB2	977225	2158249	51.17%	4.382%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039589.D
Acq On : 22 Apr 2023 23:30
Operator : CG/JU
Sample : PB152288BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK288

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 49249192

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039589.D
Acq On : 22 Apr 2023 23:30
Operator : CG/JU
Sample : PB152288BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK288

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

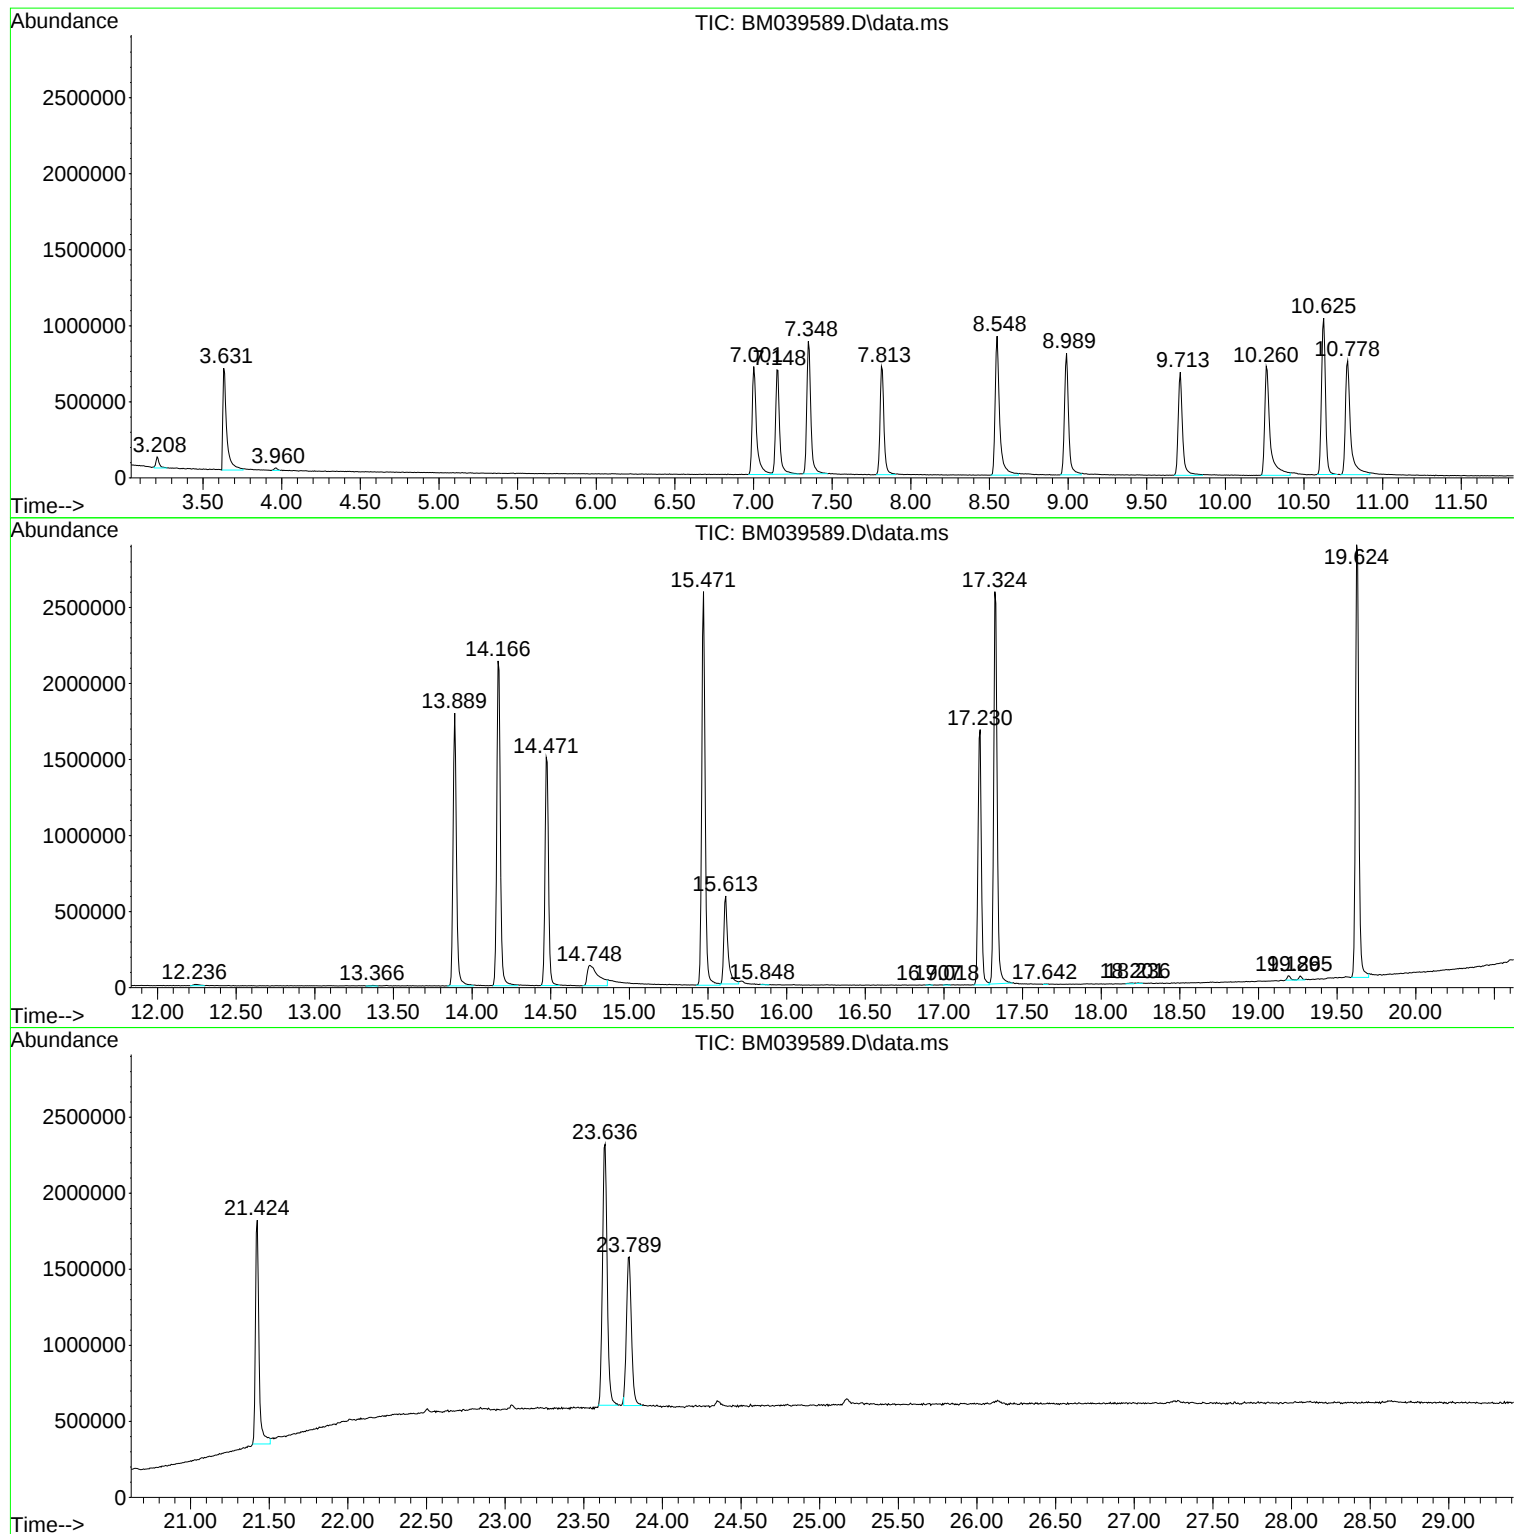

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039589.D
Acq On : 22 Apr 2023 23:30
Operator : CG/JU
Sample : PB152288BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK288

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039589.D
Acq On : 22 Apr 2023 23:30
Operator : CG/JU
Sample : PB152288BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK288

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc