

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
 Data File : BM039590.D
 Acq On : 23 Apr 2023 00:07
 Operator : CG/JU
 Sample : PB152319BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK319

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039590.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.208	26	29	37	rVB	74238	98792	2.13%	0.191%
2	3.631	98	101	130	rBV	760808	1229567	26.57%	2.382%
3	3.961	154	157	164	rVB2	16362	25898	0.56%	0.050%
4	7.002	668	674	693	rBV	790965	1525660	32.97%	2.956%
5	7.149	693	699	720	rVB	755978	1323527	28.60%	2.564%
6	7.349	727	733	754	rBV	955170	1658904	35.85%	3.214%
7	7.813	806	812	827	rBV	633919	1108115	23.95%	2.147%
8	8.549	930	937	952	rBV	986087	1940638	41.94%	3.760%
9	8.990	1005	1012	1030	rBV	890440	1595077	34.47%	3.091%
10	9.713	1128	1135	1151	rBV	735217	1387760	29.99%	2.689%
11	10.260	1221	1228	1255	rBV	806288	1905935	41.19%	3.693%
12	10.625	1282	1290	1303	rBV	914629	1590497	34.37%	3.082%
13	10.778	1309	1316	1349	rBV	866494	1933840	41.79%	3.747%
14	12.242	1558	1565	1574	rBV7	11529	36418	0.79%	0.071%
15	13.366	1750	1756	1763	rBV2	15882	31681	0.68%	0.061%
16	13.448	1767	1770	1774	rVB6	2906	4937	0.11%	0.010%
17	13.889	1838	1845	1865	rBV	1957977	2959265	63.95%	5.734%
18	14.166	1885	1892	1909	rBV	2342835	3655023	78.98%	7.082%
19	14.472	1938	1944	1959	rBV	1343282	2080991	44.97%	4.032%
20	14.742	1983	1990	2013	rBV3	162350	821598	17.75%	1.592%
21	15.472	2107	2114	2132	rBV	2802786	4212217	91.03%	8.161%
22	15.613	2132	2138	2152	rBV	638786	1161686	25.10%	2.251%
23	16.254	2243	2247	2251	rBV7	4760	7420	0.16%	0.014%
24	16.901	2354	2357	2361	rBV5	3963	6469	0.14%	0.013%
25	17.019	2374	2377	2380	rBV5	3179	5000	0.11%	0.010%
26	17.230	2406	2413	2423	rBV	1501968	2234314	48.28%	4.329%
27	17.324	2423	2429	2450	rVB	2801354	4344233	93.88%	8.417%
28	17.901	2525	2527	2532	rVB6	4585	6571	0.14%	0.013%
29	18.183	2569	2575	2578	rBV8	4605	9943	0.21%	0.019%
30	19.189	2743	2746	2754	rVB2	31925	44029	0.95%	0.085%
31	19.265	2755	2759	2763	rVV2	26116	37956	0.82%	0.074%
32	19.624	2814	2820	2835	rBV	3139451	4627518	100.00%	8.966%
33	21.424	3121	3126	3140	rBV	1332011	2006333	43.36%	3.887%
34	23.636	3495	3502	3514	rVB	1957173	3998001	86.40%	7.746%
35	23.789	3522	3528	3543	rVB2	936369	1995801	43.13%	3.867%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039590.D
Acq On : 23 Apr 2023 00:07
Operator : CG/JU
Sample : PB152319BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK319

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 51611614

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039590.D
Acq On : 23 Apr 2023 00:07
Operator : CG/JU
Sample : PB152319BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK319

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

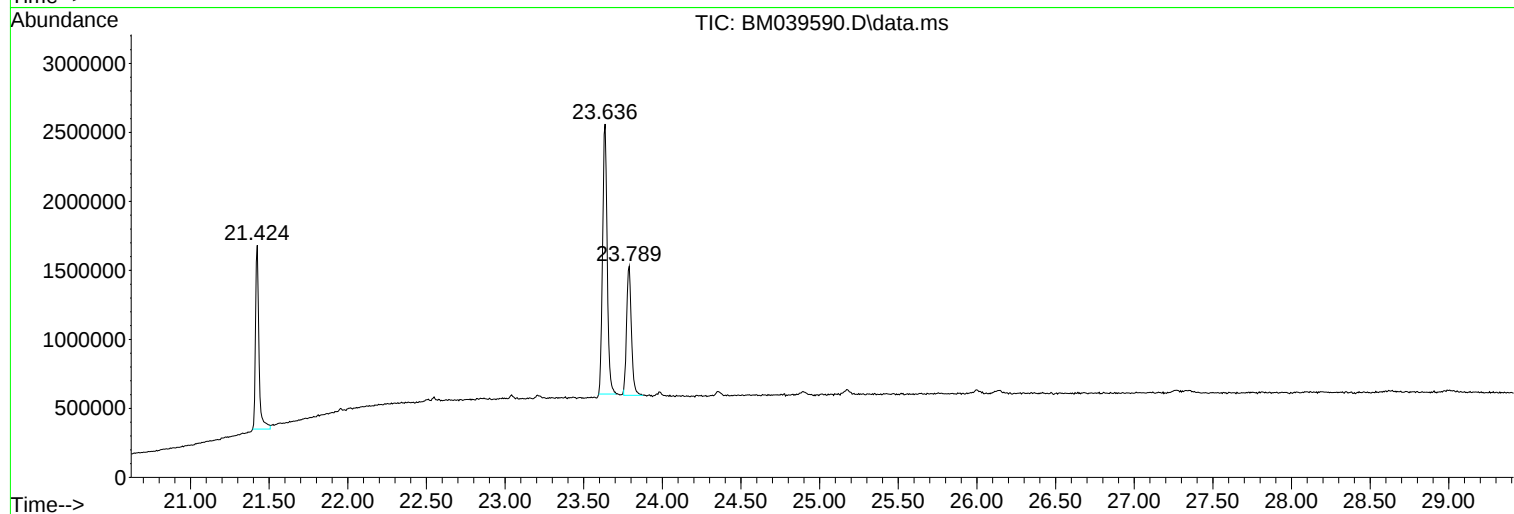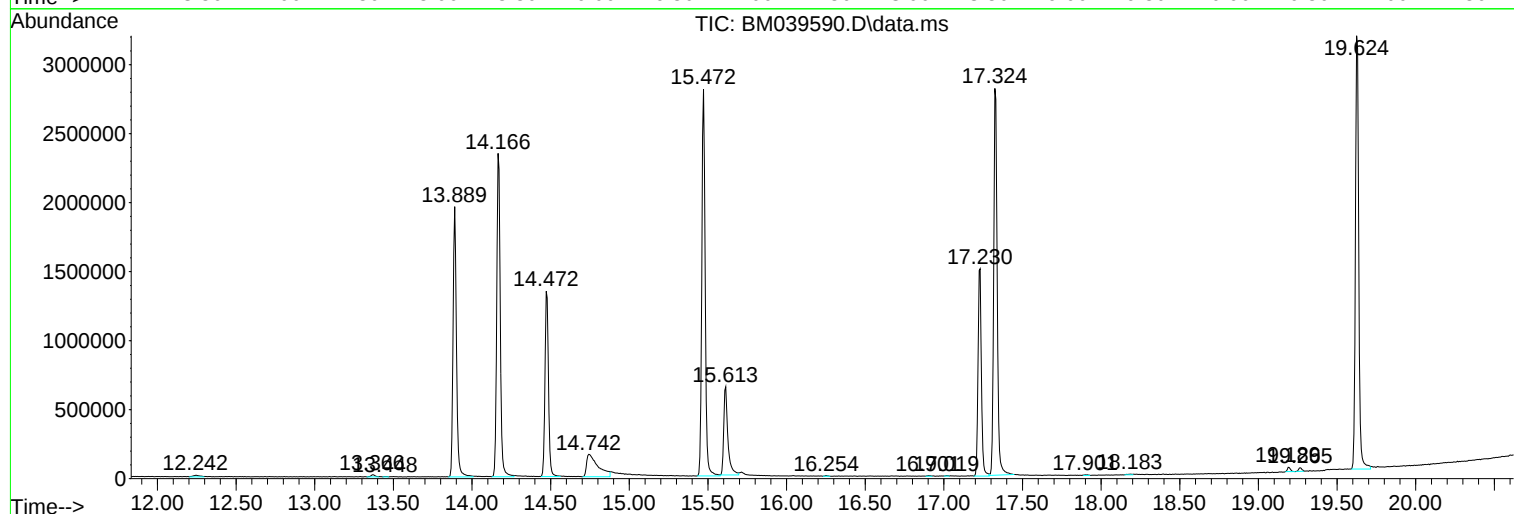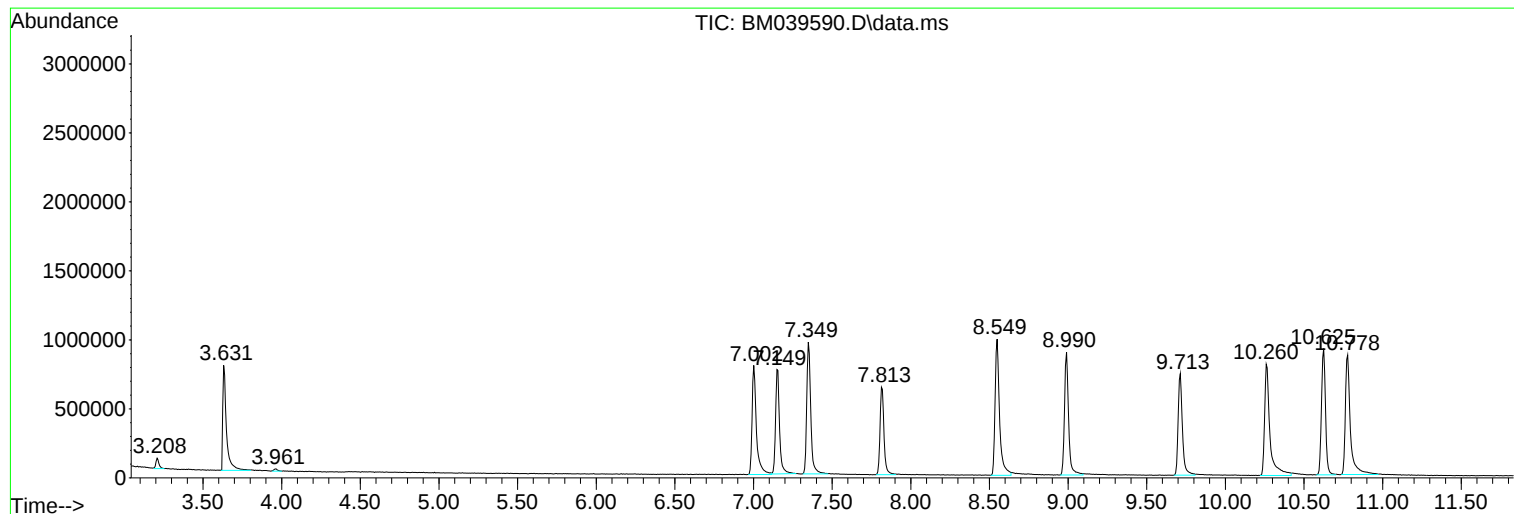

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039590.D
Acq On : 23 Apr 2023 00:07
Operator : CG/JU
Sample : PB152319BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK319

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039590.D
Acq On : 23 Apr 2023 00:07
Operator : CG/JU
Sample : PB152319BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK319

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc