

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
 Data File : BM039594.D
 Acq On : 23 Apr 2023 02:32
 Operator : CG/JU
 Sample : 02440-16
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COMR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039594.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.207	26	29	37	rVB	58736	81524	1.44%	0.156%
2	3.860	136	140	146	rVB	16032	26790	0.47%	0.051%
3	3.960	154	157	164	rVB	17427	23314	0.41%	0.044%
4	5.495	415	418	426	rVB	11592	20425	0.36%	0.039%
5	7.007	669	675	693	rBV	160998	370409	6.53%	0.707%
6	7.148	693	699	726	rVB	804040	1394014	24.58%	2.660%
7	7.348	727	733	755	rBV	783675	1424901	25.12%	2.719%
8	7.813	806	812	823	rBV	711658	1234375	21.76%	2.356%
9	8.548	931	937	954	rBV	540961	1121455	19.77%	2.140%
10	8.989	1005	1012	1035	rBV	938917	1736042	30.61%	3.313%
11	9.372	1074	1077	1084	rVB6	6553	8962	0.16%	0.017%
12	9.713	1127	1135	1150	rBV	776958	1463723	25.81%	2.793%
13	9.842	1155	1157	1164	rVB8	6309	10155	0.18%	0.019%
14	10.260	1220	1228	1253	rBV	744097	1868942	32.95%	3.566%
15	10.625	1282	1290	1309	rBV	1024998	1839318	32.43%	3.510%
16	10.789	1312	1318	1337	rVV	51418	163446	2.88%	0.312%
17	11.348	1407	1413	1421	rVV2	16538	33166	0.58%	0.063%
18	12.242	1558	1565	1570	rBV4	10259	24907	0.44%	0.048%
19	13.371	1752	1757	1761	rVB7	3397	6497	0.11%	0.012%
20	13.460	1765	1772	1775	rBV7	4179	9128	0.16%	0.017%
21	13.889	1838	1845	1861	rBV	2294960	3311859	58.39%	6.320%
22	14.166	1885	1892	1913	rBV2	2609145	4033982	71.12%	7.698%
23	14.471	1938	1944	1959	rBV	1513086	2386048	42.07%	4.553%
24	14.789	1991	1998	2004	rBV5	25402	80837	1.43%	0.154%
25	14.883	2013	2014	2021	rVB7	8743	12887	0.23%	0.025%
26	15.307	2082	2086	2091	rVB6	3319	6658	0.12%	0.013%
27	15.471	2107	2114	2132	rBV	3155860	4792192	84.49%	9.145%
28	15.612	2132	2138	2152	rVV	807928	1496169	26.38%	2.855%
29	15.712	2152	2155	2166	rVV5	28714	74349	1.31%	0.142%
30	15.789	2166	2168	2172	rVV4	6974	10160	0.18%	0.019%
31	15.842	2172	2177	2187	rVB	50398	90315	1.59%	0.172%
32	16.259	2244	2248	2253	rVB8	4476	9407	0.17%	0.018%
33	17.230	2406	2413	2423	rBV	1726079	2587829	45.62%	4.938%
34	17.324	2423	2429	2449	rVB	3493033	5273656	92.98%	10.064%
35	18.136	2563	2567	2575	rBV5	24750	64197	1.13%	0.123%
36	19.189	2742	2746	2754	rBV3	42780	75820	1.34%	0.145%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039594.D
Acq On : 23 Apr 2023 02:32
Operator : CG/JU
Sample : 02440-16
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMR1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION

37	19.265	2755	2759	2764	rVV2	32726	46970	0.83%	0.090%
38	19.418	2781	2785	2791	rBV8	28475	67626	1.19%	0.129%
39	19.624	2814	2820	2831	rBV	3904511	5672033	100.00%	10.824%
40	21.424	3121	3126	3138	rBV	1553631	2341911	41.29%	4.469%
41	23.630	3495	3501	3519	rVB2	2379982	4925793	86.84%	9.400%
42	23.783	3521	3527	3536	rVB2	1030831	2180629	38.45%	4.161%




Sum of corrected areas: 52402820

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039594.D
Acq On : 23 Apr 2023 02:32
Operator : CG/JU
Sample : 02440-16
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMR1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

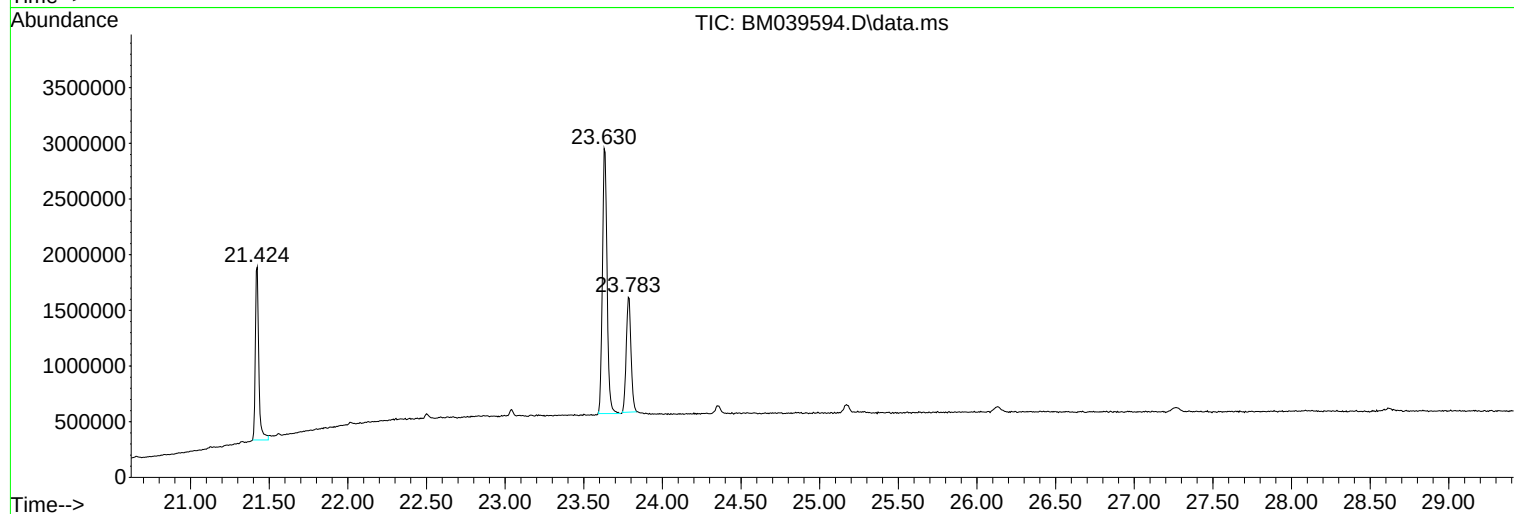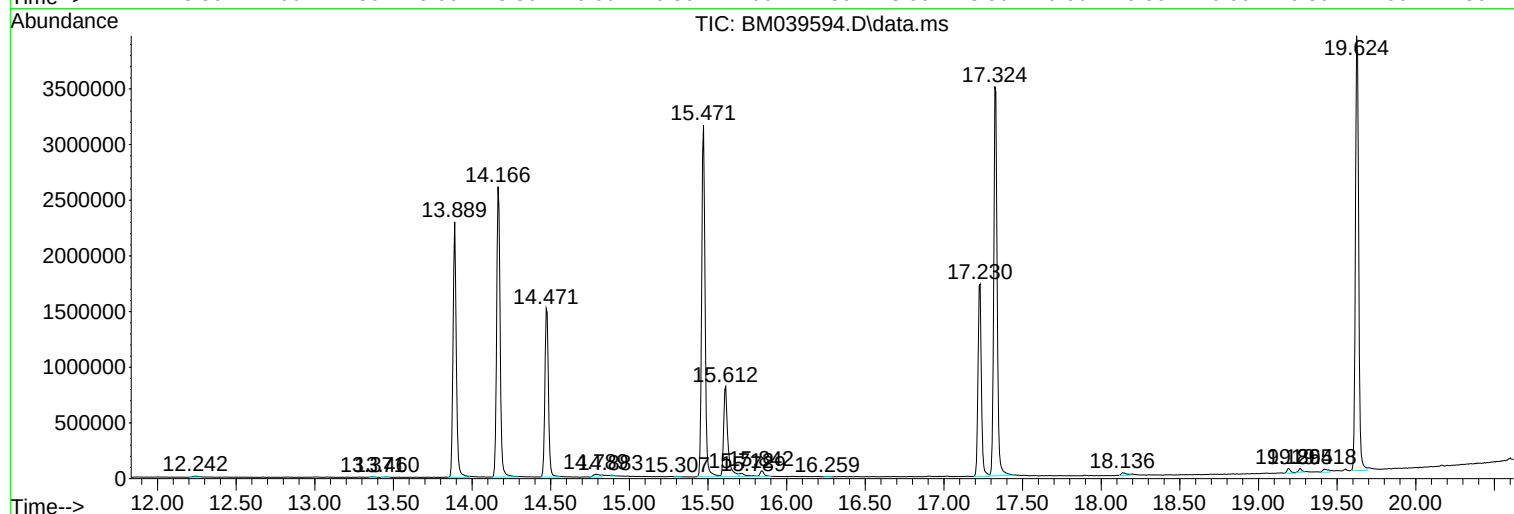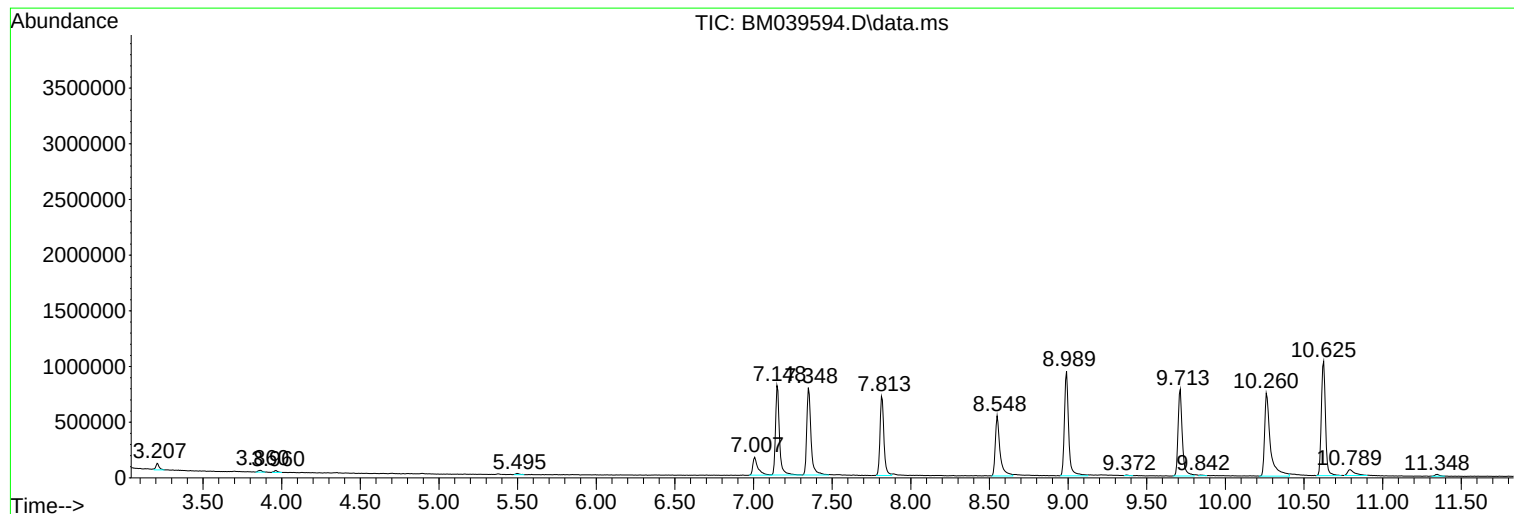

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039594.D
Acq On : 23 Apr 2023 02:32
Operator : CG/JU
Sample : 02440-16
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMR1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039594.D
Acq On : 23 Apr 2023 02:32
Operator : CG/JU
Sample : 02440-16
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMR1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc