

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
 Data File : BM039600.D
 Acq On : 23 Apr 2023 06:09
 Operator : CG/JU
 Sample : 02392-13
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039600.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.172	19	23	27	rBV	186555	258316	3.35%	0.464%
2	3.207	27	29	32	rVB	54035	55838	0.72%	0.100%
3	3.637	99	102	125	rBV	177853	321750	4.17%	0.578%
4	3.960	154	157	162	rVB	21397	31919	0.41%	0.057%
5	4.490	241	247	265	rBV	5093387	7718647	100.00%	13.863%
6	7.007	669	675	692	rBV	102156	267288	3.46%	0.480%
7	7.148	693	699	711	rBV	690035	1170162	15.16%	2.102%
8	7.348	727	733	753	rBV	626940	1147446	14.87%	2.061%
9	7.489	754	757	764	rVB7	11898	18601	0.24%	0.033%
10	7.813	804	812	828	rBV	677432	1204222	15.60%	2.163%
11	8.548	930	937	955	rBV	398635	862551	11.17%	1.549%
12	8.989	1005	1012	1025	rBV	788329	1474816	19.11%	2.649%
13	9.378	1071	1078	1084	rVB8	8712	17215	0.22%	0.031%
14	9.713	1128	1135	1151	rBV	620016	1220647	15.81%	2.192%
15	10.260	1222	1228	1253	rBV	665189	1567249	20.30%	2.815%
16	10.619	1281	1289	1305	rBV	1012772	1767119	22.89%	3.174%
17	10.772	1308	1315	1335	rBV	642061	1482433	19.21%	2.663%
18	12.248	1559	1566	1572	rBV6	9942	26438	0.34%	0.047%
19	13.366	1751	1756	1764	rBV2	22184	38433	0.50%	0.069%
20	13.889	1838	1845	1860	rBV	1933922	2867120	37.15%	5.149%
21	14.165	1885	1892	1911	rBV	2271612	3491252	45.23%	6.270%
22	14.471	1938	1944	1956	rBV	1523834	2329808	30.18%	4.184%
23	14.807	1993	2001	2006	rBV7	14473	47800	0.62%	0.086%
24	14.883	2011	2014	2022	rVB10	6407	14581	0.19%	0.026%
25	15.471	2107	2114	2132	rBV	2703365	4183655	54.20%	7.514%
26	15.607	2132	2137	2151	rBV	599927	1114197	14.44%	2.001%
27	15.842	2172	2177	2187	rVB	35412	68655	0.89%	0.123%
28	16.836	2341	2346	2352	rBV	21314	29274	0.38%	0.053%
29	17.224	2406	2412	2423	rBV	1790537	2530032	32.78%	4.544%
30	17.324	2423	2429	2449	rVB	3027412	4462125	57.81%	8.014%
31	17.901	2522	2527	2533	rVB10	9151	16704	0.22%	0.030%
32	18.130	2561	2566	2576	rBV2	55977	131575	1.70%	0.236%
33	18.983	2707	2711	2715	rBV6	14358	20469	0.27%	0.037%
34	19.189	2743	2746	2753	rVB	37581	50931	0.66%	0.091%
35	19.265	2755	2759	2764	rBV	29842	49819	0.65%	0.089%
36	19.412	2780	2784	2788	rBV5	36306	64255	0.83%	0.115%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039600.D
Acq On : 23 Apr 2023 06:09
Operator : CG/JU
Sample : 02392-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE33

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION

37	19.547	2805	2807	2812	rVB5	17245	19474	0.25%	0.035%
38	19.624	2814	2820	2836	rBV	3540902	4863755	63.01%	8.736%
39	21.130	3072	3076	3086	rBV2	105743	244030	3.16%	0.438%
40	21.418	3121	3125	3138	rBV	1514987	2214506	28.69%	3.977%
41	23.630	3494	3501	3518	rVB2	1936884	4068578	52.71%	7.307%
42	23.782	3521	3527	3543	rVB2	996068	2144253	27.78%	3.851%




Sum of corrected areas: 55677938

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039600.D
Acq On : 23 Apr 2023 06:09
Operator : CG/JU
Sample : 02392-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE33

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

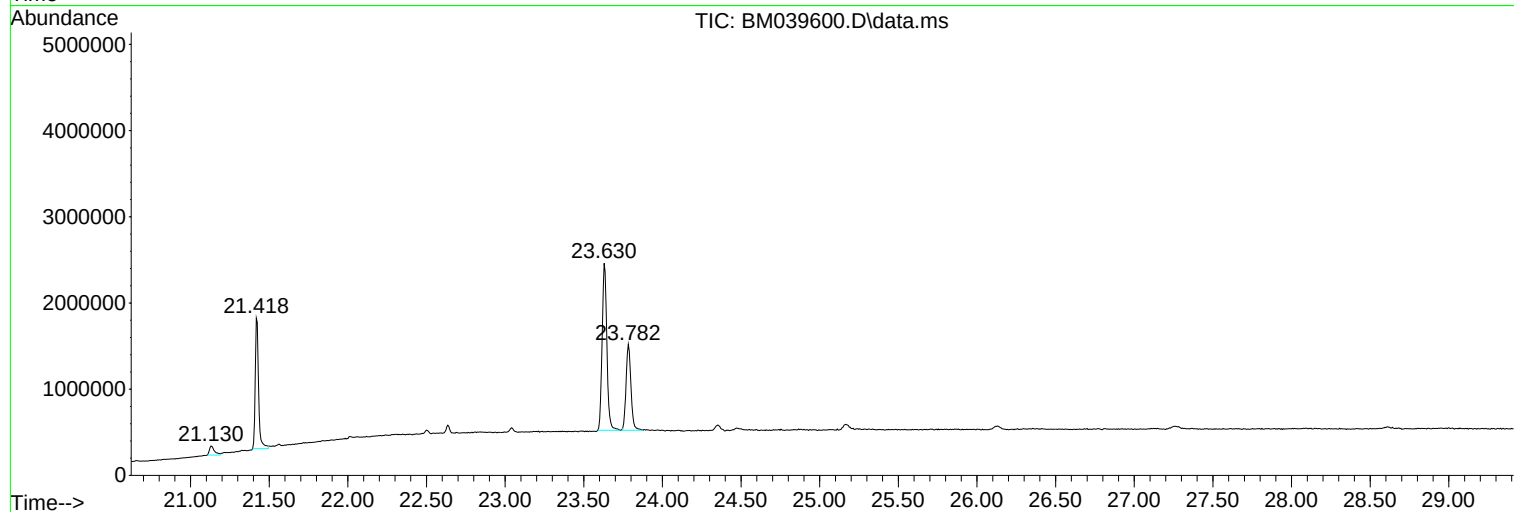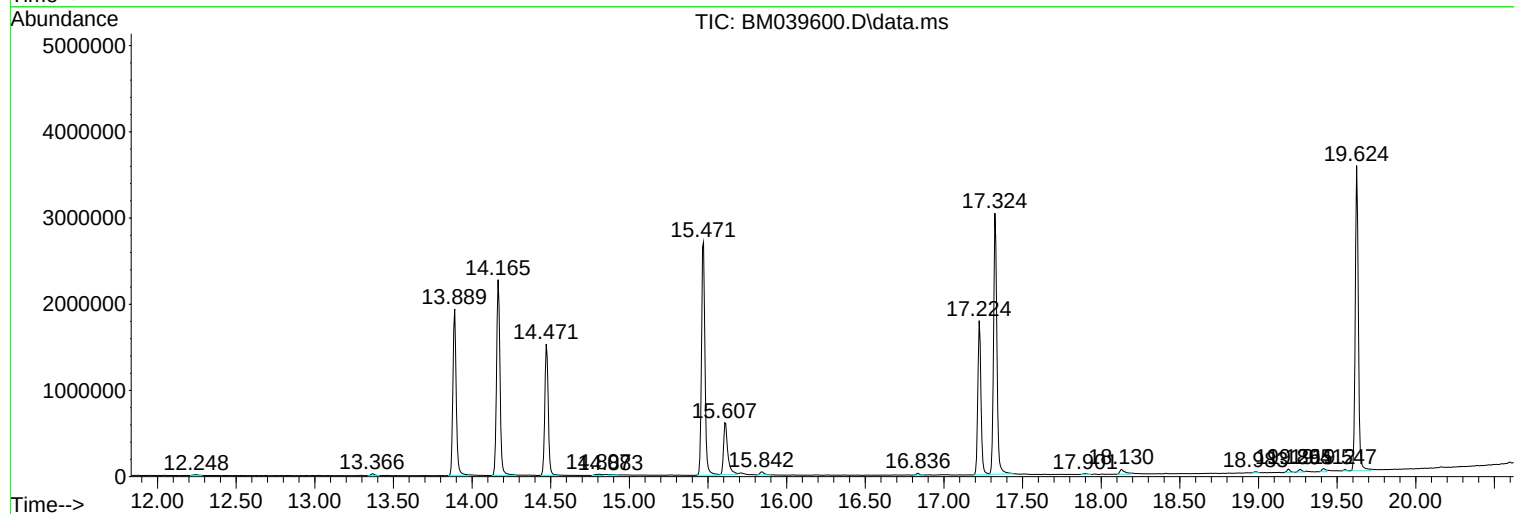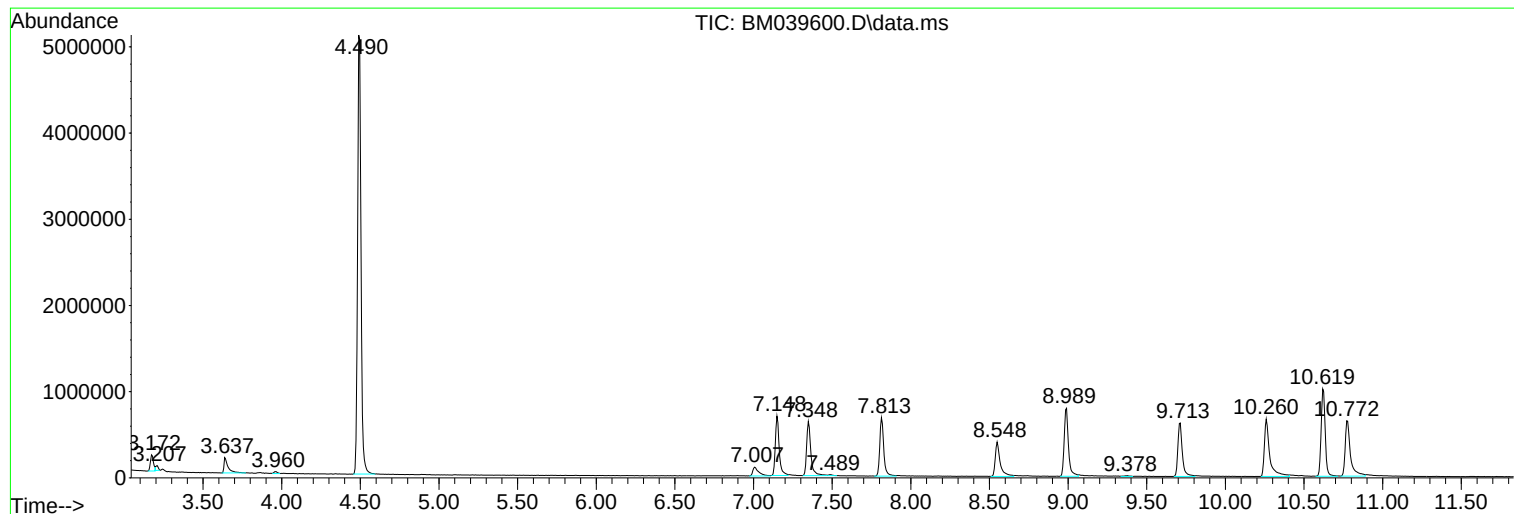

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039600.D
Acq On : 23 Apr 2023 06:09
Operator : CG/JU
Sample : 02392-13
Misc :
ALS Vial : 28 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
BHE33

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.	
21.130	2.20 ng/ul	244030	Chrysene-d12	21.418	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Octadecene, (E)-	252	C18H36	007206-19-1	96
2	1-Tetracosene	336	C24H48	010192-32-2	95
3	Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	94
4	Nonacos-1-ene	406	C29H58	018835-35-3	94
5	13-Tetradecen-1-ol acetate	254	C16H30O2	056221-91-1	93

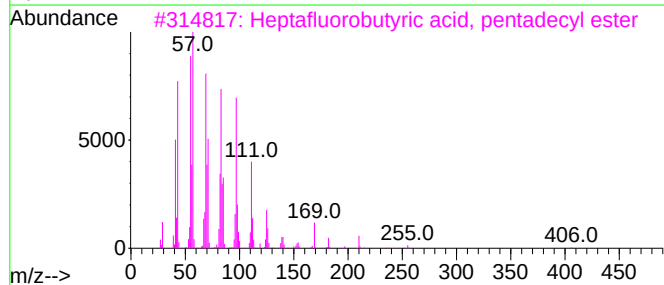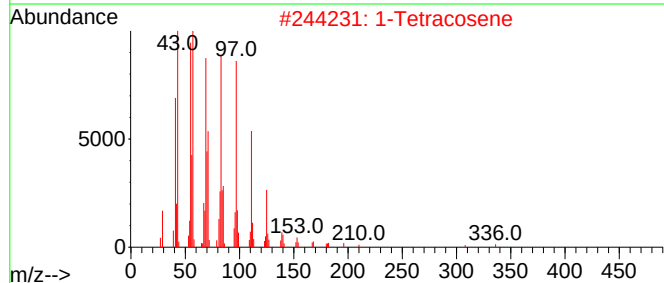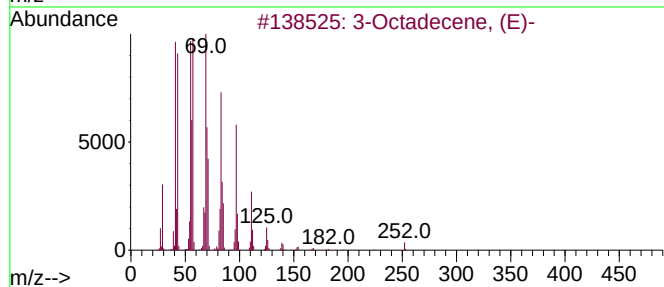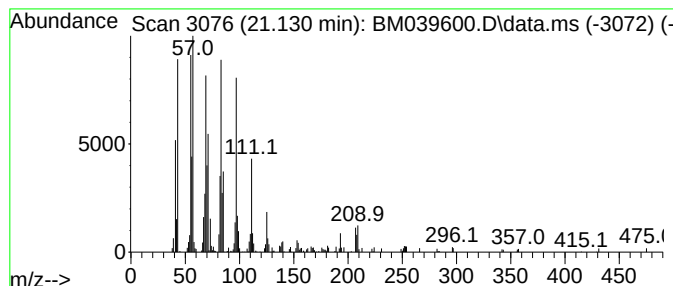

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039600.D
Acq On : 23 Apr 2023 06:09
Operator : CG/JU
Sample : 02392-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE33

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.130	2.2	ng/u1	244030	5	21.418	2214510	20.0