

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
 Data File : BM039605.D
 Acq On : 23 Apr 2023 09:09
 Operator : CG/JU
 Sample : PB152317BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK317

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039605.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.207	25	29	42	rVB	91059	129162	2.45%	0.210%
2	3.631	98	101	122	rBV	898533	1454452	27.58%	2.368%
3	3.960	154	157	165	rVB2	20370	28310	0.54%	0.046%
4	6.995	667	673	691	rBV	917252	1768499	33.54%	2.880%
5	7.148	693	699	717	rVB	924269	1536899	29.14%	2.503%
6	7.343	726	732	754	rBV	1069751	1922353	36.45%	3.130%
7	7.813	805	812	827	rBV	863448	1453414	27.56%	2.367%
8	8.542	930	936	957	rBV	1182468	2265335	42.96%	3.689%
9	8.984	1004	1011	1034	rBV	1032751	1896051	35.95%	3.087%
10	9.707	1127	1134	1148	rBV	871076	1614732	30.62%	2.629%
11	10.254	1220	1227	1250	rBV	949978	2154676	40.86%	3.509%
12	10.619	1281	1289	1305	rBV	1274582	2155920	40.88%	3.511%
13	10.772	1307	1315	1341	rBV	1043596	2274576	43.13%	3.704%
14	12.236	1559	1564	1570	rBV6	10193	26658	0.51%	0.043%
15	13.366	1752	1756	1760	rBV6	5733	8956	0.17%	0.015%
16	13.889	1836	1845	1860	rBV	2215504	3442656	65.28%	5.606%
17	14.166	1885	1892	1912	rBV	2802145	4236151	80.33%	6.898%
18	14.471	1937	1944	1961	rBV	1914599	2791255	52.93%	4.545%
19	14.736	1982	1989	2026	rBV2	189427	1082938	20.54%	1.763%
20	15.107	2049	2052	2059	rVB7	5080	7920	0.15%	0.013%
21	15.466	2107	2113	2131	rBV	3347078	4908099	93.07%	7.992%
22	15.607	2131	2137	2151	rVV	782483	1416726	26.86%	2.307%
23	15.707	2152	2154	2162	rVB4	23680	41113	0.78%	0.067%
24	16.036	2206	2210	2213	rBV6	4096	5844	0.11%	0.010%
25	16.901	2353	2357	2362	rBV8	6071	8568	0.16%	0.014%
26	17.224	2405	2412	2422	rBV	2000924	2946652	55.88%	4.798%
27	17.324	2423	2429	2453	rVB	3424361	5034114	95.46%	8.197%
28	19.189	2742	2746	2753	rBV2	37255	56311	1.07%	0.092%
29	19.265	2754	2759	2763	rBV	30878	46834	0.89%	0.076%
30	19.624	2814	2820	2840	rBV	3722290	5273515	100.00%	8.587%
31	21.424	3121	3126	3139	rBV	1586942	2488694	47.19%	4.052%
32	23.630	3494	3501	3516	rBV2	2144436	4476512	84.89%	7.289%
33	23.783	3521	3527	3541	rVB2	1123309	2458521	46.62%	4.003%




Sum of corrected areas: 61412416

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039605.D
Acq On : 23 Apr 2023 09:09
Operator : CG/JU
Sample : PB152317BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK317

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

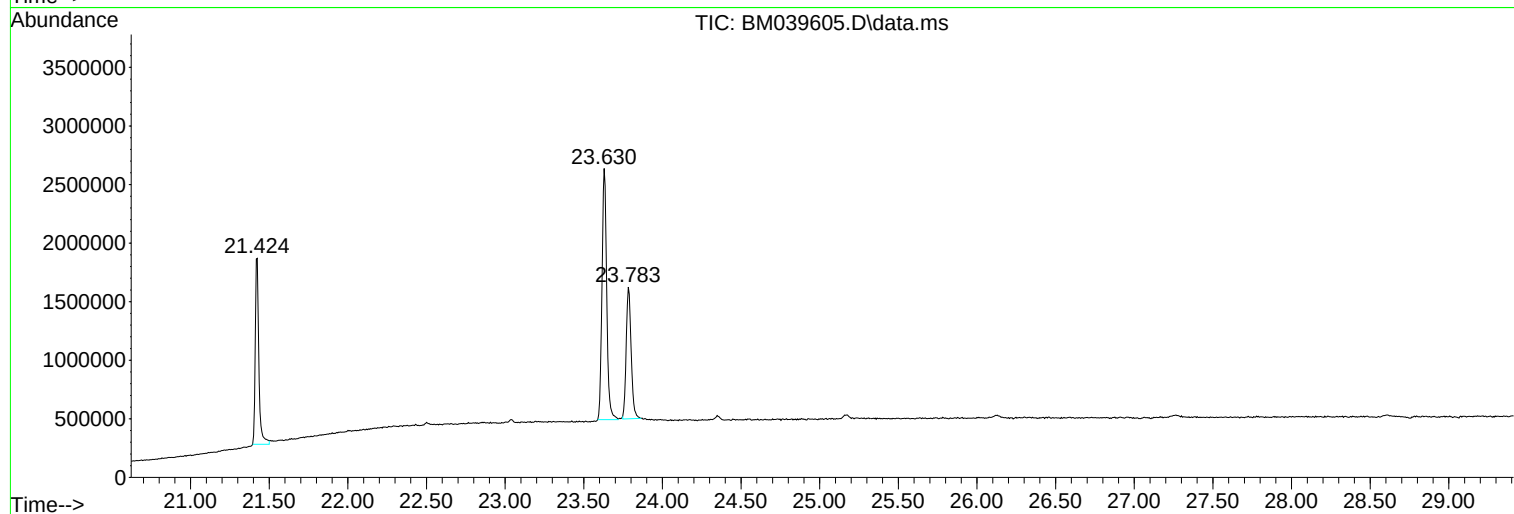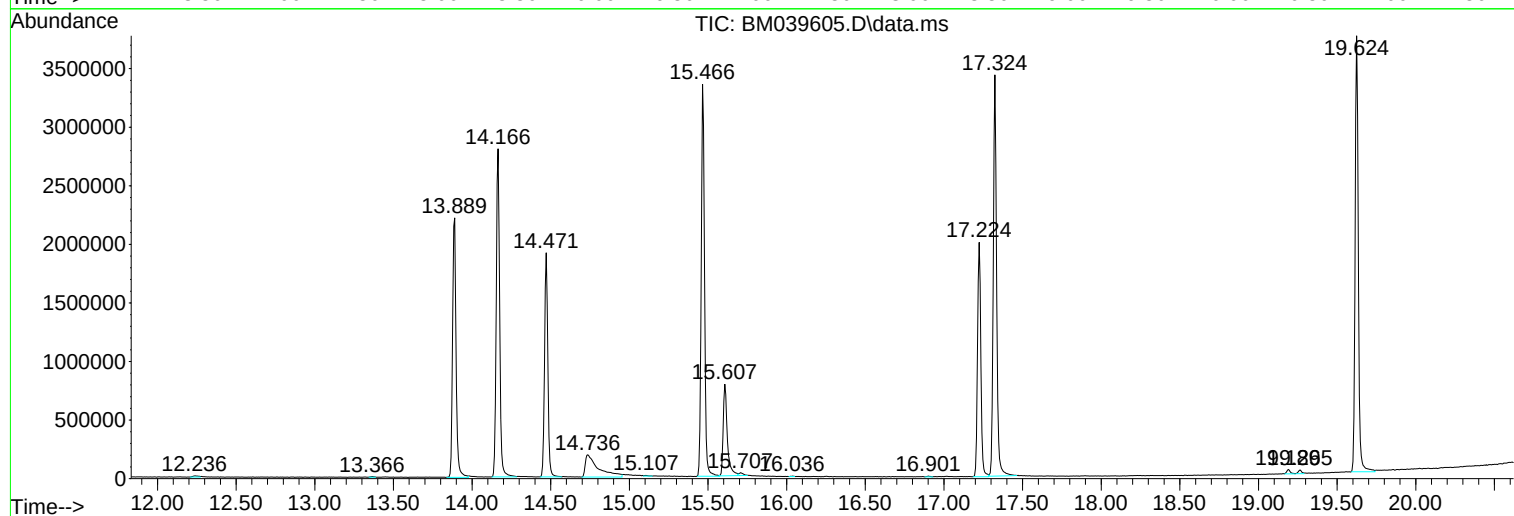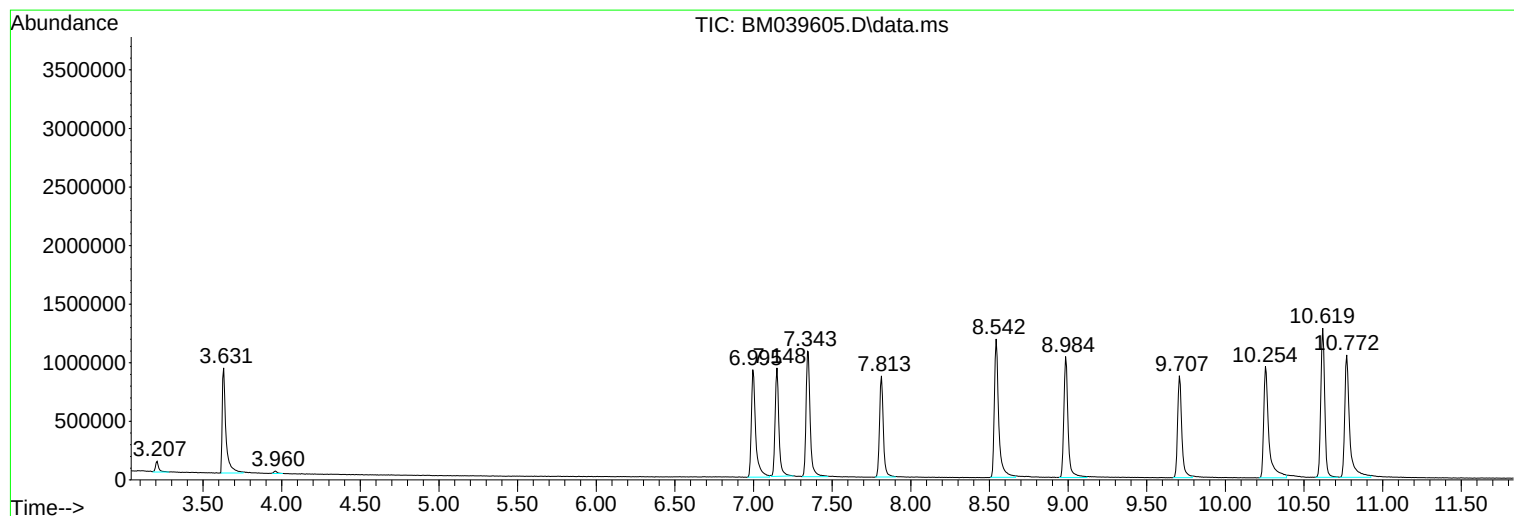

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039605.D
Acq On : 23 Apr 2023 09:09
Operator : CG/JU
Sample : PB152317BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK317

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042223\
Data File : BM039605.D
Acq On : 23 Apr 2023 09:09
Operator : CG/JU
Sample : PB152317BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK317

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------