

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042522\
 Data File : BM034798.D
 Acq On : 25 Apr 2022 14:39
 Operator : CG/JU
 Sample : N2471-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFFG2

Quant Time: Apr 26 03:04:22 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 22 16:54:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.943	152	5918	0.400	ng/ul	0.00
4) Naphthalene-d8	10.743	136	15083	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.571	164	8076	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.310	188	14869	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.487	240	10349	0.400	ng/ul	# 0.00
23) Perylene-d12	23.881	264	11670	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.382	96	33216	5.075	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	8249	0.389	ng/ul	0.00
18) Fluoranthene-d10	19.337	212	15008	0.460	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.792	128	1172	0.027	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042522\
Data File : BM034798.D
Acq On : 25 Apr 2022 14:39
Operator : CG/JU
Sample : N2471-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFFG2


Quant Time: Apr 26 03:04:22 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 22 16:54:34 2022
Response via : Initial Calibration

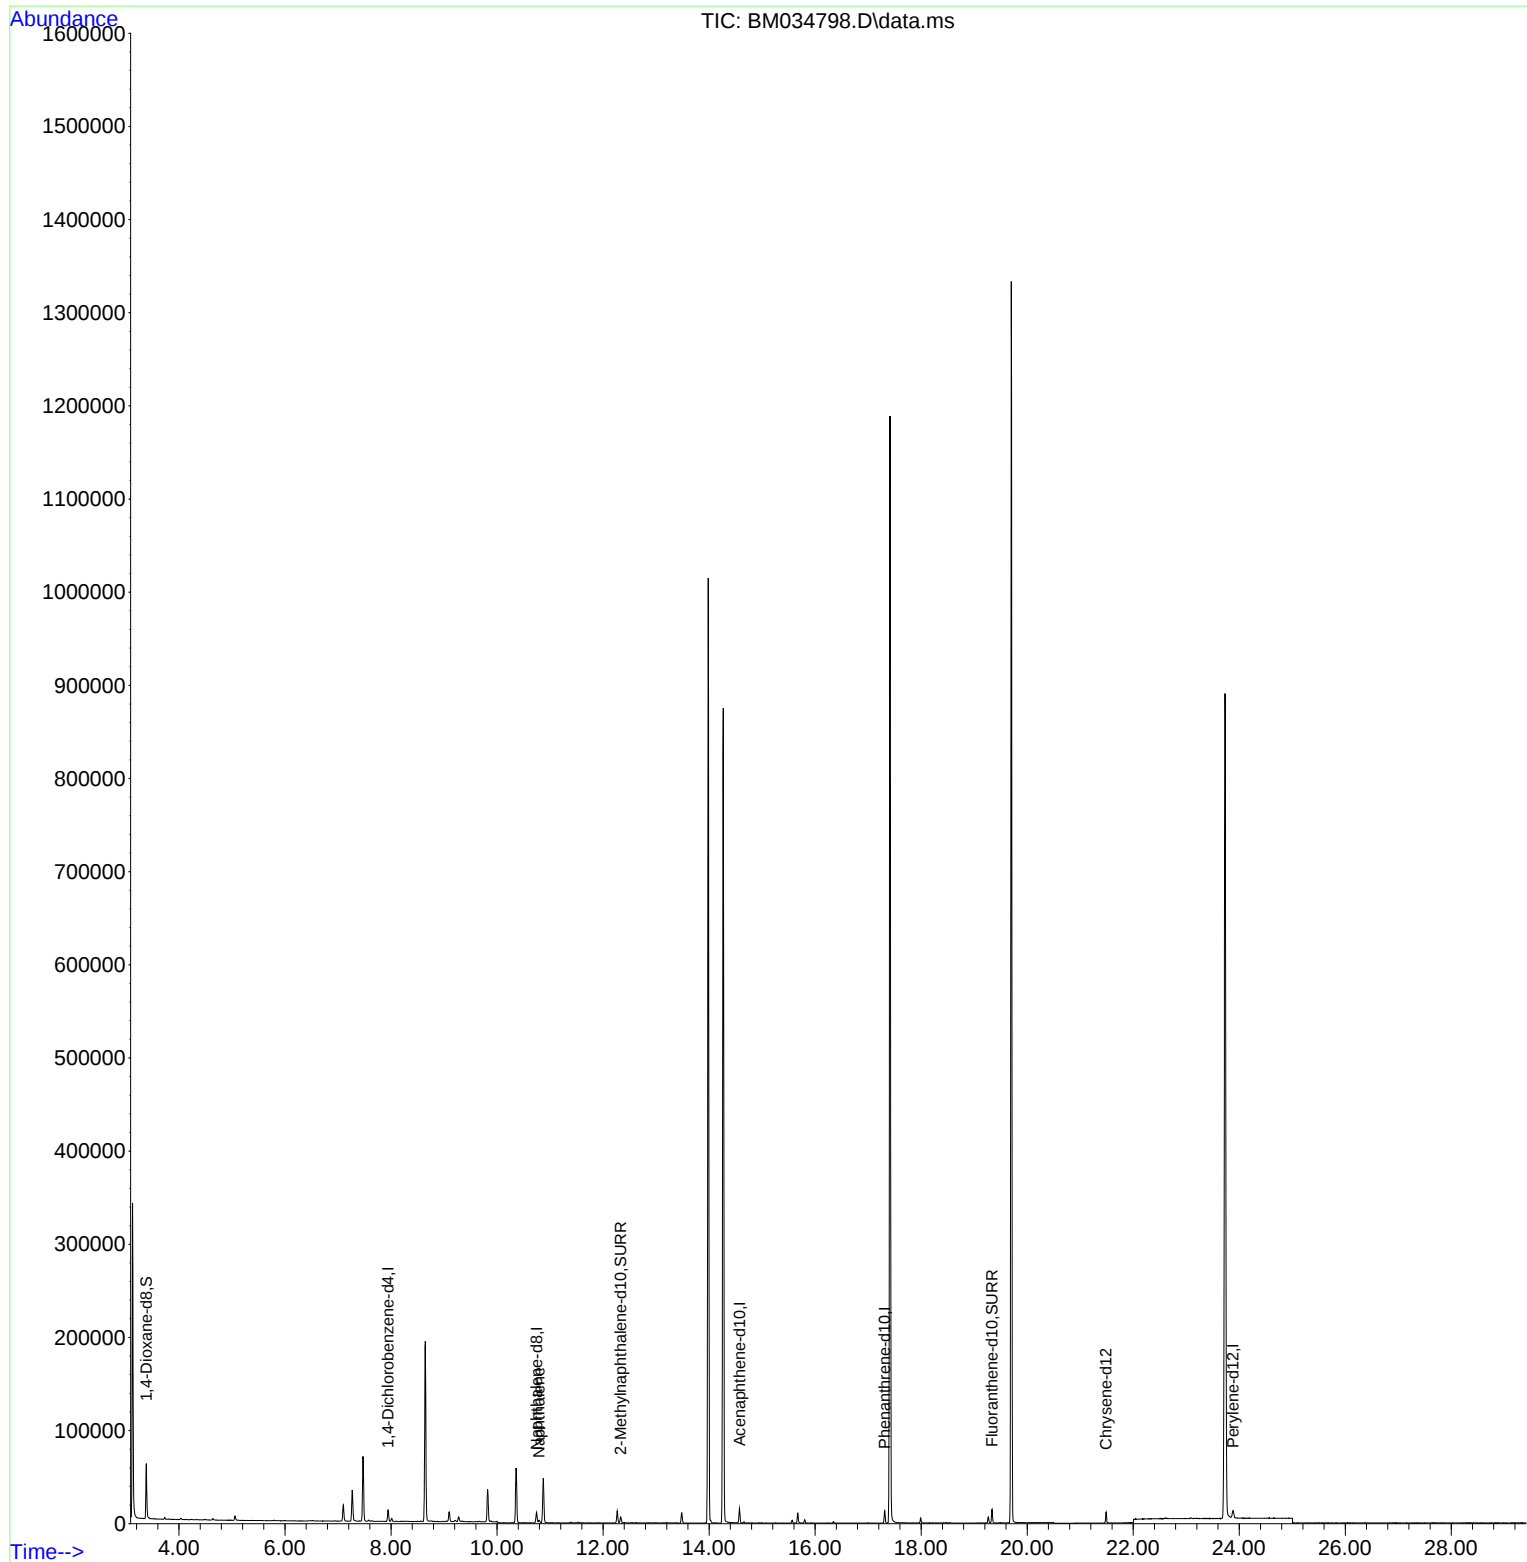

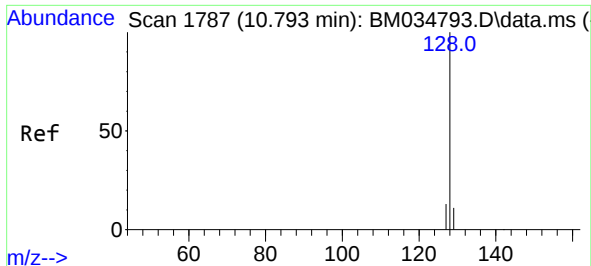

#5
Naphthalene
Concen: 0.027 ng/ul
RT: 10.792 min Scan# 11
Delta R.T. -0.004 min
Lab File: BM034798.D
Acq: 25 Apr 2022 14:39

Instrument :
BNA_M
ClientSampleId :
BFFG2

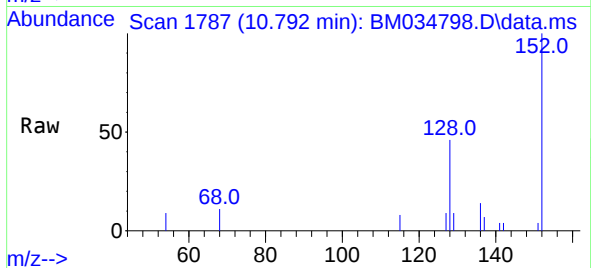

Tgt Ion:	128	Resp:	1172
Ion	Ratio	Lower	Upper
128	100		
129	19.8	13.4	20.2
127	19.0	15.2	22.8

