

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042522\
 Data File : BM034807.D
 Acq On : 25 Apr 2022 20:02
 Operator : CG/JU
 Sample : N2475-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A0BM6

Quant Time: Apr 26 03:06:29 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 22 16:54:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.943	152	6943	0.400	ng/ul	0.00
4) Naphthalene-d8	10.743	136	18106	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.571	164	9614	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.309	188	17020	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.488	240	11095	0.400	ng/ul	# 0.00
23) Perylene-d12	23.882	264	12032	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.382	96	32268	4.202	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	9179	0.361	ng/ul	0.00
18) Fluoranthene-d10	19.336	212	16303	0.466	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.420	88	882	0.121	ng/ul#	71

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042522\
Data File : BM034807.D
Acq On : 25 Apr 2022 20:02
Operator : CG/JU
Sample : N2475-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A0BM6

Quant Time: Apr 26 03:06:29 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 22 16:54:34 2022
Response via : Initial Calibration

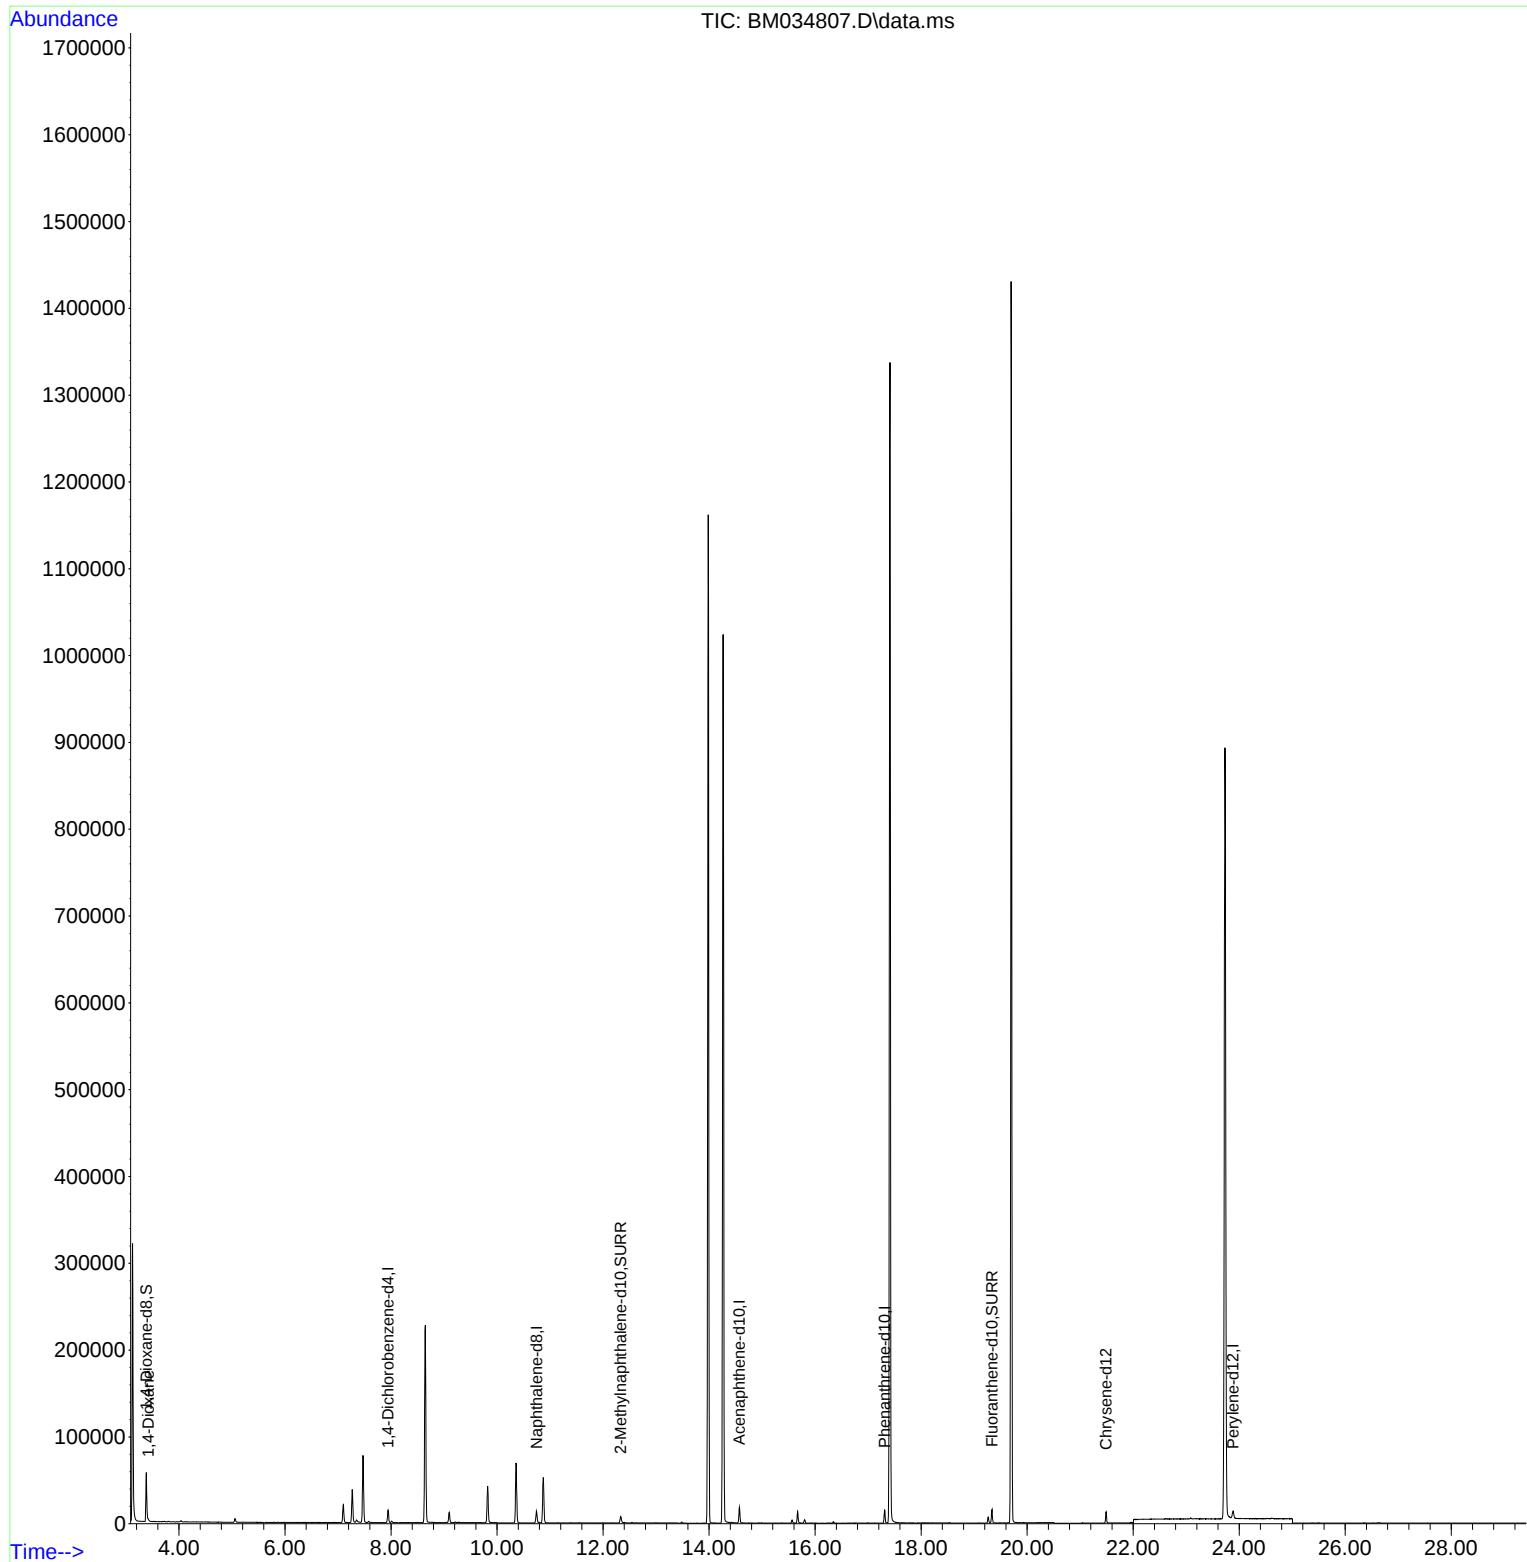


Abundance Scan 80 (3.420 min): BM034801.D\data.ms (-72)

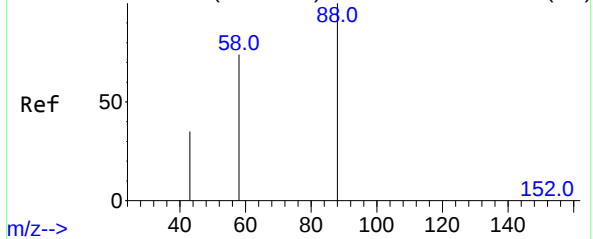


m/z-->

Abundance Scan 80 (3.420 min): BM034807.D\data.ms

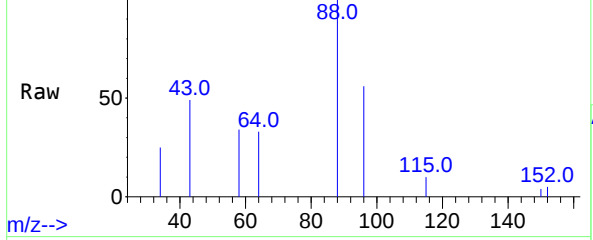

m/z-->

Abundance Scan 80 (3.420 min): BM034807.D\data.ms (-68)

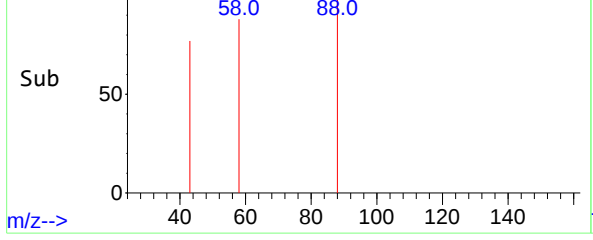


m/z-->

#2
1,4-Dioxane
Concen: 0.121 ng/ul
RT: 3.420 min Scan# 80
Delta R.T. 0.000 min
Lab File: BM034807.D
Acq: 25 Apr 2022 20:02

Instrument :
BNA_M
ClientSampleId :
A0BM6

Tgt Ion:	88	Resp:	882
Ion	Ratio	Lower	Upper
88	100		
43	49.3	49.7	74.5#
58	34.0	52.5	78.7#

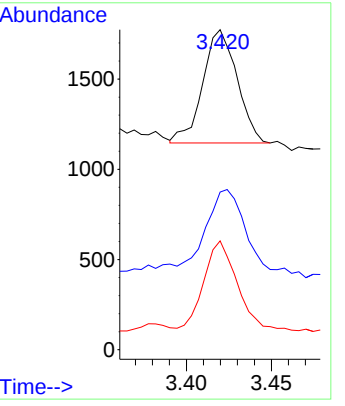

Time-->