

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042622\
 Data File : BM034841.D
 Acq On : 26 Apr 2022 17:52
 Operator : CG/JU
 Sample : N2517-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFFH1

Quant Time: Apr 27 01:27:03 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 22 16:54:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.942	152	5835	0.400	ng/ul	0.00
4) Naphthalene-d8	10.743	136	15355	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.571	164	8294	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.310	188	15755	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.487	240	11824	0.400	ng/ul	# 0.00
23) Perylene-d12	23.884	264	12820	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.382	96	19734	3.058	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.327	152	7516	0.348	ng/ul	0.00
18) Fluoranthene-d10	19.336	212	15180	0.407	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.420	88	433	0.070	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042622\
Data File : BM034841.D
Acq On : 26 Apr 2022 17:52
Operator : CG/JU
Sample : N2517-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFFH1

Quant Time: Apr 27 01:27:03 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 22 16:54:34 2022
Response via : Initial Calibration

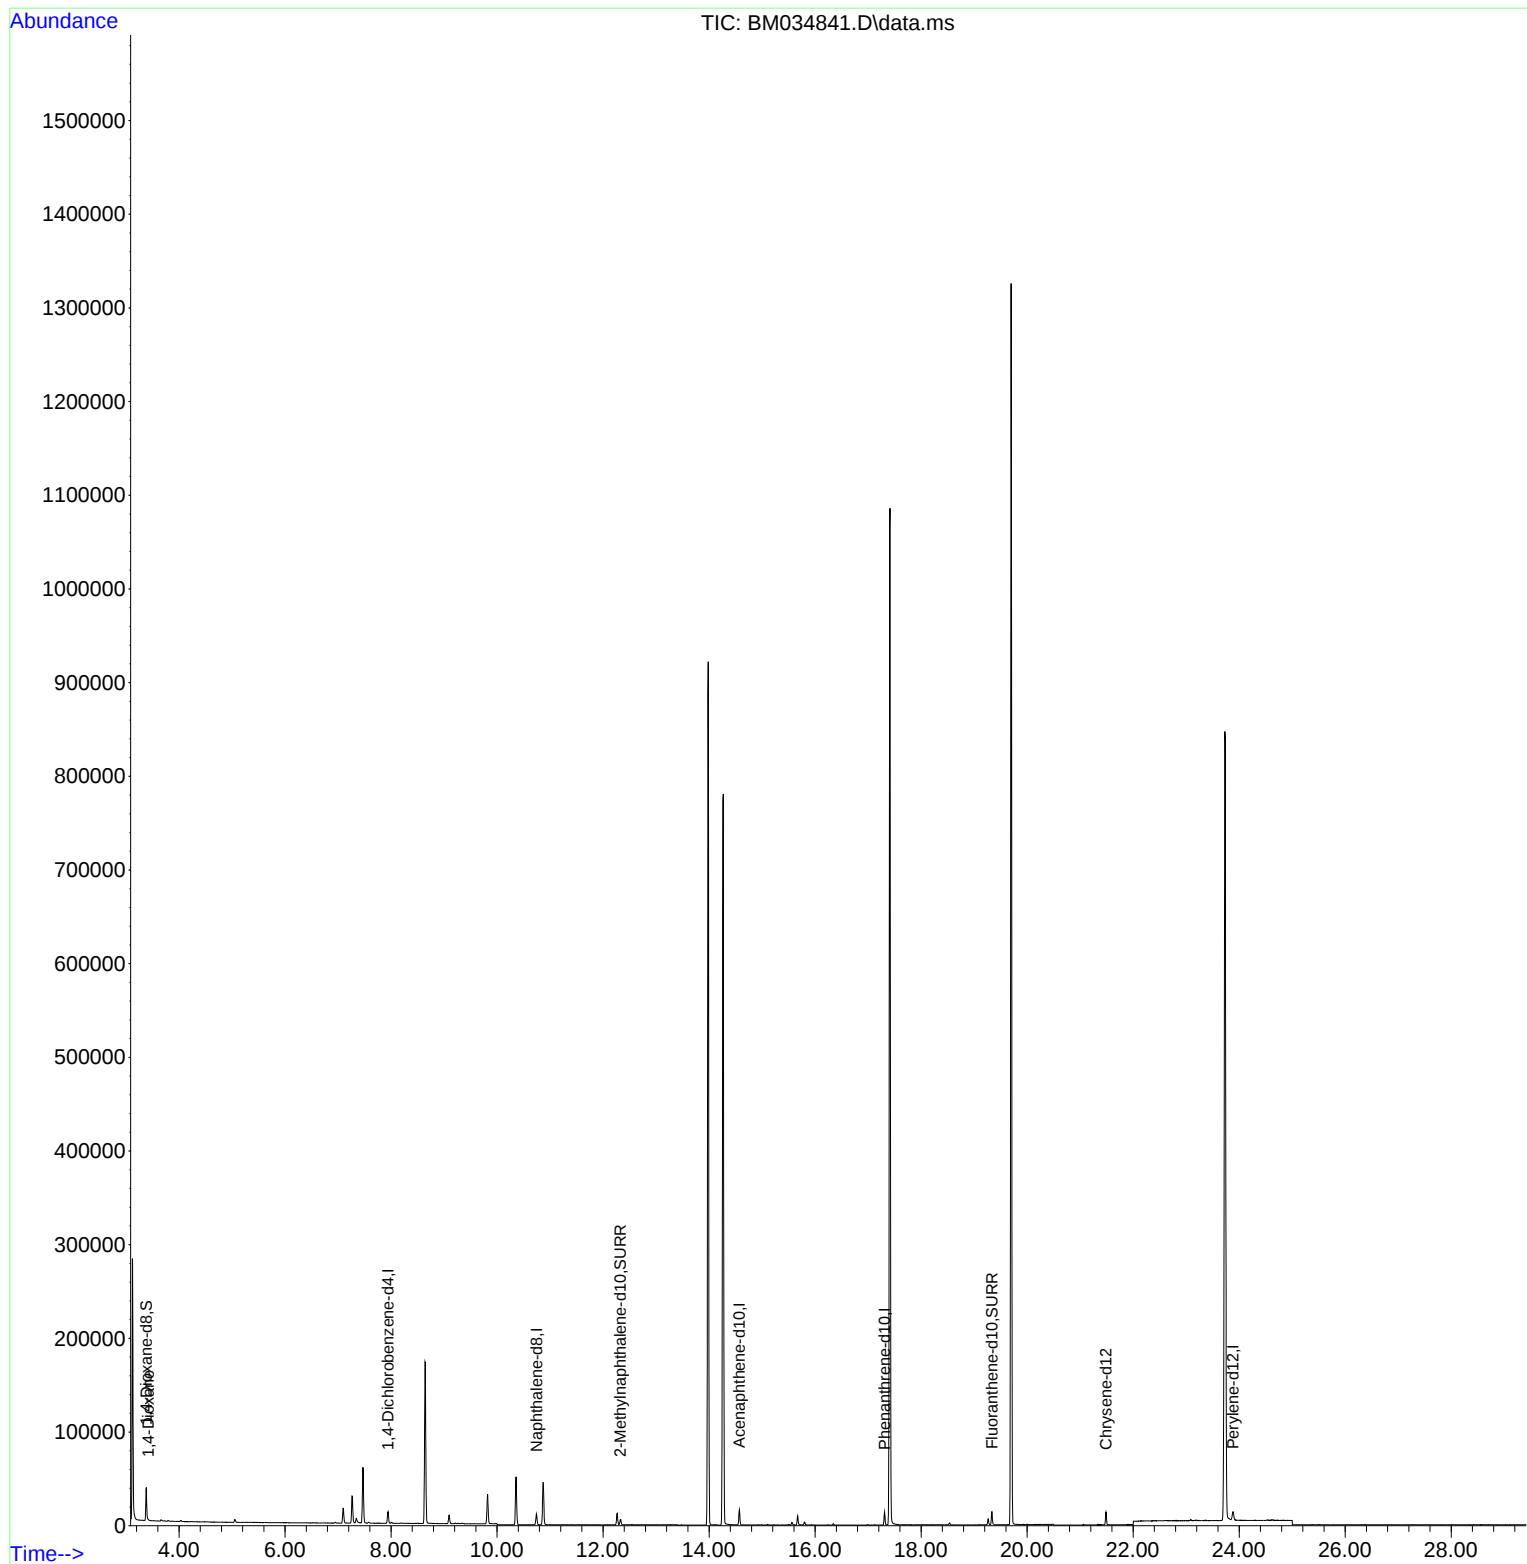


Abundance Scan 80 (3.420 min): BM034832.D\data.ms (-73)

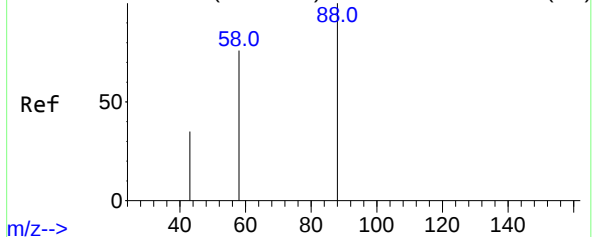


m/z-->

Abundance Scan 80 (3.420 min): BM034841.D\data.ms

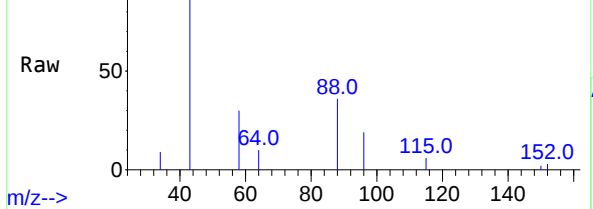

m/z-->

Abundance Scan 80 (3.420 min): BM034841.D\data.ms (-68)

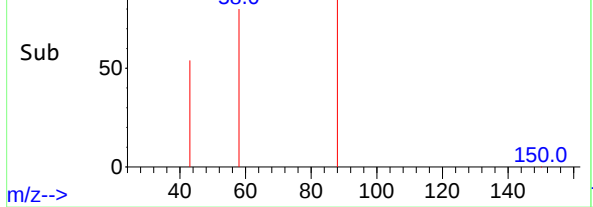

m/z-->

#2
1,4-Dioxane
Concen: 0.070 ng/ul
RT: 3.420 min Scan# 80
Delta R.T. -0.000 min
Lab File: BM034841.D
Acq: 26 Apr 2022 17:52

Instrument :
BNA_M
ClientSampleId :
BFFH1

Tgt Ion: 88 Resp: 433
Ion Ratio Lower Upper
88 100
43 274.6 49.7 74.5#
58 82.6 52.5 78.7#

