

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042622\
 Data File : BM034842.D
 Acq On : 26 Apr 2022 18:28
 Operator : CG/JU
 Sample : N2517-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFFH8

Quant Time: Apr 27 01:28:27 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 22 16:54:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.943	152	5512	0.400	ng/ul	0.00
4) Naphthalene-d8	10.743	136	14379	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.571	164	7918	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.309	188	14291	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.485	240	10258	0.400	ng/ul	# 0.00
23) Perylene-d12	23.879	264	11466	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.382	96	30890	5.067	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.327	152	8239	0.408	ng/ul	0.00
18) Fluoranthene-d10	19.336	212	15836	0.489	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.793	128	1171	0.028	ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042622\
Data File : BM034842.D
Acq On : 26 Apr 2022 18:28
Operator : CG/JU
Sample : N2517-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFFH8


Quant Time: Apr 27 01:28:27 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 22 16:54:34 2022
Response via : Initial Calibration

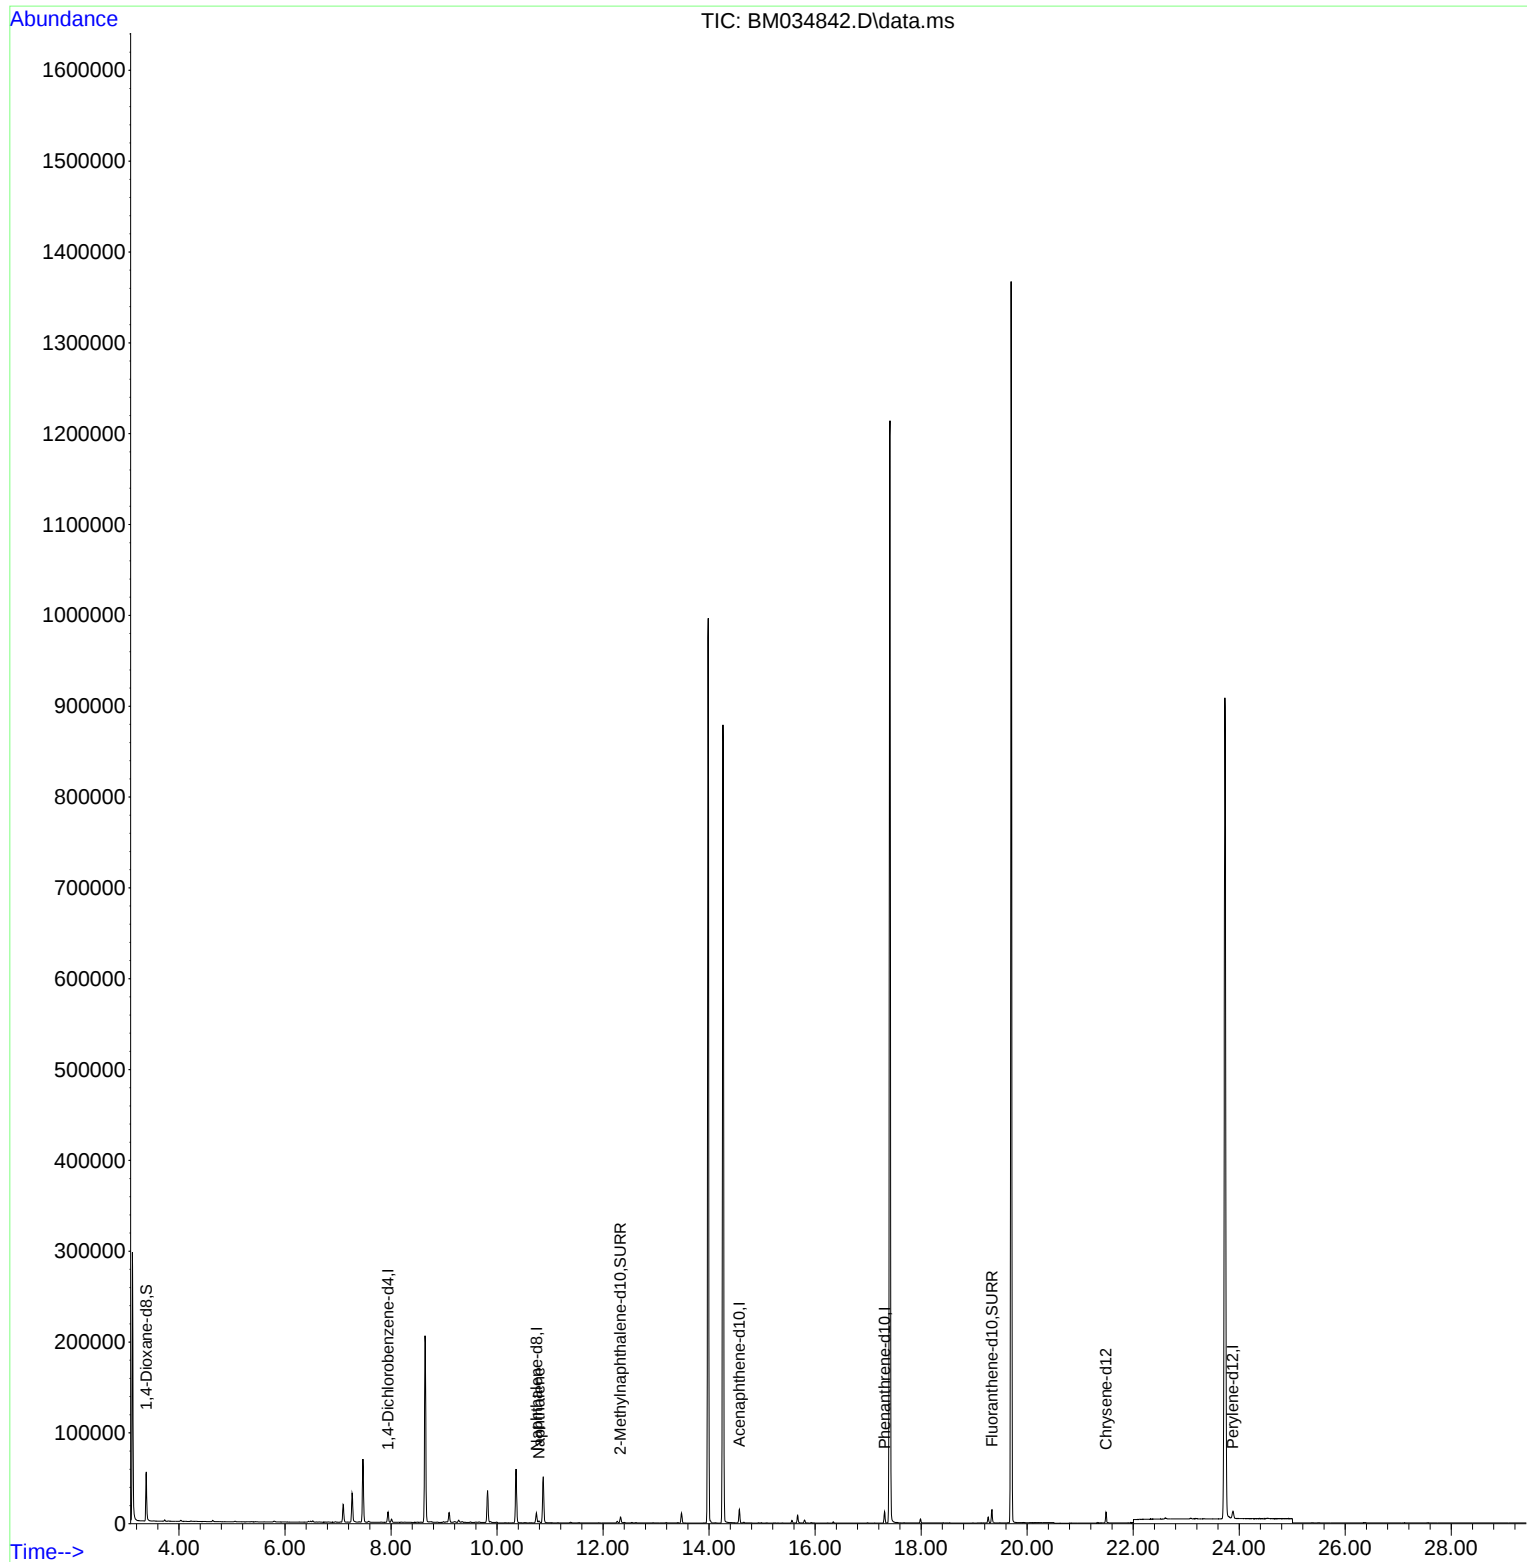

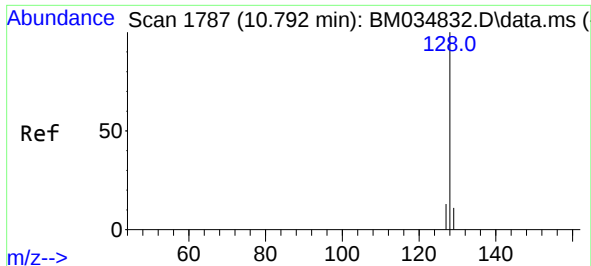

#5
Naphthalene
Concen: 0.028 ng/ul
RT: 10.793 min Scan# 11
Delta R.T. -0.004 min
Lab File: BM034842.D
Acq: 26 Apr 2022 18:28

Instrument :
BNA_M
ClientSampleId :
BFFH8

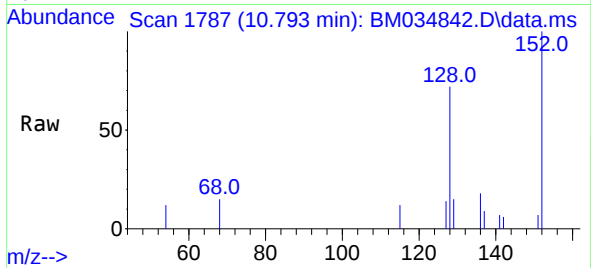

Tgt Ion:128 Resp: 1171
Ion Ratio Lower Upper
128 100
129 20.4 13.4 20.2#
127 20.2 15.2 22.8

