

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042825\
 Data File : BM050026.D
 Acq On : 28 Apr 2025 13:48
 Operator : RC/JU
 Sample : SSTDICC010
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC010

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 04/29/2025
 Supervised By :Jagrut Upadhyay 04/29/2025

Quant Time: Apr 28 17:54:15 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 28 17:38:08 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	250110	20.000	ng	0.00
21) Naphthalene-d8	10.563	136	926512	20.000	ng	0.00
39) Acenaphthene-d10	14.410	164	636652	20.000	ng	0.00
64) Phenanthrene-d10	17.157	188	1274608	20.000	ng	0.00
76) Chrysene-d12	21.397	240	1213581	20.000	ng	0.00
86) Perylene-d12	24.403	264	1224339	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.363	112	269870	18.894	ng	0.00
7) Phenol-d6	6.957	99	329701	18.366	ng	0.00
23) Nitrobenzene-d5	8.928	82	346334	18.420	ng	0.00
42) 2,4,6-Tribromophenol	15.910	330	158339	16.820	ng	0.00
45) 2-Fluorobiphenyl	13.027	172	989917	18.394	ng	0.00
79) Terphenyl-d14	19.780	244	1443528	17.601	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.257	88	58048	9.478	ng	98
3) Pyridine	3.663	79	145801	9.266	ng	98
4) n-Nitrosodimethylamine	3.569	42	57404	9.302	ng	# 93
6) Aniline	7.098	93	211256	9.319	ng	100
8) 2-Chlorophenol	7.339	128	145228	9.404	ng	99
9) Benzaldehyde	6.916	77	115030m	9.587	ng	
10) Phenol	6.981	94	168041	9.246	ng	99
11) bis(2-Chloroethyl)ether	7.192	93	138197	9.107	ng	100
12) 1,3-Dichlorobenzene	7.657	146	178565	9.572	ng	96
13) 1,4-Dichlorobenzene	7.804	146	177312	9.461	ng	99
14) 1,2-Dichlorobenzene	8.122	146	174224	9.624	ng	100
15) Benzyl Alcohol	8.022	79	110234	8.854	ng	98
16) 2,2'-oxybis(1-Chloropr...	8.292	45	177776	9.637	ng	97
17) 2-Methylphenol	8.228	107	111639	9.325	ng	99
18) Hexachloroethane	8.845	117	63487	9.530	ng	98
19) n-Nitroso-di-n-propyla...	8.575	70	110641	9.609	ng	98
20) 3+4-Methylphenols	8.563	107	146303	9.049	ng	99
22) Acetophenone	8.592	105	214790	9.325	ng	98
24) Nitrobenzene	8.969	77	150534	9.259	ng	99
25) Isophorone	9.498	82	300179	9.366	ng	99
26) 2-Nitrophenol	9.686	139	72521	8.732	ng	97
27) 2,4-Dimethylphenol	9.757	122	123406	8.960	ng	97
28) bis(2-Chloroethoxy)met...	9.975	93	184837	9.331	ng	99
29) 2,4-Dichlorophenol	10.245	162	137916	8.938	ng	99
30) 1,2,4-Trichlorobenzene	10.428	180	177721	9.453	ng	97
31) Naphthalene	10.610	128	444206	9.467	ng	99
32) Benzoic acid	9.875	122	63971m	7.282	ng	
33) 4-Chloroaniline	10.739	127	181907	9.458	ng	99
34) Hexachlorobutadiene	10.898	225	111307	9.327	ng	99
35) Caprolactam	11.516	113	39344	8.745	ng	94
36) 4-Chloro-3-methylphenol	11.880	107	131076	9.194	ng	98
37) 2-Methylnaphthalene	12.227	142	296053	9.411	ng	97
38) 1-Methylnaphthalene	12.451	142	312512	9.387	ng	97
40) 1,2,4,5-Tetrachloroben...	12.604	216	197943	8.981	ng	99
41) Hexachlorocyclopentadiene	12.580	237	96522	7.166	ng	99
43) 2,4,6-Trichlorophenol	12.857	196	121240	8.673	ng	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042825\
 Data File : BM050026.D
 Acq On : 28 Apr 2025 13:48
 Operator : RC/JU
 Sample : SSTDICC010
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

SSTDICC010

Manual Integrations**APPROVED**

Reviewed By :Rahul Chavli 04/29/2025

Supervised By :Jagrut Upadhyay 04/29/2025

Quant Time: Apr 28 17:54:15 2025

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Apr 28 17:38:08 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 2,4,5-Trichlorophenol	12.945	196	132882	8.815	ng	96
46) 1,1'-Biphenyl	13.245	154	443960	9.381	ng	99
47) 2-Chloronaphthalene	13.286	162	354101	9.447	ng	99
48) 2-Nitroaniline	13.498	65	77101	8.764	ng	94
49) Acenaphthylene	14.133	152	545774	9.235	ng	100
50) Dimethylphthalate	13.868	163	438261	9.419	ng	99
51) 2,6-Dinitrotoluene	13.992	165	86242	8.953	ng	98
52) Acenaphthene	14.474	154	317735	9.288	ng	98
53) 3-Nitroaniline	14.333	138	78720	8.559	ng	# 99
54) 2,4-Dinitrophenol	14.563	184	31979	10.558	ng	96
55) Dibenzofuran	14.810	168	535023	9.401	ng	99
56) 4-Nitrophenol	14.710	139	40722	9.668	ng	96
57) 2,4-Dinitrotoluene	14.792	165	116476	8.750	ng	95
58) Fluorene	15.462	166	427384	9.174	ng	98
59) 2,3,4,6-Tetrachlorophenol	15.051	232	115185	8.828	ng	98
60) Diethylphthalate	15.233	149	414149	9.447	ng	100
61) 4-Chlorophenyl-phenyle...	15.457	204	227926	8.908	ng	94
62) 4-Nitroaniline	15.498	138	74565m	8.397	ng	
63) Azobenzene	15.745	77	347347	9.454	ng	99
65) 4,6-Dinitro-2-methylph...	15.562	198	56182	7.042	ng	93
66) n-Nitrosodiphenylamine	15.668	169	364601	9.315	ng	99
67) 4-Bromophenyl-phenylether	16.351	248	137532	8.923	ng	99
68) Hexachlorobenzene	16.468	284	160195	9.016	ng	99
69) Atrazine	16.621	200	126168	8.937	ng	98
70) Pentachlorophenol	16.827	266	74839	7.483	ng	95
71) Phenanthrene	17.198	178	659374	9.172	ng	100
72) Anthracene	17.292	178	661260	9.089	ng	99
73) Carbazole	17.568	167	573667	9.087	ng	99
74) Di-n-butylphthalate	18.121	149	689248	9.168	ng	99
75) Fluoranthene	19.221	202	727607	8.621	ng	99
77) Benzidine	19.415	184	339970	7.887	ng	99
78) Pyrene	19.586	202	761625	8.937	ng	99
80) Butylbenzylphthalate	20.474	149	290617	9.105	ng	93
81) Benzo(a)anthracene	21.380	228	747128	8.940	ng	100
82) 3,3'-Dichlorobenzidine	21.309	252	262017	8.190	ng	100
83) Chrysene	21.444	228	709862	9.178	ng	99
84) Bis(2-ethylhexyl)phtha...	21.297	149	439949	9.228	ng	98
85) Di-n-octyl phthalate	22.427	149	726208	9.236	ng	99
87) Indeno(1,2,3-cd)pyrene	27.791	276	791344	8.674	ng	99
88) Benzo(b)fluoranthene	23.450	252	703118	8.831	ng	98
89) Benzo(k)fluoranthene	23.515	252	704142	8.741	ng	99
90) Benzo(a)pyrene	24.262	252	652617	8.751	ng	99
91) Dibenzo(a,h)anthracene	27.844	278	638913	8.591	ng	98
92) Benzo(g,h,i)perylene	28.850	276	630261	8.852	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042825\
 Data File : BM050026.D
 Acq On : 28 Apr 2025 13:48
 Operator : RC/JU
 Sample : SSTDICC010
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

SSTDICC010

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 04/29/2025

Supervised By :Jagrut Upadhyay 04/29/2025


Quant Time: Apr 28 17:54:15 2025

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Apr 28 17:38:08 2025

Response via : Initial Calibration

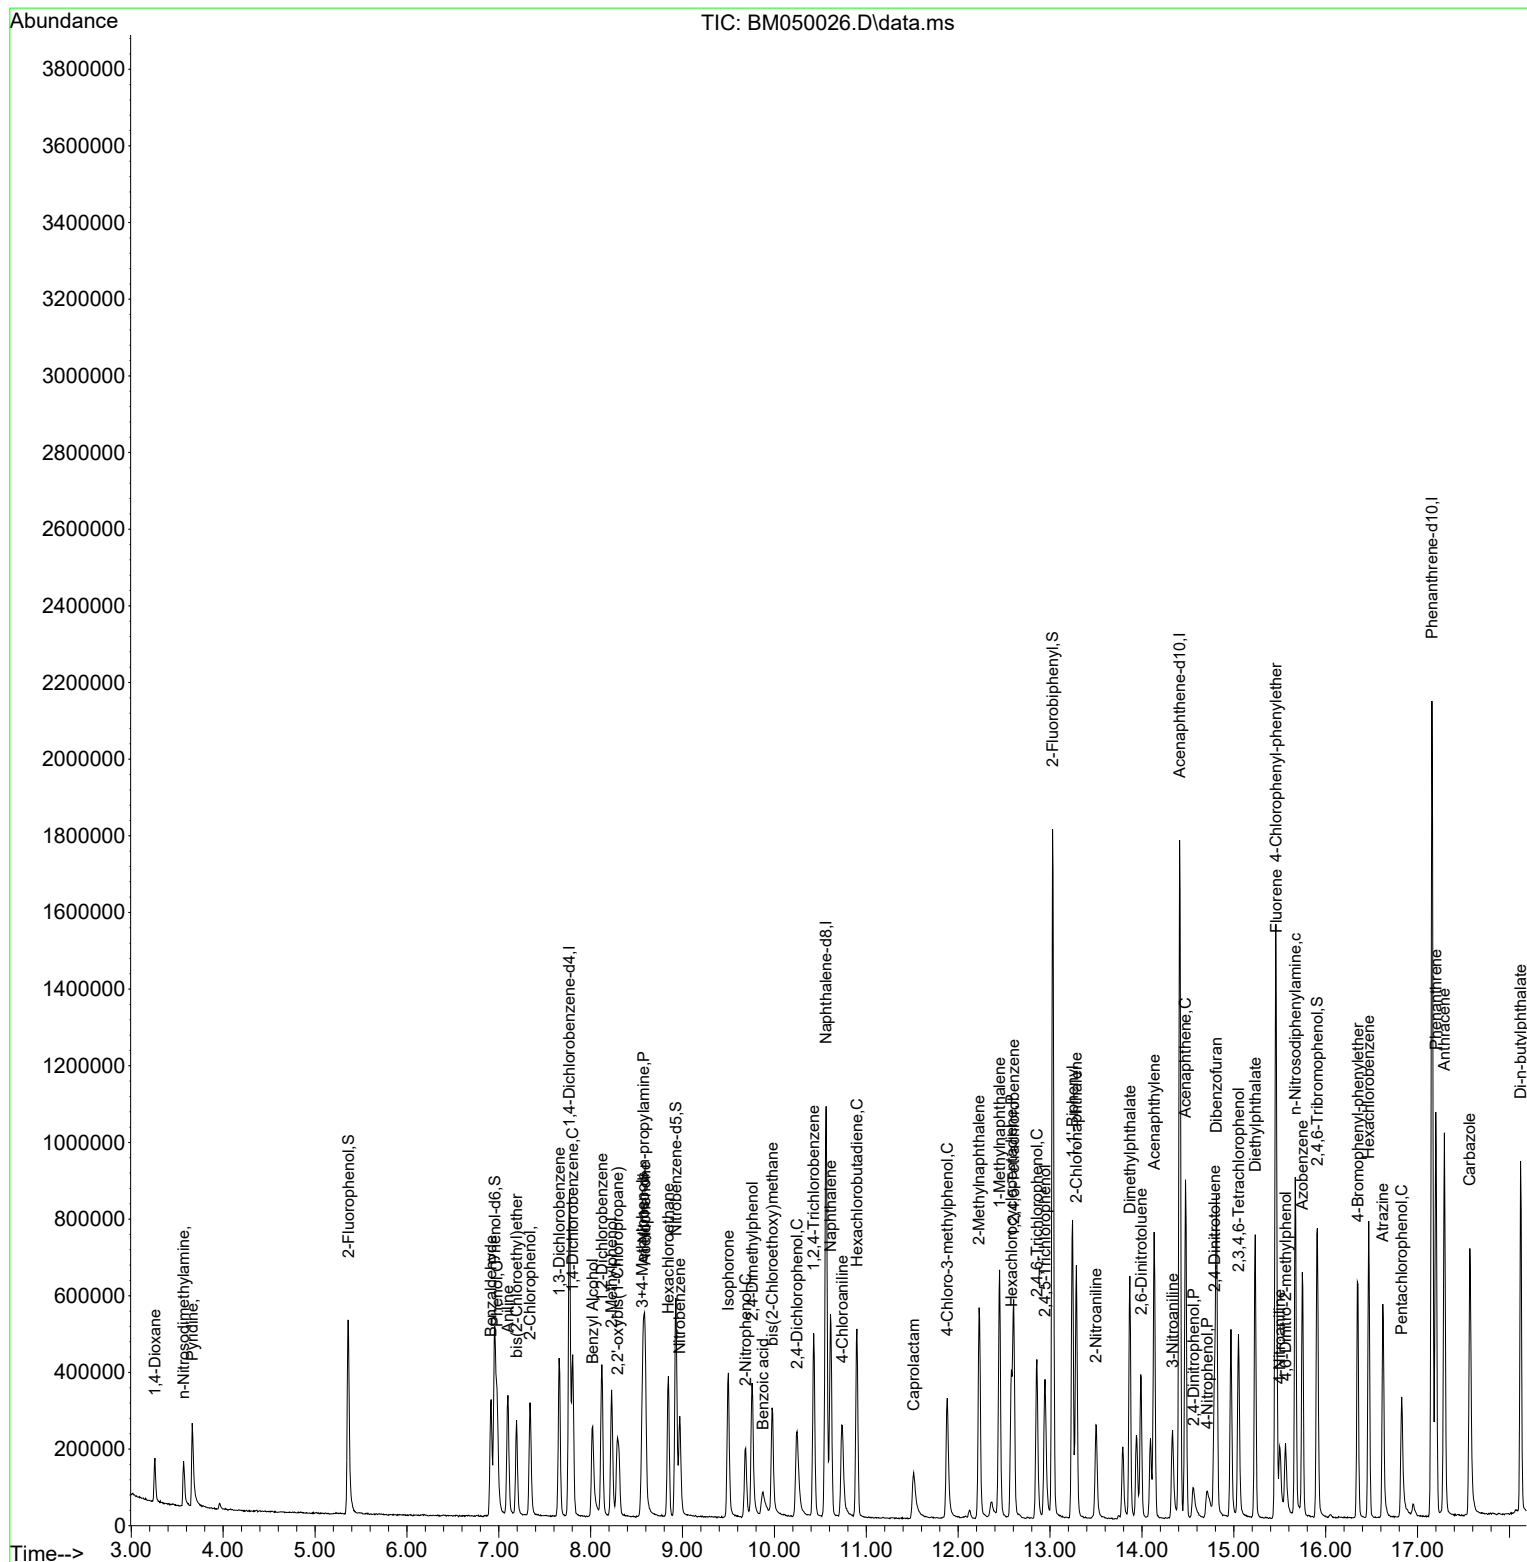

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042825\
Data File : BM050026.D
Acq On : 28 Apr 2025 13:48
Operator : RC/JU
Sample : SSTDICC010
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDICC010

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 04/29/2025
Supervised By :Jagrut Upadhyay 04/29/2025

Quant Time: Apr 28 17:54:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 17:38:08 2025
Response via : Initial Calibration

