

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042825\
 Data File : BM050027.D
 Acq On : 28 Apr 2025 14:27
 Operator : RC/JU
 Sample : SSTDICC020
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

SSTDICC020

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 04/29/2025

Supervised By :Jagrut Upadhyay 04/29/2025

Quant Time: Apr 28 17:55:16 2025

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Apr 28 17:38:08 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	242715	20.000	ng	0.00
21) Naphthalene-d8	10.563	136	896366	20.000	ng	0.00
39) Acenaphthene-d10	14.410	164	614688	20.000	ng	0.00
64) Phenanthrene-d10	17.157	188	1244440	20.000	ng	0.00
76) Chrysene-d12	21.398	240	1204355	20.000	ng	0.00
86) Perylene-d12	24.403	264	1191041	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.357	112	537488	38.777	ng	0.00
7) Phenol-d6	6.951	99	678404	38.941	ng	0.00
23) Nitrobenzene-d5	8.928	82	712171	39.151	ng	0.00
42) 2,4,6-Tribromophenol	15.904	330	345020	37.960	ng	0.00
45) 2-Fluorobiphenyl	13.027	172	2005788	38.602	ng	0.00
79) Terphenyl-d14	19.780	244	3208242	39.418	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.258	88	115944	19.509	ng	99
3) Pyridine	3.658	79	298256	19.532	ng	98
4) n-Nitrosodimethylamine	3.569	42	115296	19.251	ng	# 100
6) Aniline	7.098	93	429222	19.511	ng	99
8) 2-Chlorophenol	7.340	128	290876	19.409	ng	99
9) Benzaldehyde	6.910	77	235594	20.233	ng	98
10) Phenol	6.981	94	344567	19.537	ng	98
11) bis(2-Chloroethyl)ether	7.193	93	285330	19.375	ng	99
12) 1,3-Dichlorobenzene	7.657	146	352660	19.480	ng	99
13) 1,4-Dichlorobenzene	7.804	146	354975	19.518	ng	99
14) 1,2-Dichlorobenzene	8.122	146	345385	19.660	ng	99
15) Benzyl Alcohol	8.016	79	234541	19.413	ng	98
16) 2,2'-oxybis(1-Chloropr...	8.293	45	350829	19.598	ng	98
17) 2-Methylphenol	8.228	107	225978	19.450	ng	99
18) Hexachloroethane	8.845	117	126530	19.571	ng	99
19) n-Nitroso-di-n-propyla...	8.575	70	223538	20.006	ng	99
20) 3+4-Methylphenols	8.557	107	307585	19.604	ng	97
22) Acetophenone	8.592	105	434539	19.499	ng	98
24) Nitrobenzene	8.969	77	309341	19.667	ng	99
25) Isophorone	9.498	82	609252	19.648	ng	99
26) 2-Nitrophenol	9.681	139	154364	19.211	ng	97
27) 2,4-Dimethylphenol	9.751	122	259319	19.460	ng	99
28) bis(2-Chloroethoxy)met...	9.975	93	378162	19.732	ng	100
29) 2,4-Dichlorophenol	10.234	162	292336	19.582	ng	99
30) 1,2,4-Trichlorobenzene	10.428	180	352792	19.397	ng	98
31) Naphthalene	10.610	128	890530	19.618	ng	99
32) Benzoic acid	9.881	122	154412m	18.168	ng	
33) 4-Chloroaniline	10.734	127	362366	19.475	ng	99
34) Hexachlorobutadiene	10.898	225	223143	19.327	ng	99
35) Caprolactam	11.516	113	84917	19.509	ng	93
36) 4-Chloro-3-methylphenol	11.875	107	270510	19.613	ng	99
37) 2-Methylnaphthalene	12.228	142	593403	19.498	ng	99
38) 1-Methylnaphthalene	12.445	142	634293	19.694	ng	99
40) 1,2,4,5-Tetrachloroben...	12.604	216	402355	18.909	ng	99
41) Hexachlorocyclopentadiene	12.575	237	222254	17.091	ng	100
43) 2,4,6-Trichlorophenol	12.851	196	260161	19.276	ng	96

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042825\
 Data File : BM050027.D
 Acq On : 28 Apr 2025 14:27
 Operator : RC/JU
 Sample : SSTDICC020
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC020

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 04/29/2025
 Supervised By :Jagrut Upadhyay 04/29/2025

Quant Time: Apr 28 17:55:16 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 28 17:38:08 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 2,4,5-Trichlorophenol	12.939	196	278307	19.123	ng	98
46) 1,1'-Biphenyl	13.239	154	892394	19.530	ng	99
47) 2-Chloronaphthalene	13.286	162	709815	19.614	ng	100
48) 2-Nitroaniline	13.498	65	165324	19.465	ng	99
49) Acenaphthylene	14.133	152	1112766	19.502	ng	99
50) Dimethylphthalate	13.869	163	883120	19.659	ng	99
51) 2,6-Dinitrotoluene	13.986	165	183493	19.729	ng	99
52) Acenaphthene	14.474	154	643177	19.474	ng	99
53) 3-Nitroaniline	14.327	138	174626	19.666	ng	97
54) 2,4-Dinitrophenol	14.551	184	80991	18.373	ng	99
55) Dibenzofuran	14.810	168	1074975	19.562	ng	99
56) 4-Nitrophenol	14.686	139	110948	19.021	ng	96
57) 2,4-Dinitrotoluene	14.786	165	252994	19.685	ng	100
58) Fluorene	15.457	166	879470	19.553	ng	99
59) 2,3,4,6-Tetrachlorophenol	15.051	232	244928	19.442	ng	99
60) Diethylphthalate	15.233	149	848021	20.034	ng	99
61) 4-Chlorophenyl-phenyle...	15.451	204	473276	19.157	ng	95
62) 4-Nitroaniline	15.492	138	170438	19.880	ng	95
63) Azobenzene	15.745	77	707026	19.930	ng	99
65) 4,6-Dinitro-2-methylph...	15.557	198	136910	17.576	ng	94
66) n-Nitrosodiphenylamine	15.669	169	741920	19.415	ng	99
67) 4-Bromophenyl-phenylether	16.345	248	285352	18.962	ng	98
68) Hexachlorobenzene	16.468	284	327912	18.903	ng	98
69) Atrazine	16.621	200	266068	19.303	ng	98
70) Pentachlorophenol	16.821	266	175794	18.004	ng	99
71) Phenanthrene	17.198	178	1348190	19.208	ng	100
72) Anthracene	17.292	178	1364462	19.210	ng	100
73) Carbazole	17.568	167	1194316	19.377	ng	99
74) Di-n-butylphthalate	18.121	149	1432688	19.519	ng	99
75) Fluoranthene	19.221	202	1555160	18.872	ng	99
77) Benzidine	19.409	184	777502	18.175	ng	99
78) Pyrene	19.580	202	1603874	18.964	ng	100
80) Butylbenzylphthalate	20.474	149	620751	19.597	ng	94
81) Benzo(a)anthracene	21.380	228	1591290	19.187	ng	100
82) 3,3'-Dichlorobenzidine	21.303	252	582038	18.333	ng	99
83) Chrysene	21.445	228	1461777	19.044	ng	99
84) Bis(2-ethylhexyl)phtha...	21.298	149	933505	19.730	ng	98
85) Di-n-octyl phthalate	22.427	149	1525599	19.552	ng	100
87) Indeno(1,2,3-cd)pyrene	27.791	276	1671967	18.840	ng	99
88) Benzo(b)fluoranthene	23.450	252	1439776	18.588	ng	99
89) Benzo(k)fluoranthene	23.515	252	1489410	19.005	ng	100
90) Benzo(a)pyrene	24.262	252	1365706	18.825	ng	99
91) Dibenzo(a,h)anthracene	27.838	278	1360269	18.803	ng	99
92) Benzo(g,h,i)perylene	28.850	276	1316513	19.008	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042825\
 Data File : BM050027.D
 Acq On : 28 Apr 2025 14:27
 Operator : RC/JU
 Sample : SSTDICC020
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

SSTDICC020


Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 04/29/2025

Supervised By :Jagrut Upadhyay 04/29/2025

Quant Time: Apr 28 17:55:16 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 28 17:38:08 2025
 Response via : Initial Calibration

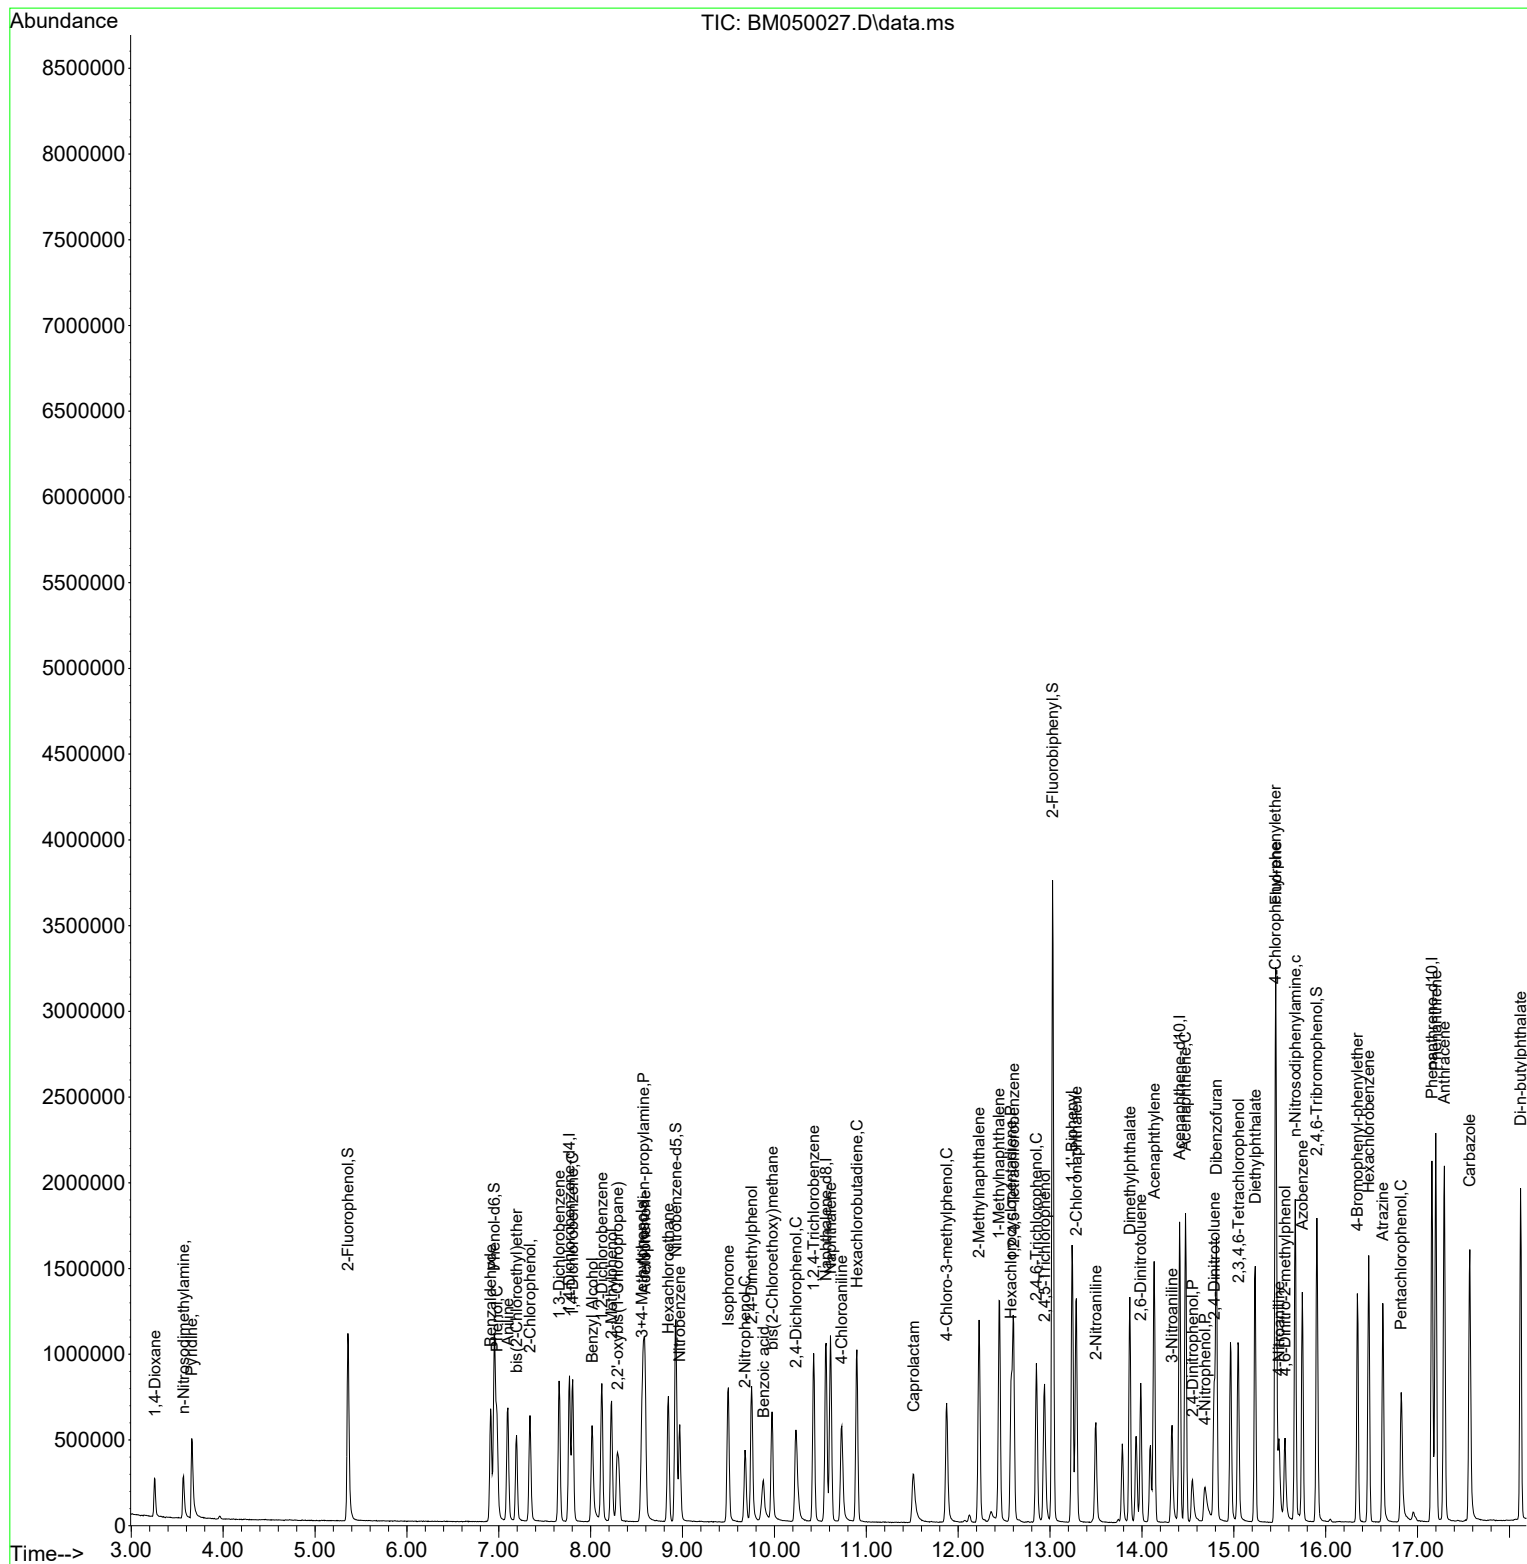

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042825\
Data File : BM050027.D
Acq On : 28 Apr 2025 14:27
Operator : RC/JU
Sample : SSTDICC020
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDICC020

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 04/29/2025
Supervised By :Jagrut Upadhyay 04/29/2025

Quant Time: Apr 28 17:55:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 17:38:08 2025
Response via : Initial Calibration

